

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112918\
 Data File : VU028399.D
 Acq On : 29 Nov 2018 17:20
 Operator : MD/SY
 Sample : J6134-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 MW-6

Quant Time: Dec 05 04:18:59 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U112818W.M
 Quant Title : SW846 8260
 QLast Update : Thu Nov 29 01:04:49 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.98	168	255019	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.89	114	490163	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.09	117	469736	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.48	152	225994	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.31	65	225472	52.90	ug/l	0.00
Spiked Amount 50.000			Recovery	=	105.80%	
35) Dibromofluoromethane	4.88	113	164568	50.49	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.98%	
50) Toluene-d8	7.57	98	646453	49.59	ug/l	0.00
Spiked Amount 50.000			Recovery	=	99.18%	
62) 4-Bromofluorobenzene	10.31	95	241648	51.43	ug/l	0.00
Spiked Amount 50.000			Recovery	=	102.86%	
Target Compounds						
11) Tert butyl alcohol	2.82	59	185450	191.531	ug/l	99
16) Acetone	2.32	43	4507	1.729	ug/l	90
19) Methyl tert-butyl Ether	3.00	73	18842	1.687	ug/l	95
20) Methylene Chloride	2.70	84	4738	1.216	ug/l	91
52) Toluene	7.63	92	5218	0.570	ug/l	98
84) 1,2,4-Trimethylbenzene	11.15	105	6967	0.464	ug/l	98
95) Naphthalene	13.75	128	10515	3.357	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112918\
Data File : VU028399.D
Acq On : 29 Nov 2018 17:20
Operator : MD/SY
Sample : J6134-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
MW-6

Quant Time: Dec 05 04:18:59 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U112818W.M
Quant Title : SW846 8260
QLast Update : Thu Nov 29 01:04:49 2018
Response via : Initial Calibration

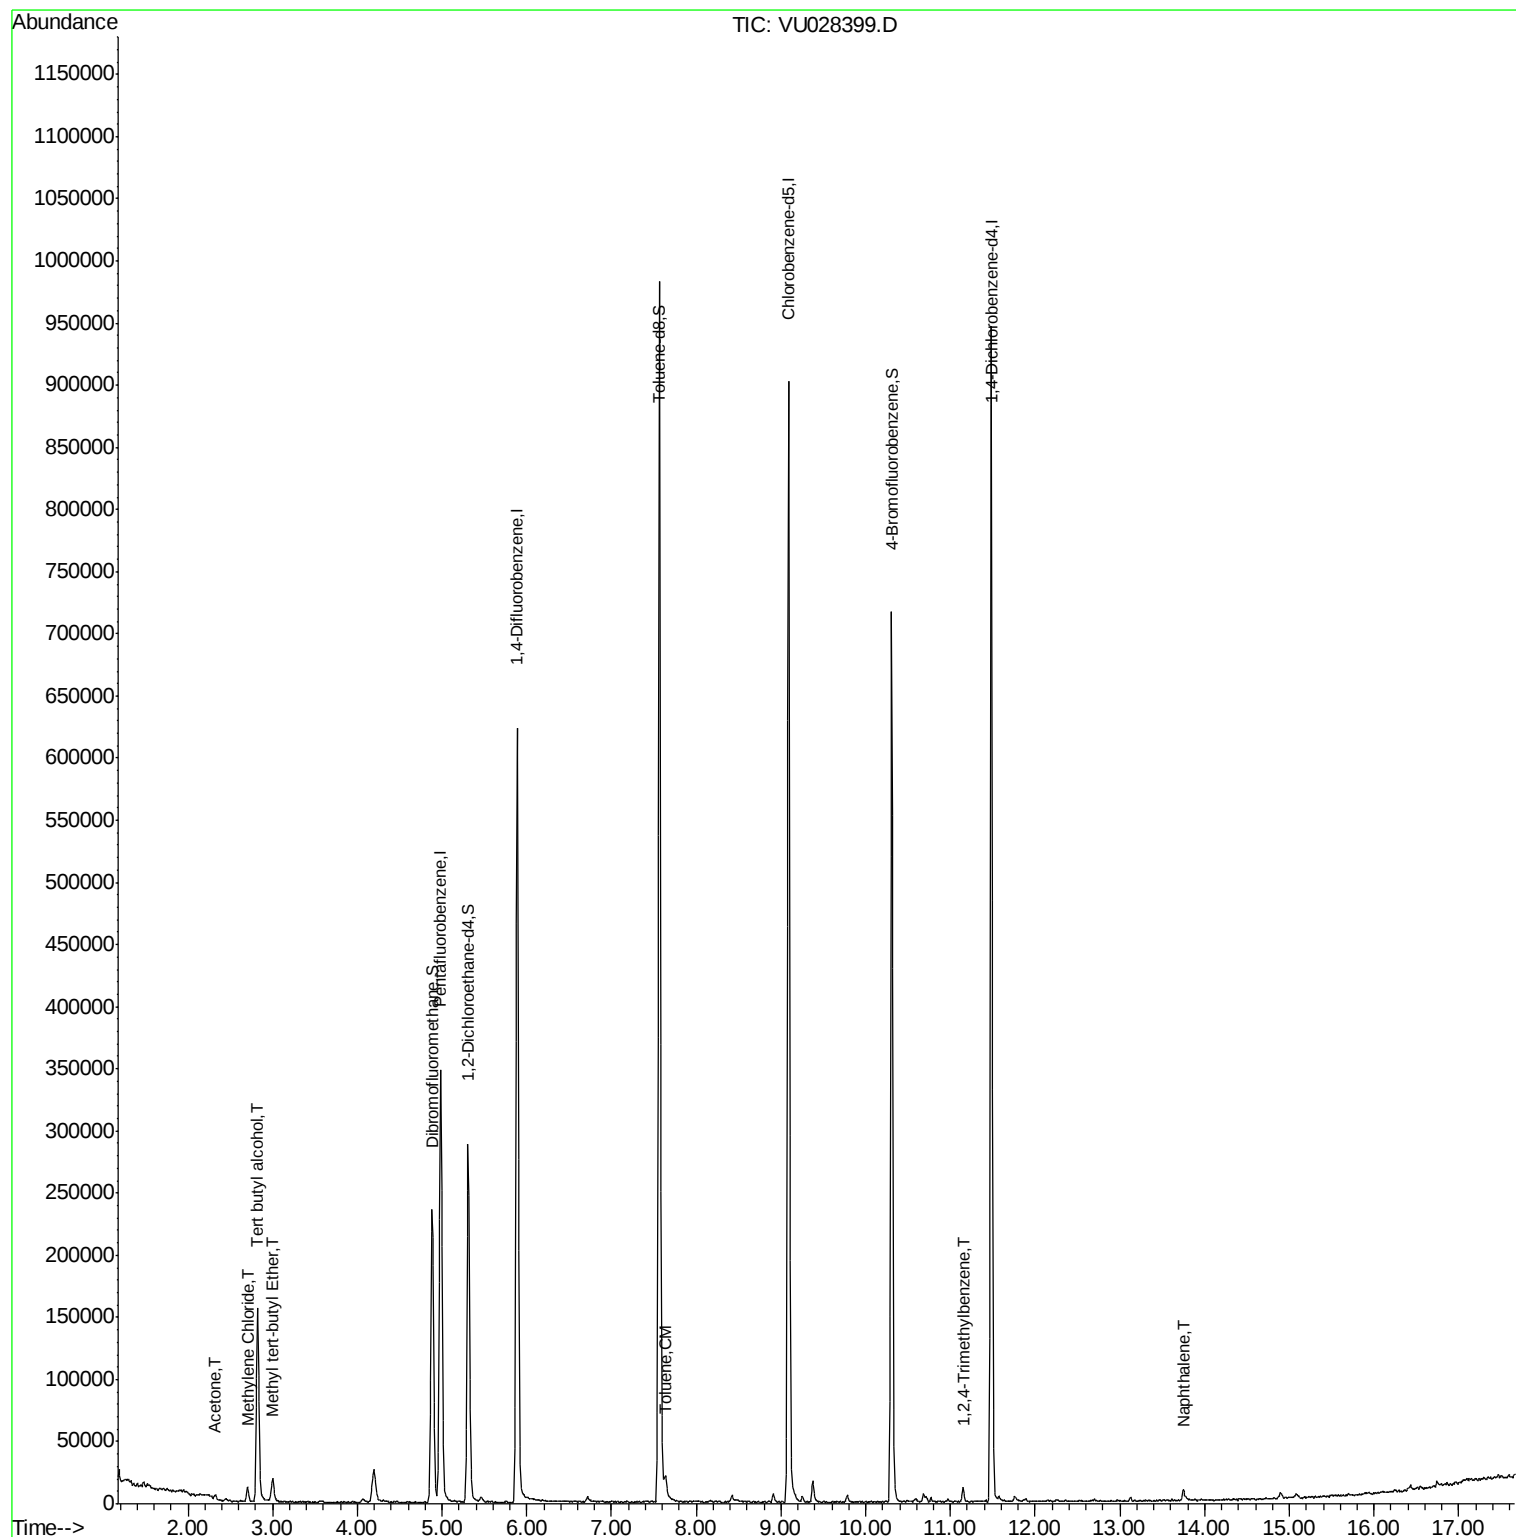

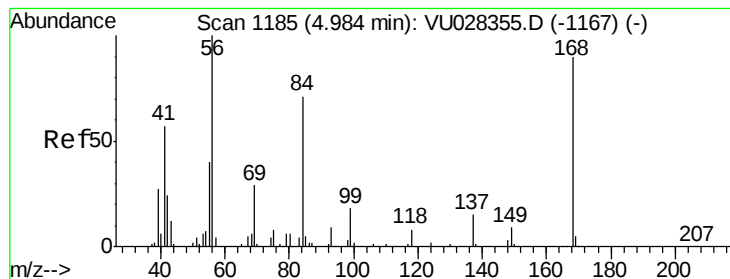

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.98 min Scan# 1185

Delta R.T. -0.00 min

Lab File: VU028399.D

Acq: 29 Nov 2018 17:20

Instrument :

MSVOA_U

ClientSampleId :


MW-6

Tgt Ion:168 Resp: 255019

Ion Ratio Lower Upper

168 100

99 62.3 49.6 74.4

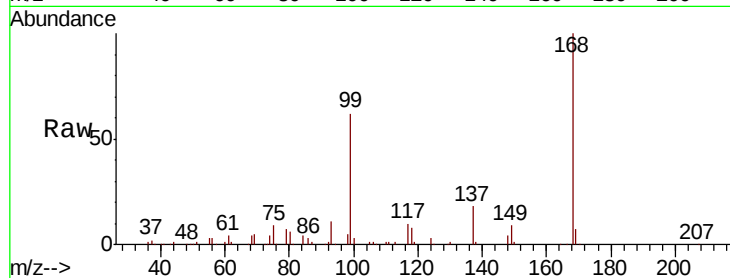

Abundance Ion 167.90 (167.60 to 168.60): VU028355.D (-1167) (-)

Ion 98.90 (98.60 to 99.60): VU028399.D (-1092) (-)

4.98

120000

100000

80000

60000



40000

20000

0

4.90 4.95 5.00 5.05 5.10

Time-->

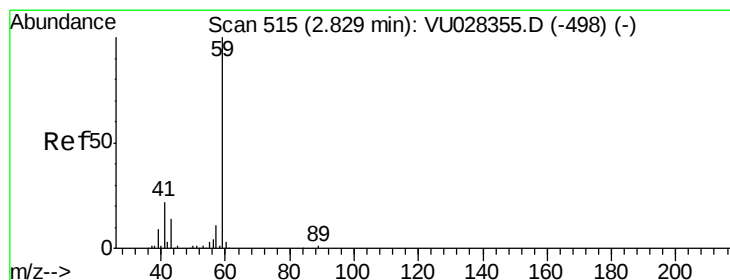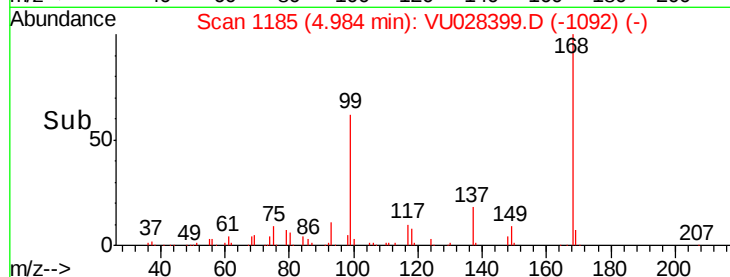

#11

Tert butyl alcohol

Concen: 191.531 ug/l

RT: 2.82 min Scan# 513

Delta R.T. -0.01 min

Lab File: VU028399.D


Acq: 29 Nov 2018 17:20

Tgt Ion: 59 Resp: 185450

Ion Ratio Lower Upper

59 100

57 10.1 8.3 12.5

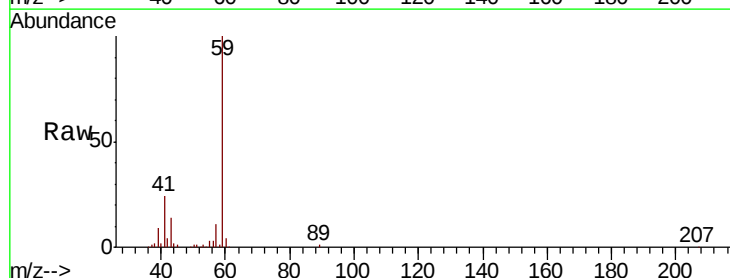

Abundance Ion 59.00 (58.70 to 59.70): VU028355.D (-498) (-)

Ion 57.00 (56.70 to 57.70): VU028399.D (-422) (-)

2.82

100000

80000

60000


40000


20000

0

2.80 2.90

Time-->

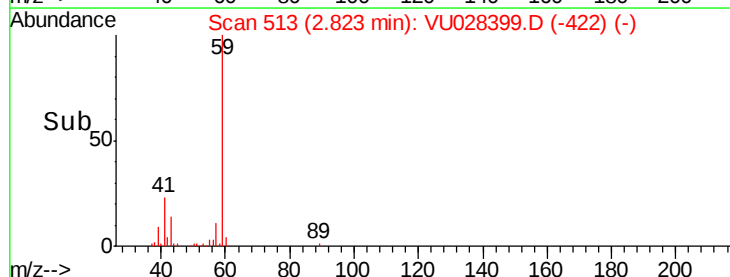

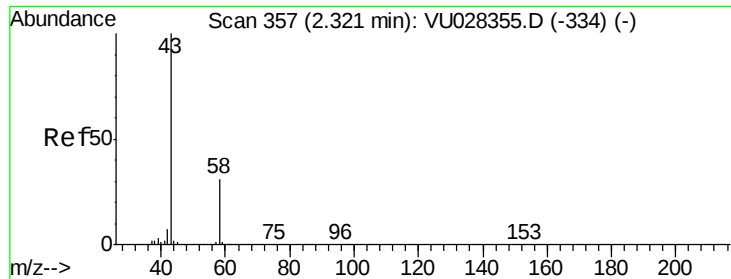

#16

Acetone

Concen: 1.729 ug/l

RT: 2.32 min Scan# 358

Delta R.T. 0.00 min

Lab File: VU028399.D

Acq: 29 Nov 2018 17:20

Instrument :

MSVOA_U

ClientSampleId :


MW-6

Tgt Ion: 43 Resp: 4507

Ion Ratio Lower Upper




43 100

58 25.0 24.4 36.6

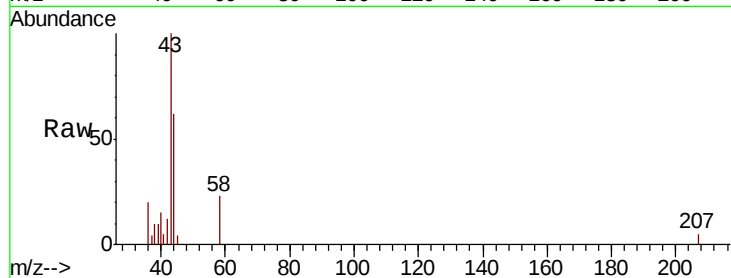

Abundance Ion 43.00 (42.70 to 43.70): VU0

Ion 58.00 (57.70 to 58.70): VU0

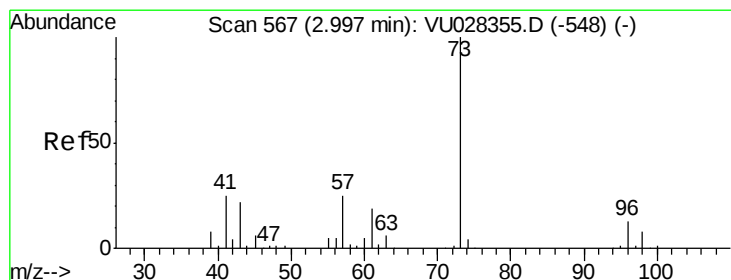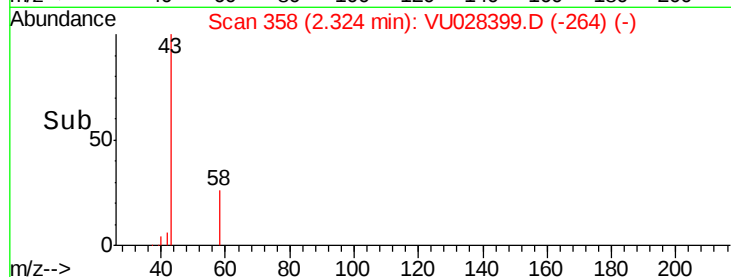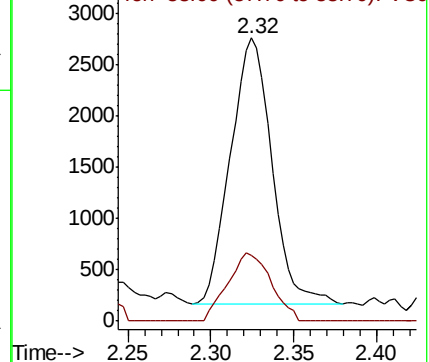

#19

Methyl tert-butyl Ether

Concen: 1.687 ug/l

RT: 3.00 min Scan# 569

Delta R.T. 0.01 min

Lab File: VU028399.D


Acq: 29 Nov 2018 17:20

Tgt Ion: 73 Resp: 18842

Ion Ratio Lower Upper



73 100


57 27.4 20.1 30.1

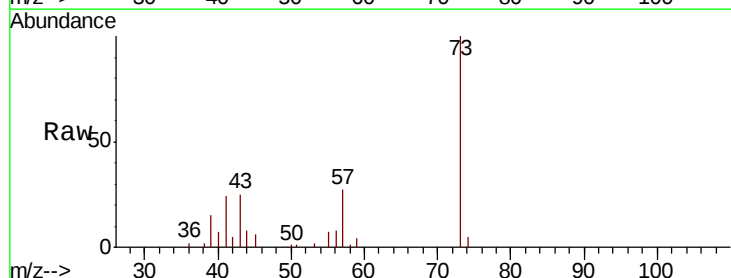

Abundance Ion 73.00 (72.70 to 73.70): VU0

Ion 57.00 (56.70 to 57.70): VU0

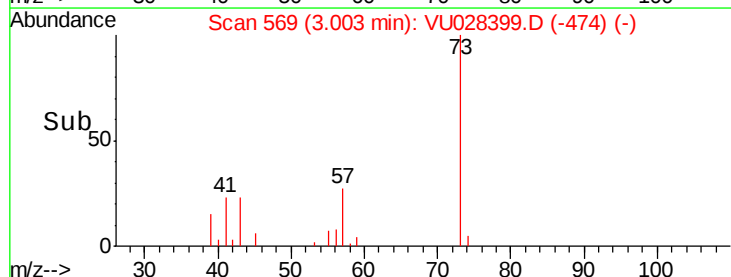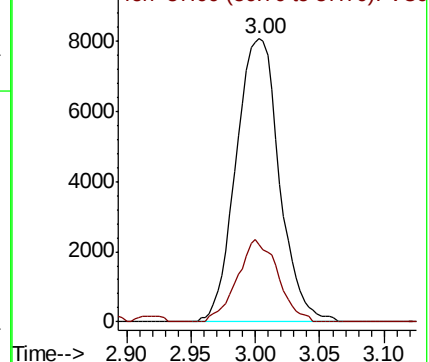


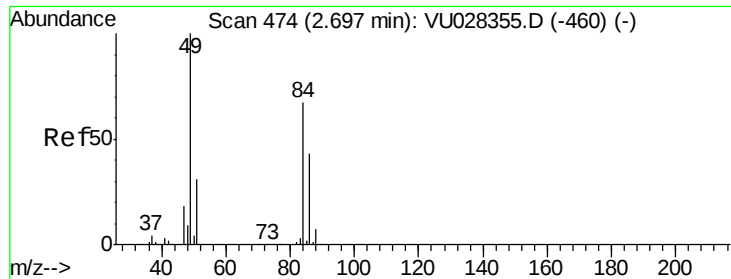




#20
Methylene Chloride
Concen: 1.216 ug/l
RT: 2.70 min Scan# 476
Delta R.T. 0.01 min
Lab File: VU028399.D
Acq: 29 Nov 2018 17:20

Instrument :
MSVOA_U
ClientSampleId :
MW-6

Tgt Ion: 84 Resp: 4738
Ion Ratio Lower Upper
84 100
49 133.1 120.0 180.0
51 45.7 36.9 55.3
86 61.0 51.1 76.7

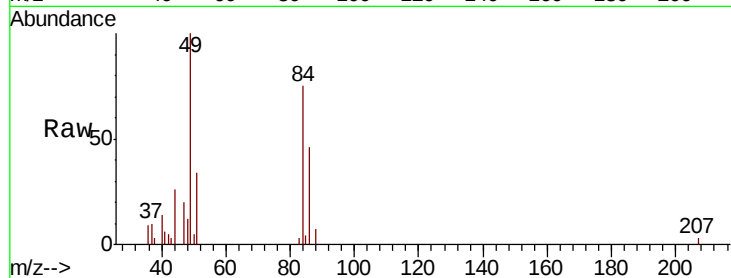


Abundance Ion 83.90 (83.60 to 84.60): VU0
Ion 48.90 (48.60 to 49.60): VU0
Ion 50.90 (50.60 to 51.60): VU0
Ion 85.90 (85.60 to 86.60): VU0

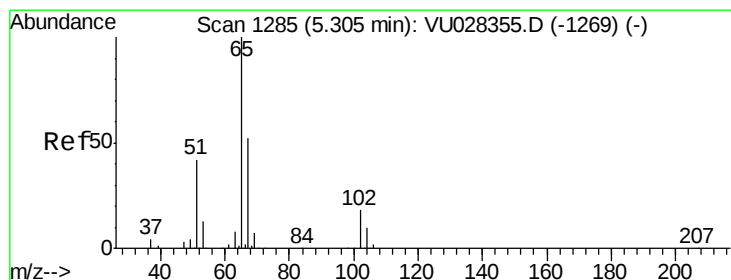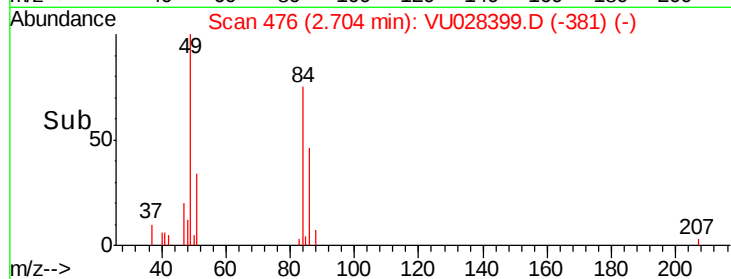
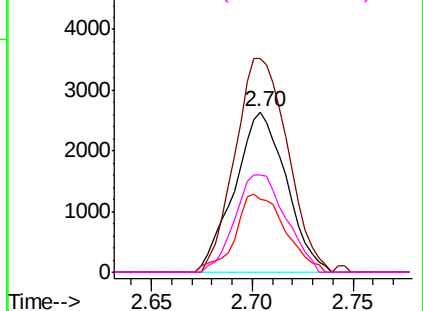



#33
1,2-Dichloroethane-d4
Concen: 52.903 ug/l
RT: 5.31 min Scan# 1286
Delta R.T. 0.00 min
Lab File: VU028399.D
Acq: 29 Nov 2018 17:20

Tgt Ion: 65 Resp: 225472
Ion Ratio Lower Upper
65 100
67 53.9 0.0 106.8

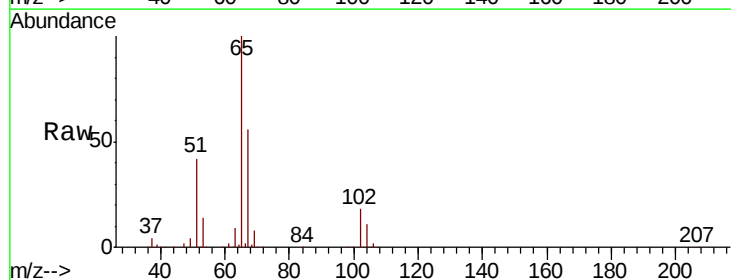

Abundance Ion 64.90 (64.60 to 65.60): VU0
Ion 66.90 (66.60 to 67.60): VU0



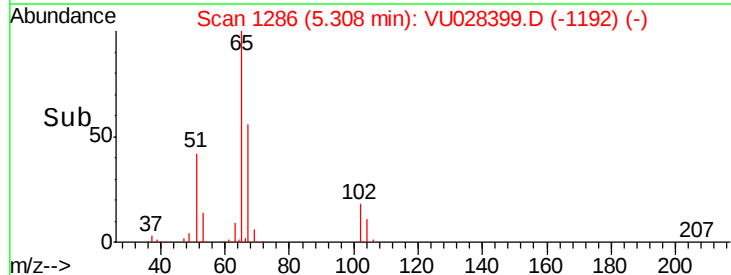
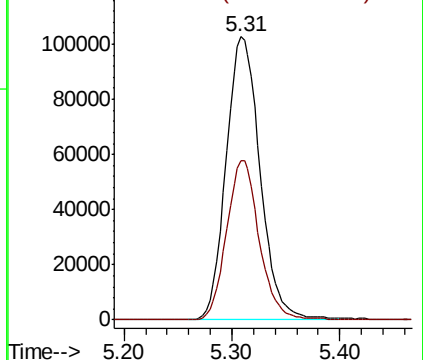


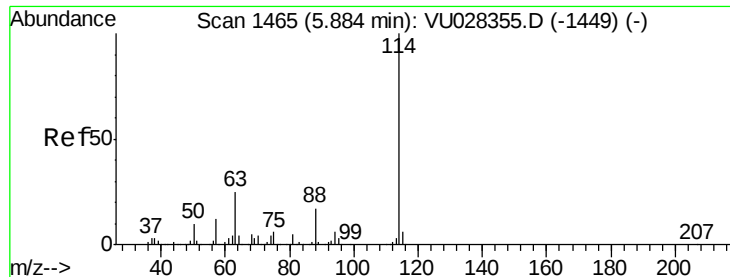

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 5.89 min Scan# 1466
 Delta R.T. 0.00 min
 Lab File: VU028399.D
 Acq: 29 Nov 2018 17:20




Instrument :
 MSVOA_U
 ClientSampleId :
 MW-6


Tgt Ion:114 Resp: 490163
 Ion Ratio Lower Upper
 114 100
 63 25.0 0.0 50.0
 88 17.3 0.0 34.4

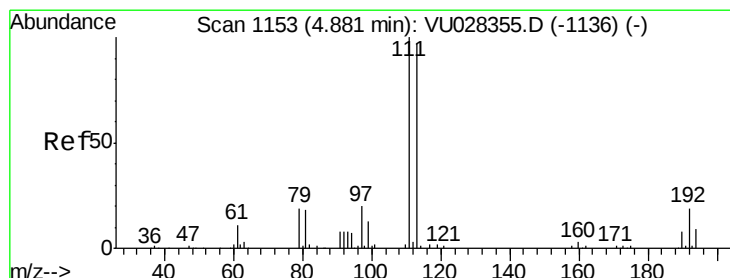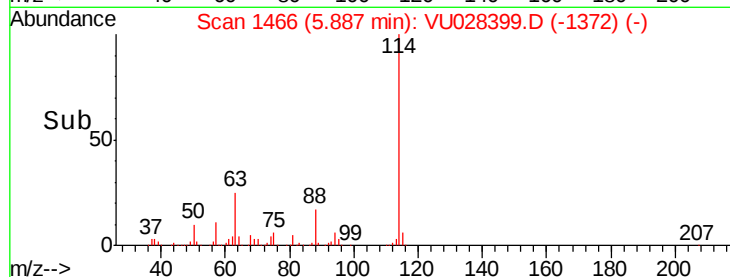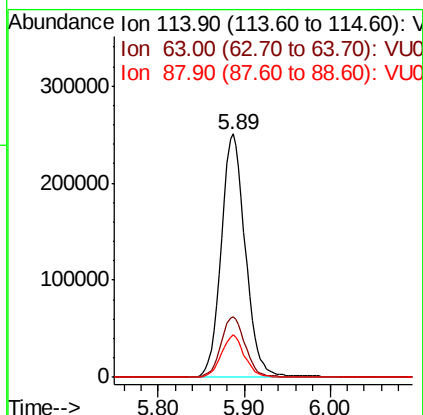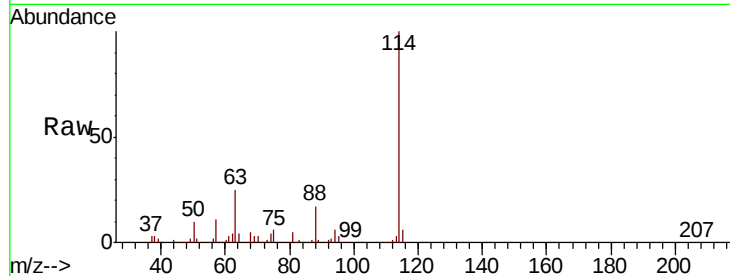

#35
 Dibromofluoromethane
 Concen: 50.490 ug/l
 RT: 4.88 min Scan# 1154
 Delta R.T. 0.00 min
 Lab File: VU028399.D
 Acq: 29 Nov 2018 17:20

Tgt Ion:113 Resp: 164568
 Ion Ratio Lower Upper
 113 100
 111 102.8 82.9 124.3
 192 18.0 15.4 23.0


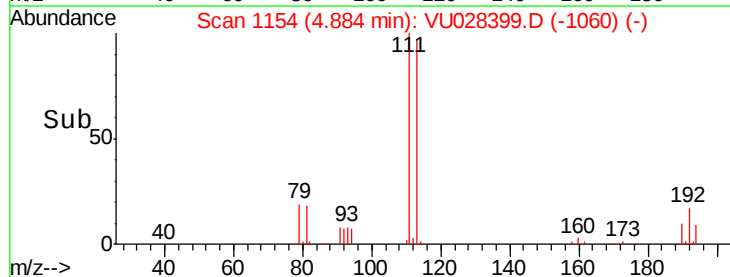
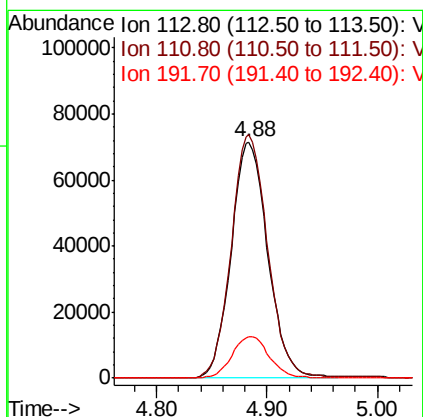
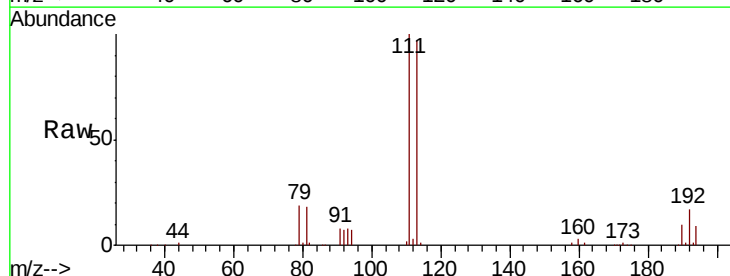


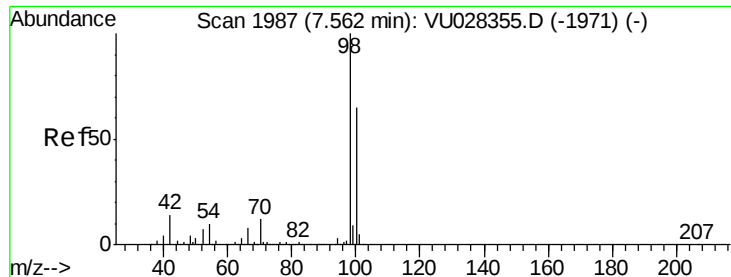

#50
Toluene-d8
Concen: 49.593 ug/l
RT: 7.57 min Scan# 1988
Delta R.T. 0.00 min
Lab File: VU028399.D
Acq: 29 Nov 2018 17:20




Instrument :
MSVOA_U
ClientSampleId :
MW-6


Tgt Ion: 98 Resp: 646453
Ion Ratio Lower Upper
98 100
100 63.3 50.8 76.2

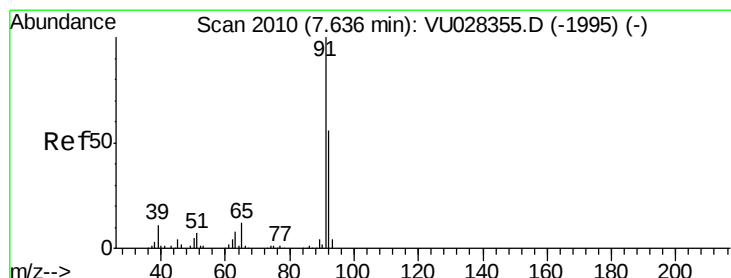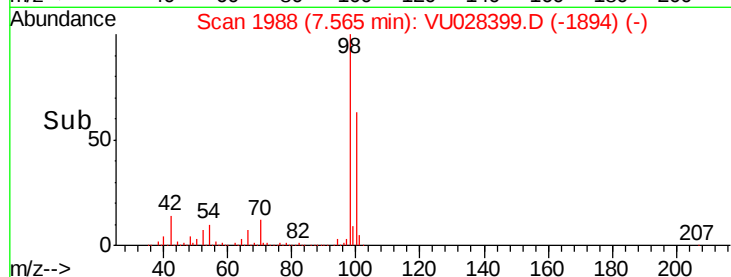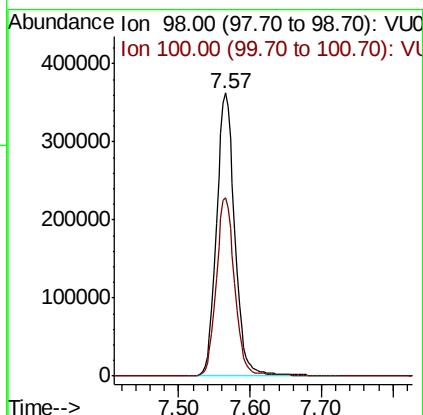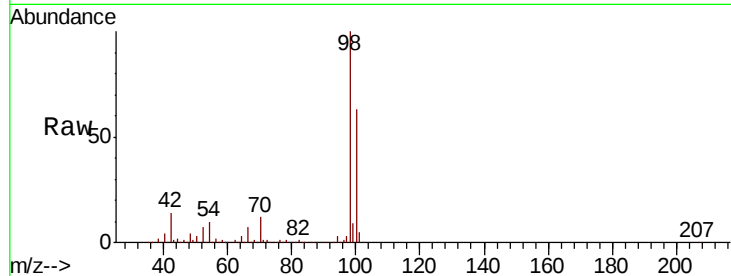

#52
Toluene
Concen: 0.570 ug/l
RT: 7.63 min Scan# 2009
Delta R.T. -0.00 min
Lab File: VU028399.D
Acq: 29 Nov 2018 17:20

Tgt Ion: 92 Resp: 5218
Ion Ratio Lower Upper
92 100
91 175.0 141.8 212.6


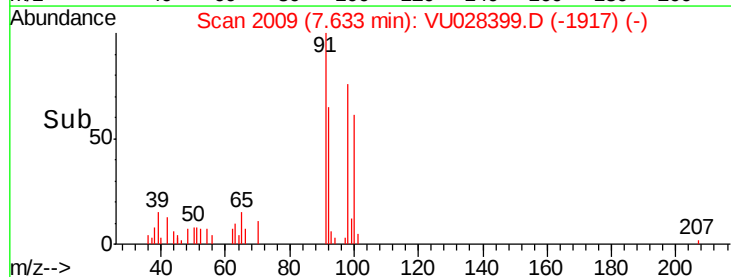
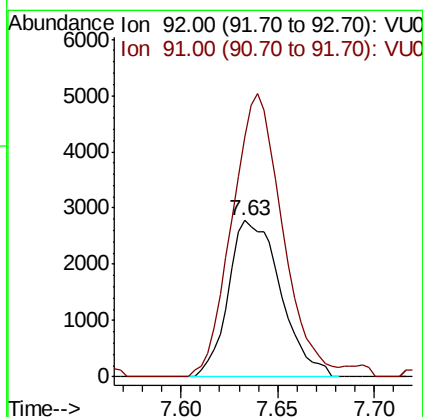
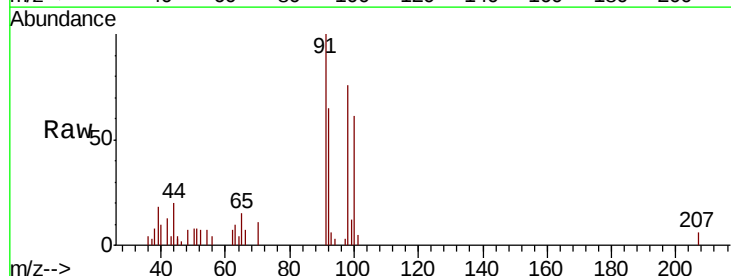


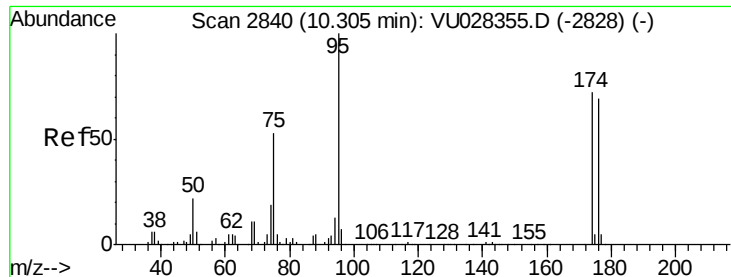

#62
4-Bromofluorobenzene
Concen: 51.433 ug/l
RT: 10.31 min Scan# 2841
Delta R.T. 0.00 min
Lab File: VU028399.D
Acq: 29 Nov 2018 17:20




Instrument :
MSVOA_U
ClientSampled :
MW-6


Tgt Ion: 95 Resp: 241648
Ion Ratio Lower Upper
95 100
174 71.8 0.0 145.4
176 71.0 0.0 140.8

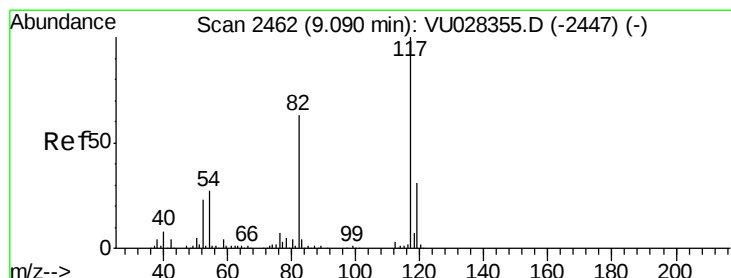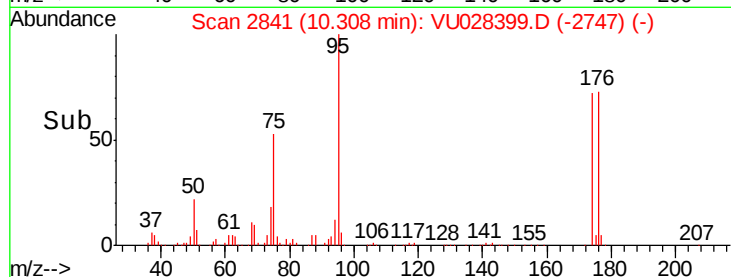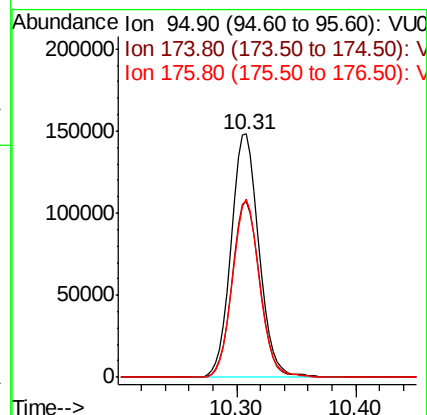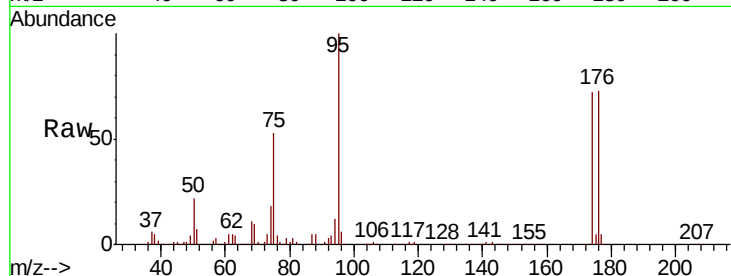

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.09 min Scan# 2462
Delta R.T. -0.00 min
Lab File: VU028399.D
Acq: 29 Nov 2018 17:20

Tgt Ion: 117 Resp: 469736
Ion Ratio Lower Upper
117 100
82 62.0 50.3 75.5
119 31.6 24.8 37.2

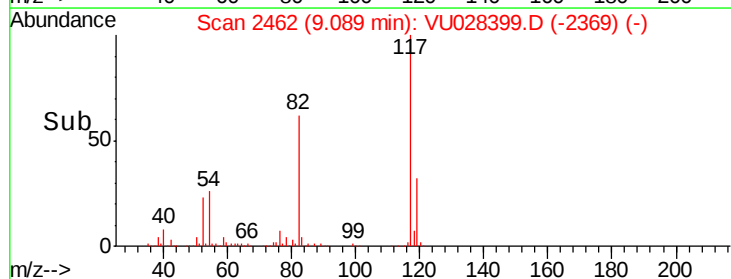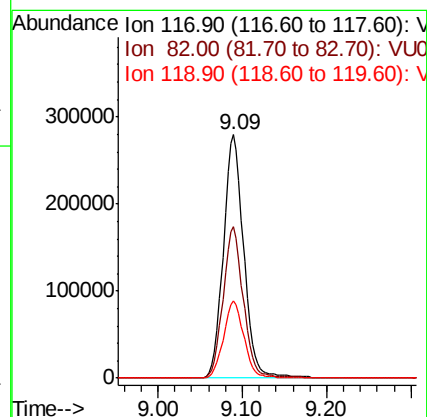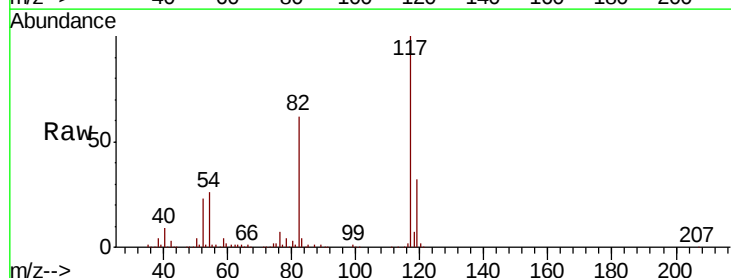

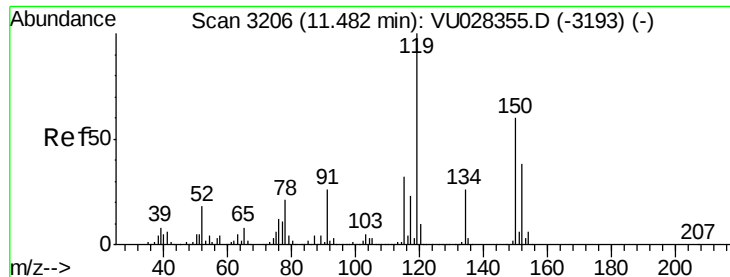

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 11.48 min Scan# 3206

Delta R.T. -0.00 min

Lab File: VU028399.D

Acq: 29 Nov 2018 17:20

Instrument :

MSVOA_U

ClientSampleId :

MW-6


Tgt Ion:152 Resp: 225994

Ion Ratio Lower Upper

152 100

115 60.7 45.0 134.8




150 155.6 0.0 349.2

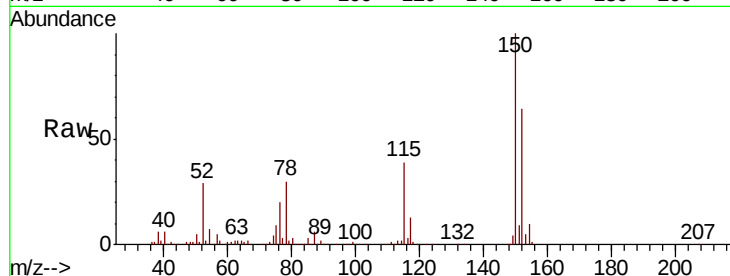

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

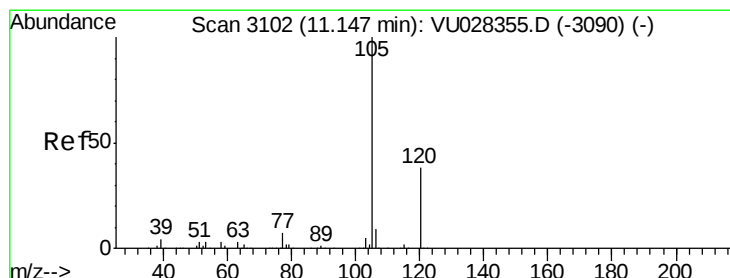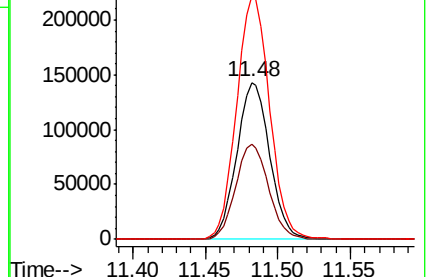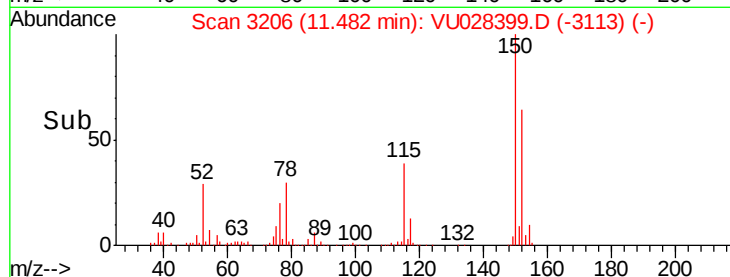

#84

1,2,4-Trimethylbenzene

Concen: 0.464 ug/l

RT: 11.15 min Scan# 3102

Delta R.T. -0.00 min

Lab File: VU028399.D


Acq: 29 Nov 2018 17:20

Tgt Ion:105 Resp: 6967

Ion Ratio Lower Upper



105 100


120 44.2 21.4 64.3

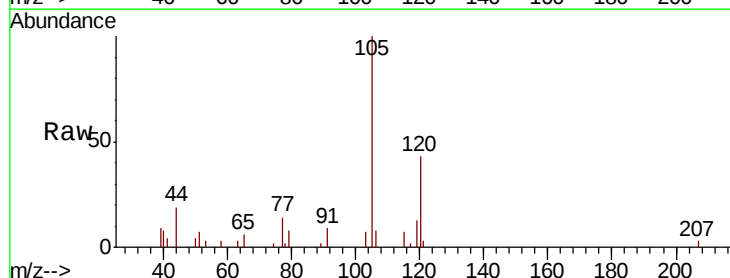

Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

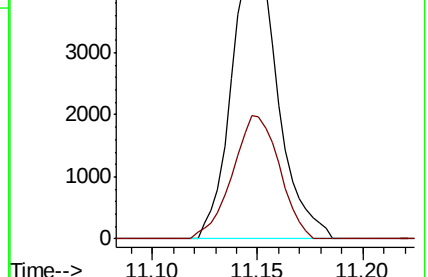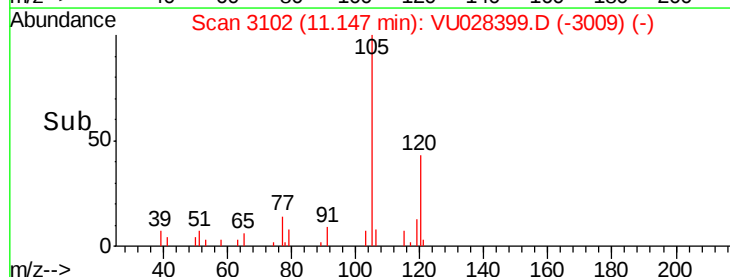

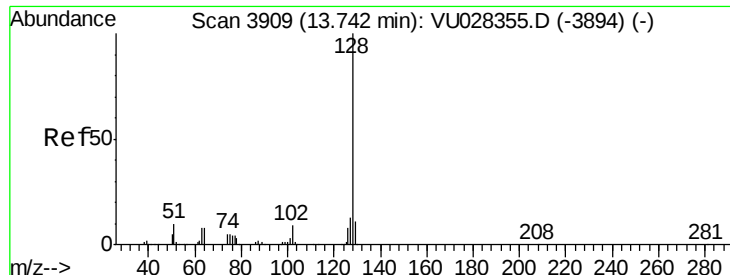

#95

Naphthalene

Concen: 3.357 ug/l

RT: 13.75 min Scan# 3912

Delta R.T. 0.01 min

Lab File: VU028399.D

Acq: 29 Nov 2018 17:20

Instrument :

MSVOA_U

ClientSampleId :

MW-6


Tgt Ion:128 Resp: 10515

Ion Ratio Lower Upper

128 100

127 11.6 10.6 15.8

129 10.2 8.6 12.8

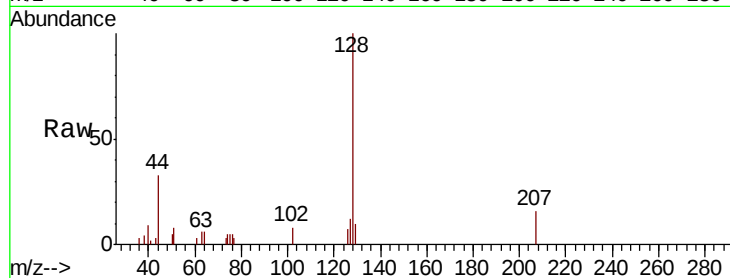

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

