


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112918\
Data File : VU028379.D
Acq On : 29 Nov 2018 08:46
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U112818W.M
Title : SW846 8260
Last Update : Thu Nov 29 01:04:49 2018

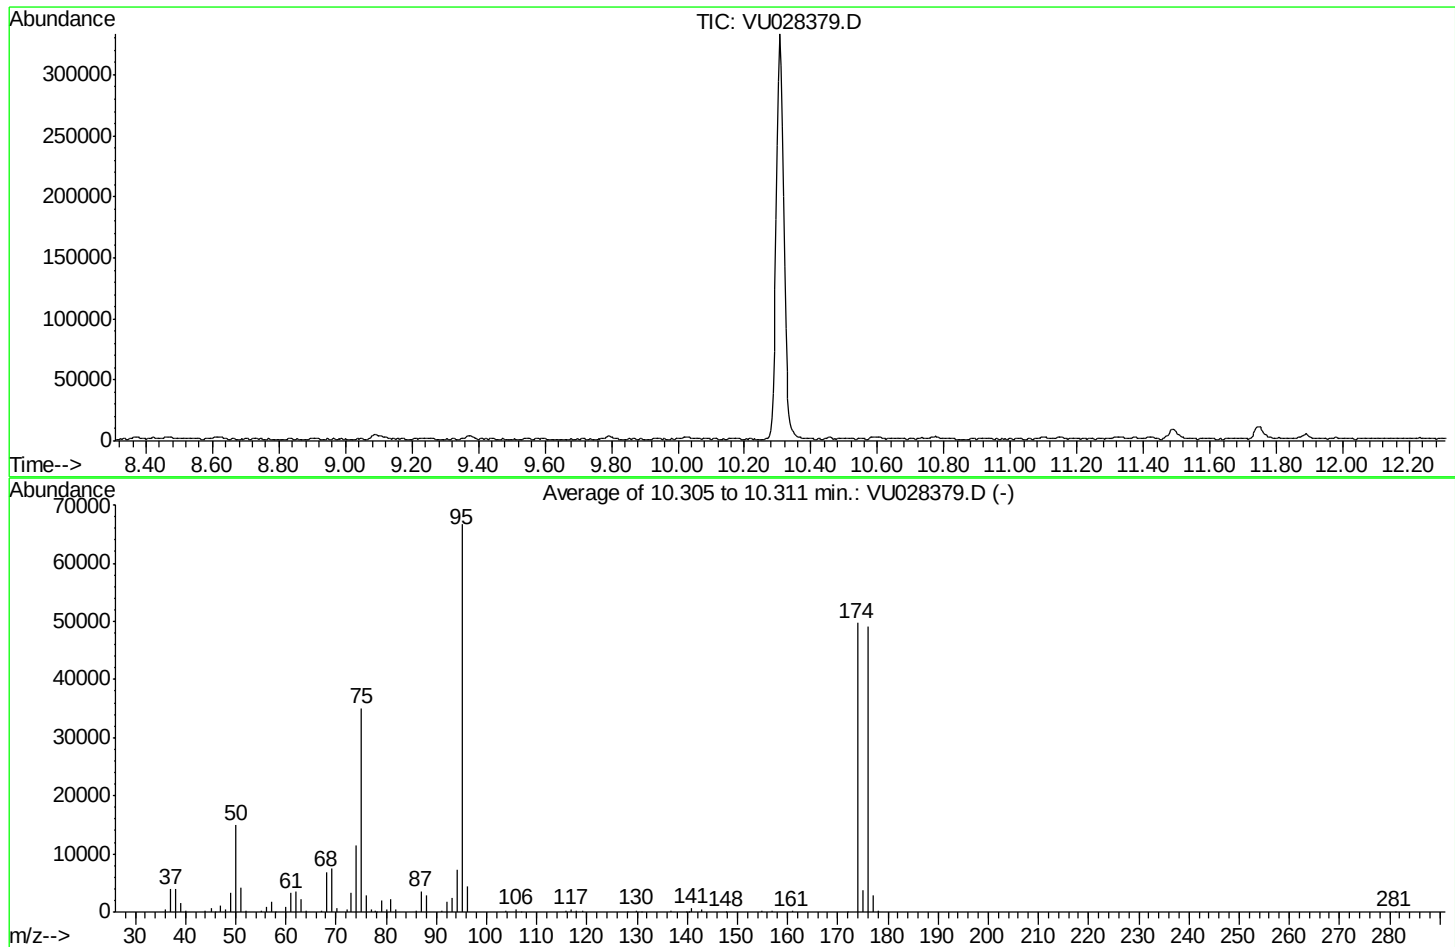

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	14927	PASS
75	95	30	60	52.4	34957	PASS
95	95	100	100	100.0	66682	PASS
96	95	5	9	6.7	4460	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	74.6	49712	PASS
175	174	5	9	7.4	3670	PASS
176	174	95	101	98.7	49058	PASS
177	176	5	9	6.0	2931	PASS