

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U112919\
 Data File : VU035917.D
 Acq On : 29 Nov 2019 12:56
 Operator : JC/SP
 Sample : K5992-18
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Quant Time: Nov 30 04:07:13 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR112119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Nov 30 03:20:00 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	226598	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.45	117	272169	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.84	152	99471	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	133515	4.51	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.20%
7) Chloroethane-d5	1.93	69	131283	5.12	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.40%
11) 1,1-Dichloroethene-d2	2.59	63	169159	3.07	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.40%
20) 2-Butanone-d5	4.70	46	367437	53.64	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.28%
24) Chloroform-d	5.11	84	247990	4.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.00%
26) 1,2-Dichloroethane-d4	5.75	65	134744	4.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.80%
32) Benzene-d6	5.77	84	467139	4.50	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.00%
36) 1,2-Dichloropropane-d6	6.73	67	163687	4.68	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.60%
41) Toluene-d8	7.93	98	356535	3.72	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.40%
43) trans-1,3-Dichloropropene-	8.21	79	54052	3.97	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.40%
46) 2-Hexanone-d5	8.68	63	269613	49.27	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.54%
57) 1,1,2,2-Tetrachloroethane-	10.78	84	136956	4.65	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.00%
64) 1,2-Dichlorobenzene-d4	12.22	152	117406	5.43	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.60%


Target Compounds				Ovalue
13) Acetone	2.68	43	15252	2.535 ug/L 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU112919\
Data File : VU035917.D
Acq On : 29 Nov 2019 12:56
Operator : JC/SP
Sample : K5992-18
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Time: Nov 30 04:07:13 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR112119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Nov 30 03:20:00 2019
Response via : Initial Calibration

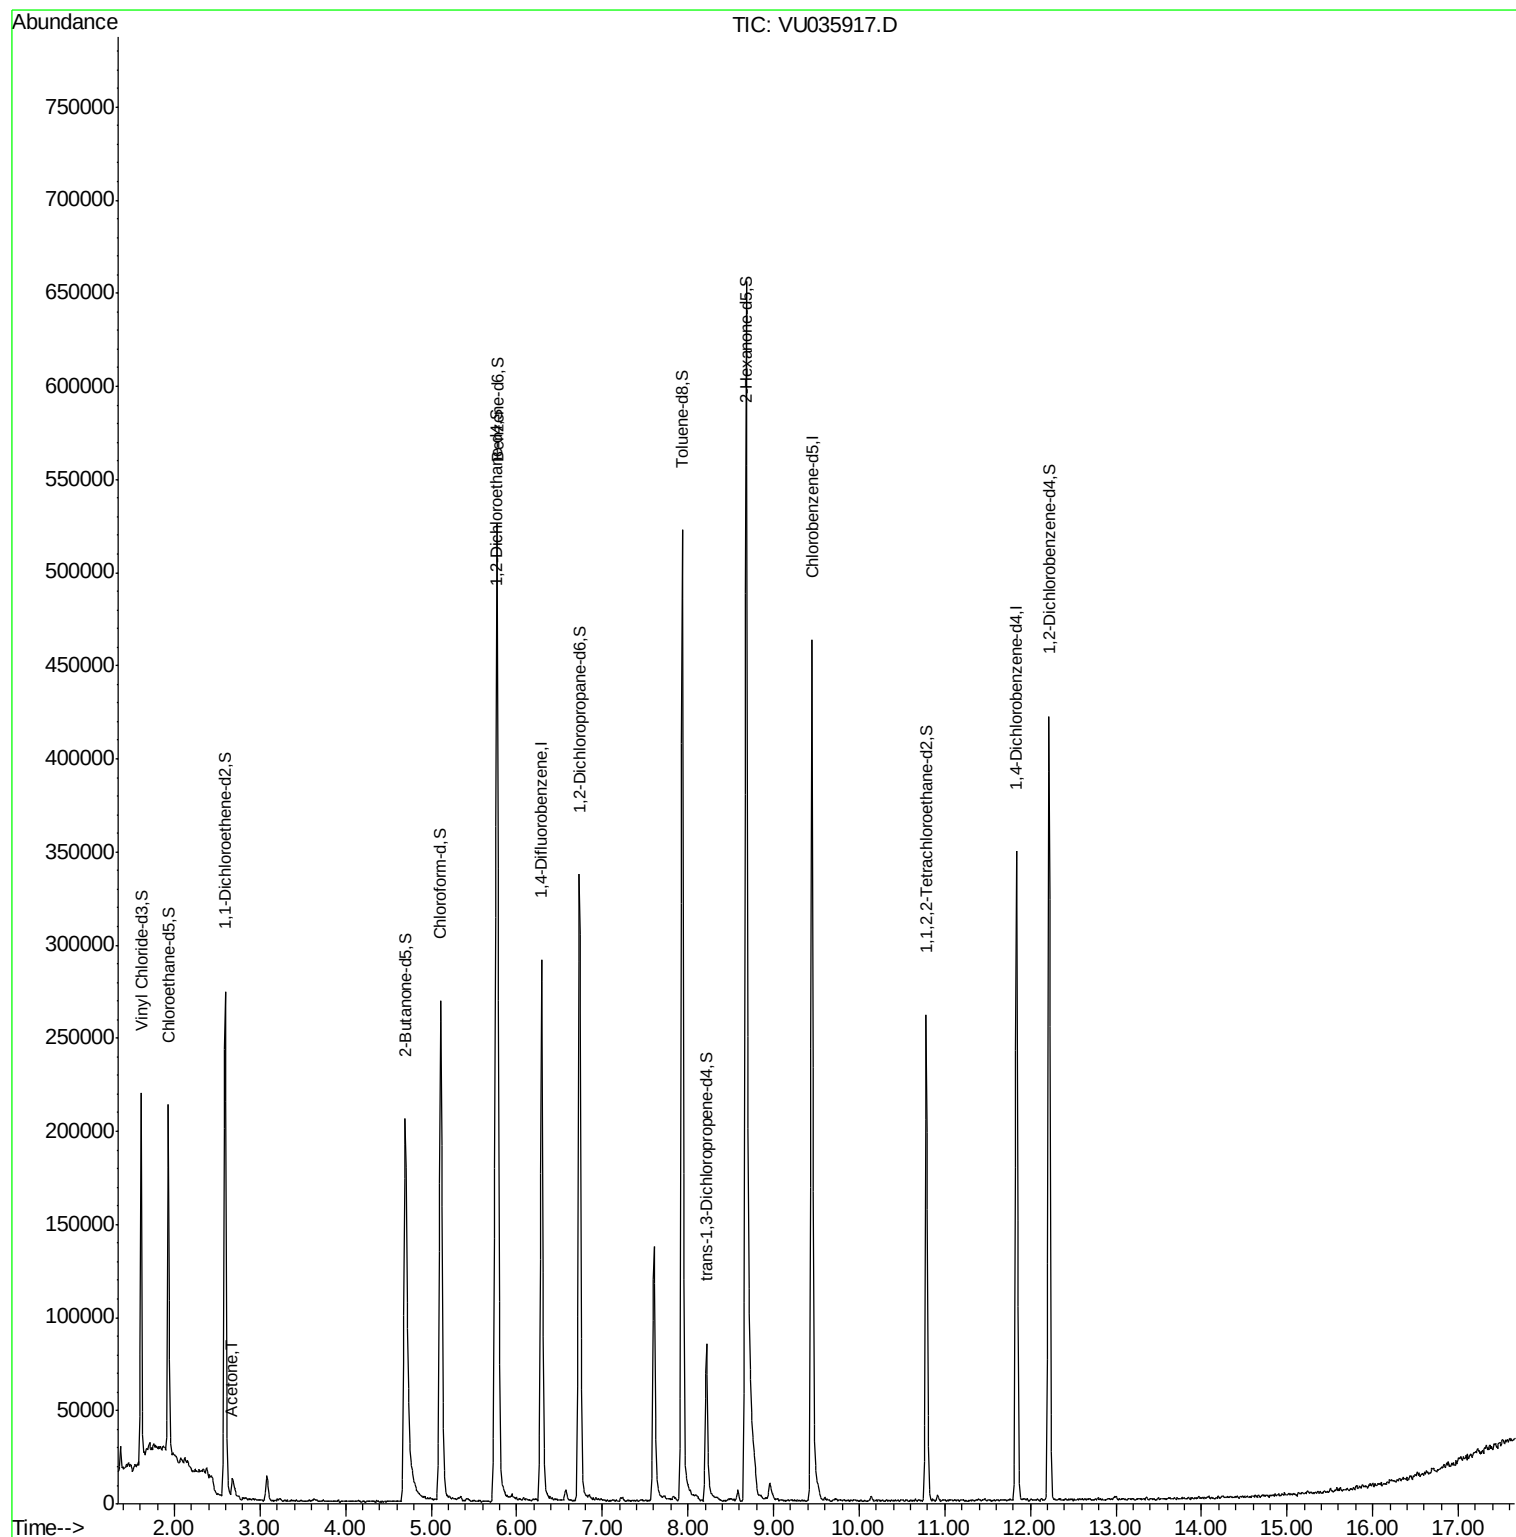

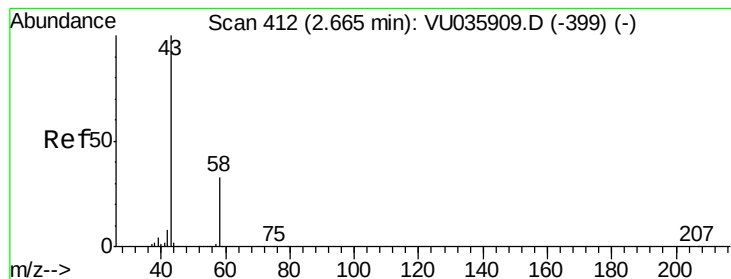

#13

Acetone

Concen: 2.535 ug/L

RT: 2.68 min Scan# 416

Delta R.T. 0.01 min

Lab File: VU035917.D

Acq: 29 Nov 2019 12:56

Instrument :

MSVOA_U

ClientSampleId :

VHBLK01

Tot Ion: 43 Resp: 15252

Ion Ratio Lower Upper

43 100

58 26.9 0.0 61.2

