

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U112919\
 Data File : VU035918.D
 Acq On : 29 Nov 2019 13:20
 Operator : JC/SP
 Sample : K5930-09
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Quant Time: Nov 30 04:06:46 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR112119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Nov 30 03:20:00 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	214120	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.45	117	250692	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.84	152	90810	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	133248	4.76	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.20%
7) Chloroethane-d5	1.93	69	129598	5.35	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	107.00%
11) 1,1-Dichloroethene-d2	2.59	63	163667	3.15	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.00%
20) 2-Butanone-d5	4.70	46	370108	57.18	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	114.36%
24) Chloroform-d	5.11	84	240978	5.09	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.80%
26) 1,2-Dichloroethane-d4	5.75	65	135175	5.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.60%
32) Benzene-d6	5.77	84	449269	4.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.00%
36) 1,2-Dichloropropane-d6	6.73	67	155335	4.82	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.40%
41) Toluene-d8	7.93	98	350066	3.97	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.40%
43) trans-1,3-Dichloropropene-	8.22	79	53526	4.26	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.20%
46) 2-Hexanone-d5	8.68	63	272308	54.02	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	108.04%
57) 1,1,2,2-Tetrachloroethane-	10.79	84	133515	4.92	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.40%
64) 1,2-Dichlorobenzene-d4	12.22	152	110785	5.62	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	112.40%


Target Compounds				Ovalue
13) Acetone	2.68	43	14295	2.514 ug/L 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU112919\
Data File : VU035918.D
Acq On : 29 Nov 2019 13:20
Operator : JC/SP
Sample : K5930-09
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Time: Nov 30 04:06:46 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR112119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Nov 30 03:20:00 2019
Response via : Initial Calibration

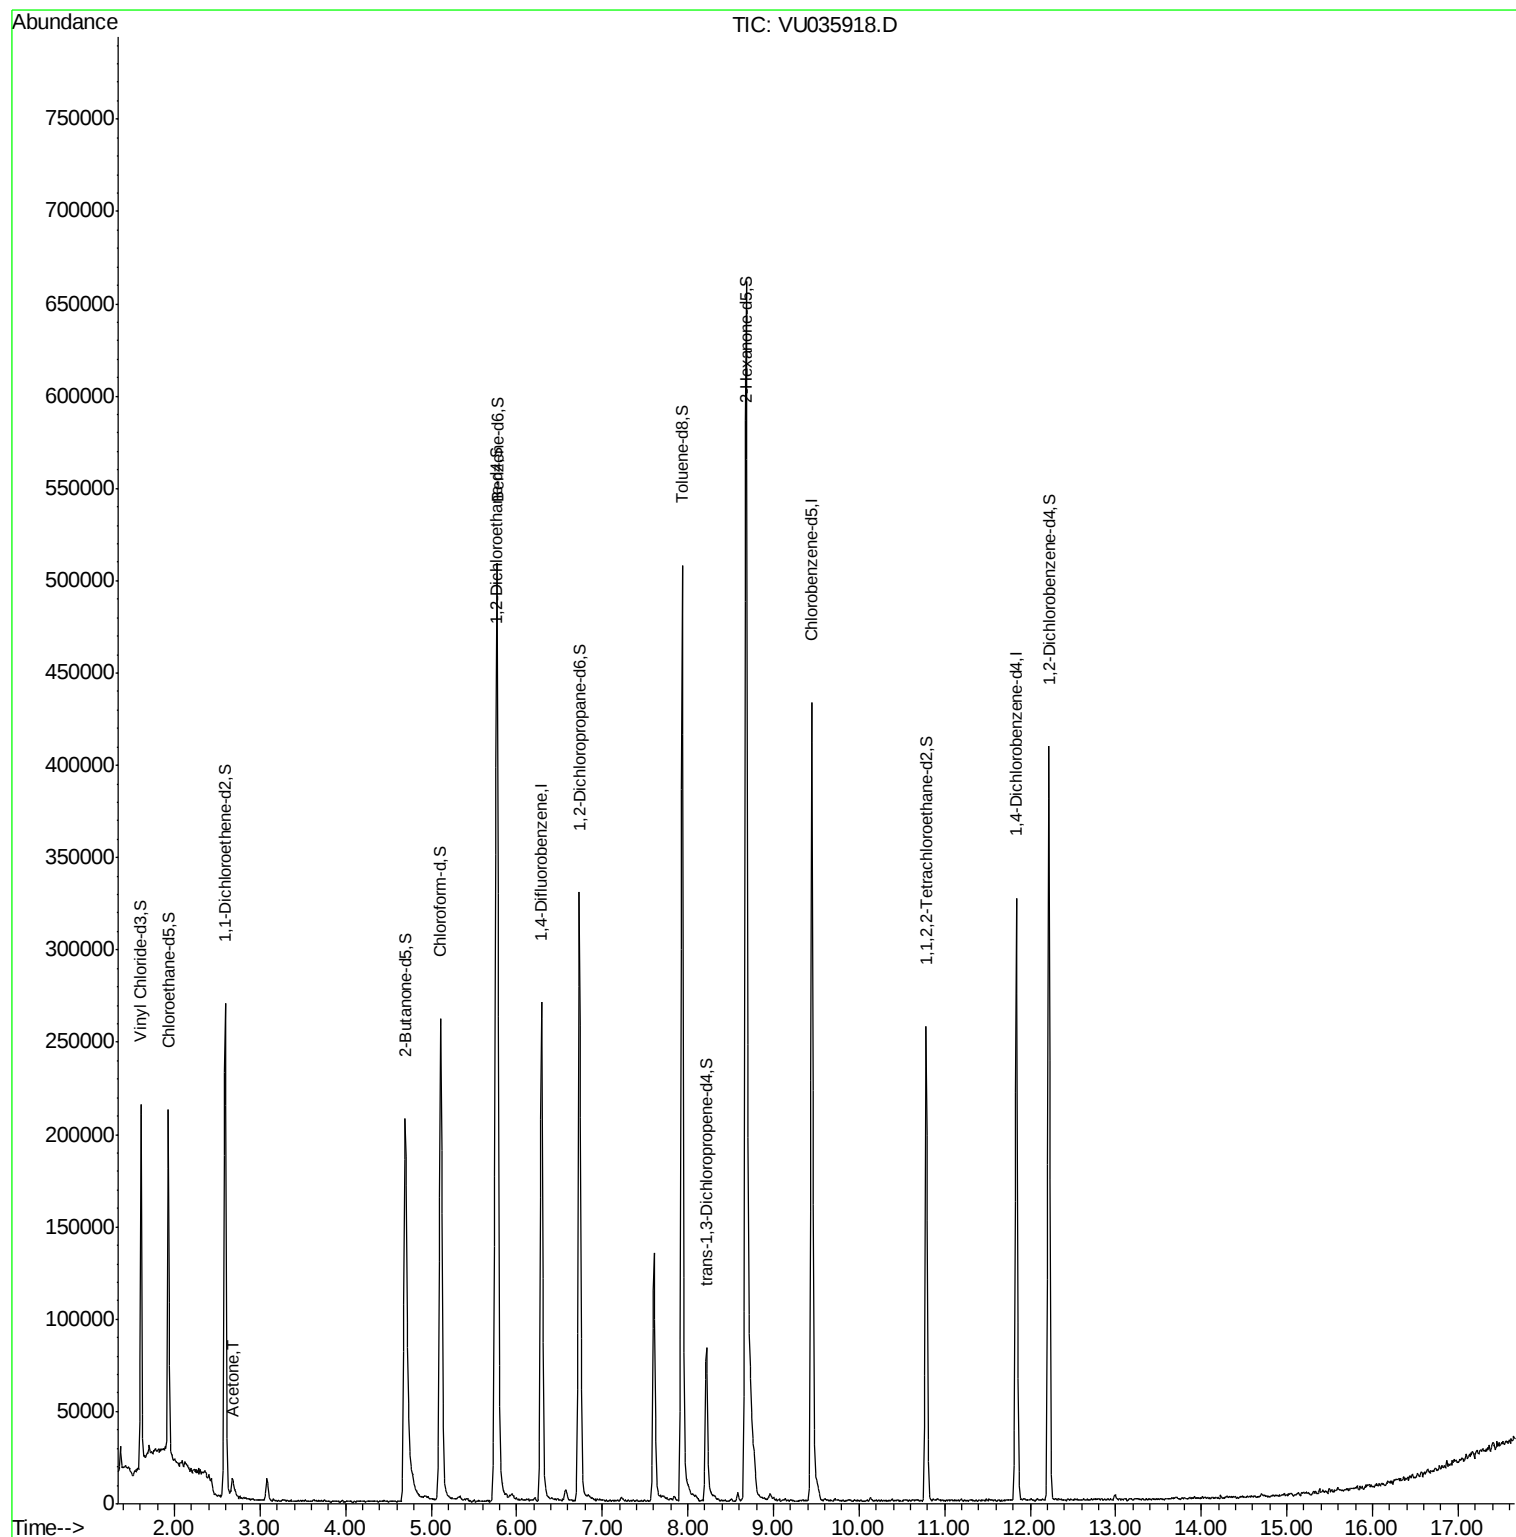

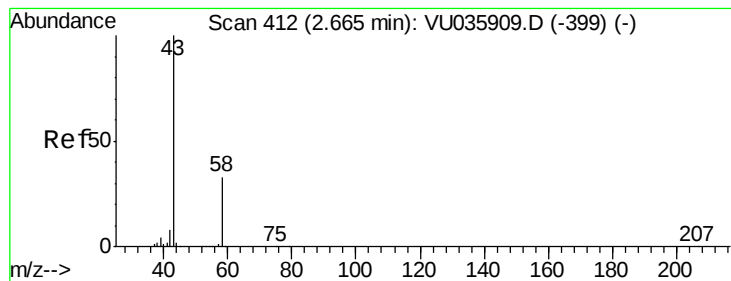

#13
 Acetone
 Concen: 2.514 ug/L
 RT: 2.68 min Scan# 417
 Delta R.T. 0.02 min
 Lab File: VU035918.D
 Acq: 29 Nov 2019 13:20

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Tot Ion: 43 Resp: 14295
 Ion Ratio Lower Upper
 43 100
 58 35.5 0.0 61.2

