
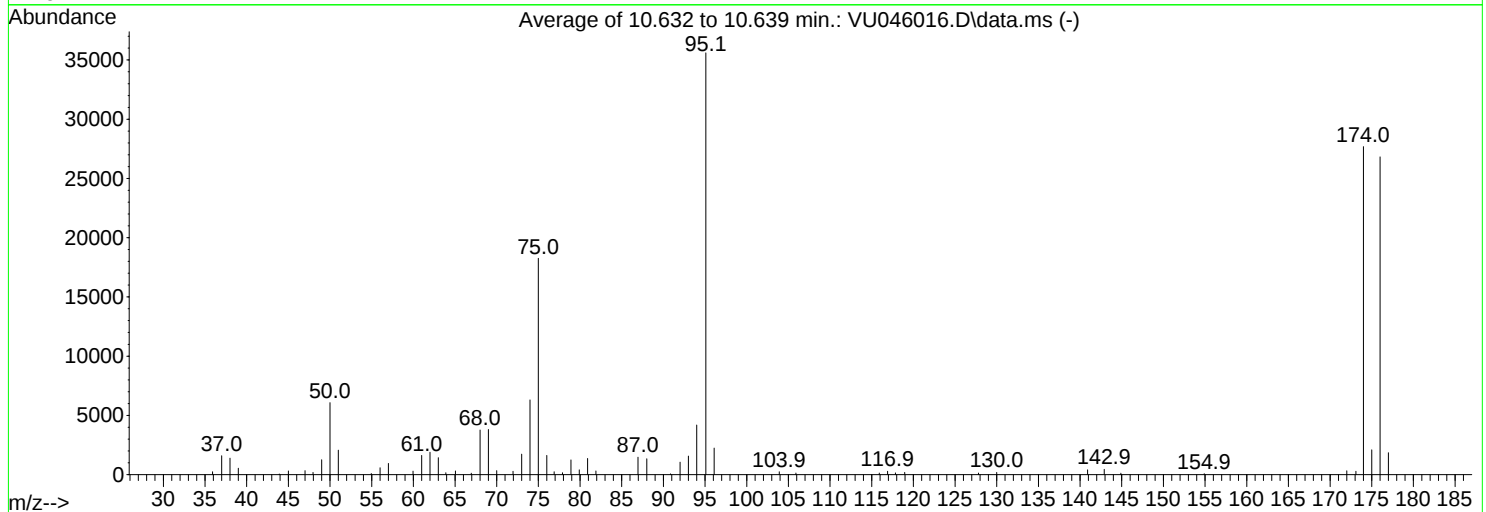


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112921\
 Data File : VU046016.D
 Acq On : 29 Nov 2021 11:15
 Operator : SY/MD
 Sample : BFB018
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB018

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis
 Last Update : Wed Dec 01 00:33:27 2021

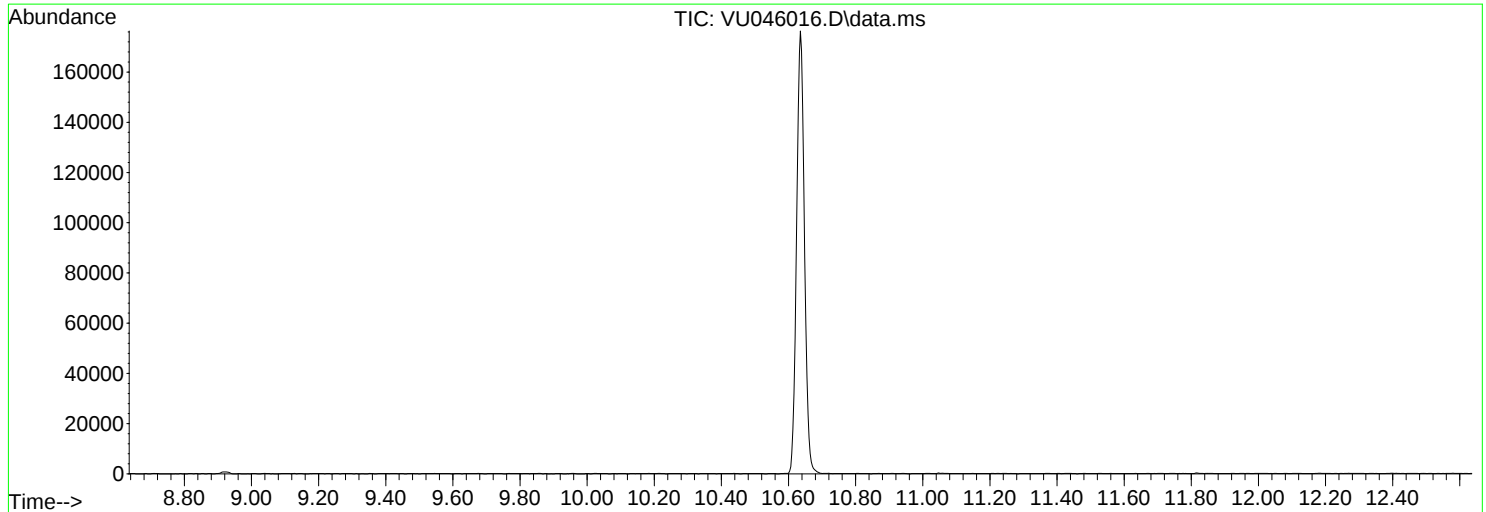

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	6079	PASS
75	95	30	80	51.3	18256	PASS
95	95	100	100	100.0	35603	PASS
96	95	5	9	6.3	2240	PASS
173	174	0.00	2	1.0	287	PASS
174	95	50	120	77.7	27680	PASS
175	174	5	9	7.6	2092	PASS
176	174	95	101	96.9	26819	PASS
177	176	5	9	6.9	1847	PASS

m/z	Abundance
43.90	223.0

Instrument :
MSVOA_U
ClientSampleId :
BFB018

m/z	Abundance
35.90	255.0
37.00	1525.0
38.00	1389.0
39.00	512.0
44.00	269.0
45.00	318.0
47.00	336.0
47.90	179.0
49.00	1315.0
50.00	5958.0
51.00	2082.0
55.00	101.0
56.00	588.0
57.00	922.0
60.00	322.0
61.00	1580.0
62.00	1939.0
63.00	1401.0
63.90	169.0
65.00	339.0
67.00	116.0
68.00	3734.0
69.00	3764.0
70.00	301.0
71.90	287.0
73.00	1798.0
74.00	6244.0
75.00	18224.0
76.00	1595.0
76.90	255.0
77.90	156.0
78.90	1242.0
79.90	374.0
80.90	1374.0
81.90	303.0
86.90	1492.0
88.00	1200.0
90.80	116.0
92.00	1027.0
93.00	1527.0
94.00	4073.0
95.10	35160.0
96.10	2348.0
103.90	218.0
105.90	141.0
115.90	110.0
116.90	272.0
117.90	153.0
119.00	203.0
127.80	139.0
130.00	176.0
140.90	392.0
142.90	485.0
144.90	103.0
172.00	324.0
173.10	265.0
174.00	26808.0
175.00	1977.0
176.00	25672.0
177.00	1781.0

Instrument :
MSVOA_U
ClientSampleId :
BFB018

m/z	Abundance
35.90	266.0
37.00	1681.0
38.00	1416.0
39.00	562.0
44.00	282.0
45.00	333.0
47.00	359.0
47.90	195.0
49.00	1269.0
50.00	6342.0
51.00	2102.0
54.90	103.0
56.00	605.0
57.00	970.0
59.90	299.0
61.00	1690.0
62.00	1953.0
63.00	1474.0
63.90	166.0
65.00	312.0
67.00	122.0
68.00	3895.0
69.00	3928.0
70.00	348.0
71.90	294.0
73.00	1748.0
74.00	6546.0
75.00	18896.0
76.00	1665.0
76.90	254.0
77.90	166.0
78.90	1287.0
79.90	414.0
80.90	1418.0
81.90	326.0
86.90	1527.0
88.00	1368.0
90.90	100.0
92.00	1074.0
93.00	1604.0
94.00	4292.0
95.10	36784.0
96.10	2317.0
103.90	282.0
105.90	141.0
115.90	137.0
116.90	290.0
117.90	160.0
119.00	200.0
127.80	146.0
130.00	201.0
140.90	412.0
142.90	463.0
144.90	122.0
154.90	122.0
172.00	339.0
173.10	304.0
174.00	28488.0
175.00	2175.0
176.00	27648.0
177.00	1925.0

Instrument :
MSVOA_U
ClientSampleId :
BFB018

m/z	Abundance
35.90	217.0
37.00	1595.0
38.00	1363.0
39.00	537.0
43.90	272.0
45.00	292.0
47.00	318.0
48.00	188.0
49.00	1181.0
50.00	5938.0
51.00	2014.0
54.90	100.0
56.00	550.0
57.00	963.0
59.90	259.0
61.00	1587.0
62.00	1781.0
63.00	1418.0
63.90	167.0
65.10	270.0
66.90	116.0
68.00	3671.0
69.00	3745.0
70.00	355.0
72.00	272.0
73.00	1634.0
74.00	6150.0
75.00	17648.0
76.00	1588.0
76.90	233.0
77.90	185.0
78.90	1202.0
79.90	427.0
80.90	1284.0
81.90	311.0
87.00	1401.0
88.00	1451.0
92.00	1051.0
93.00	1588.0
94.00	4208.0
95.10	34864.0
96.10	2056.0
103.90	251.0
105.90	130.0
115.90	149.0
116.90	293.0
117.80	146.0
118.90	180.0
127.80	128.0
130.00	195.0
140.90	415.0
142.90	402.0
144.90	124.0
154.90	130.0
172.00	326.0
173.10	291.0
174.00	27744.0
175.00	2124.0
176.00	27136.0
177.00	1835.0

Instrument :
MSVOA_U
ClientSampleId :
BFB018