
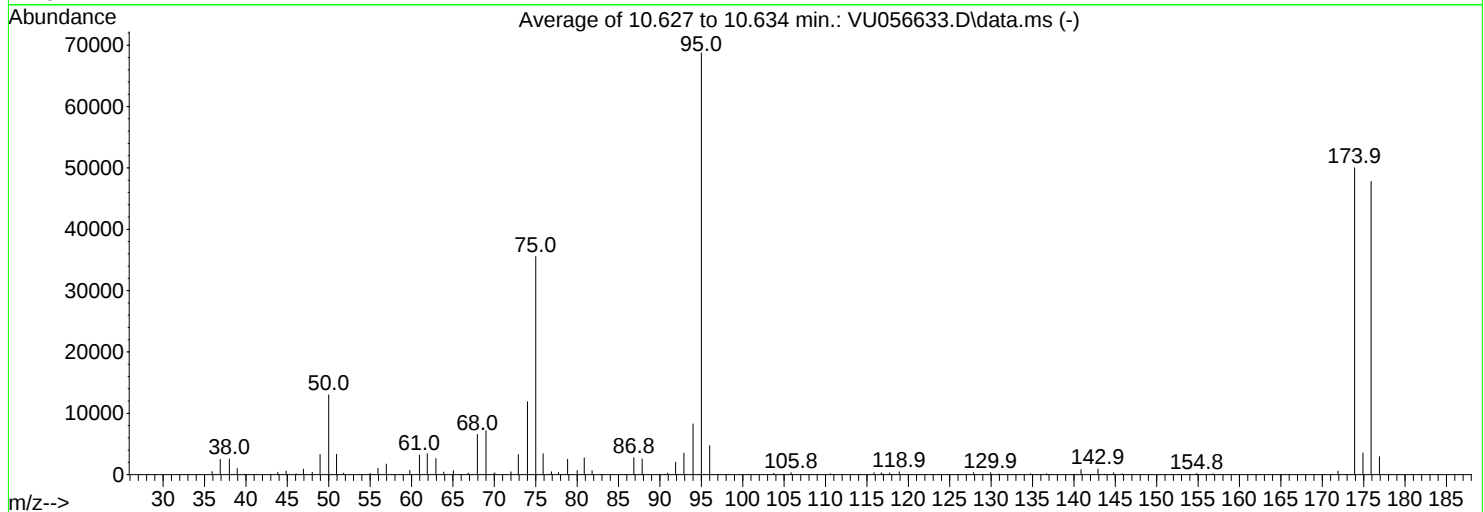


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112923\
 Data File : VU056633.D
 Acq On : 29 Nov 2023 08:34
 Operator : MD/SY
 Sample : BFB084
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB084

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Nov 29 23:29:11 2023

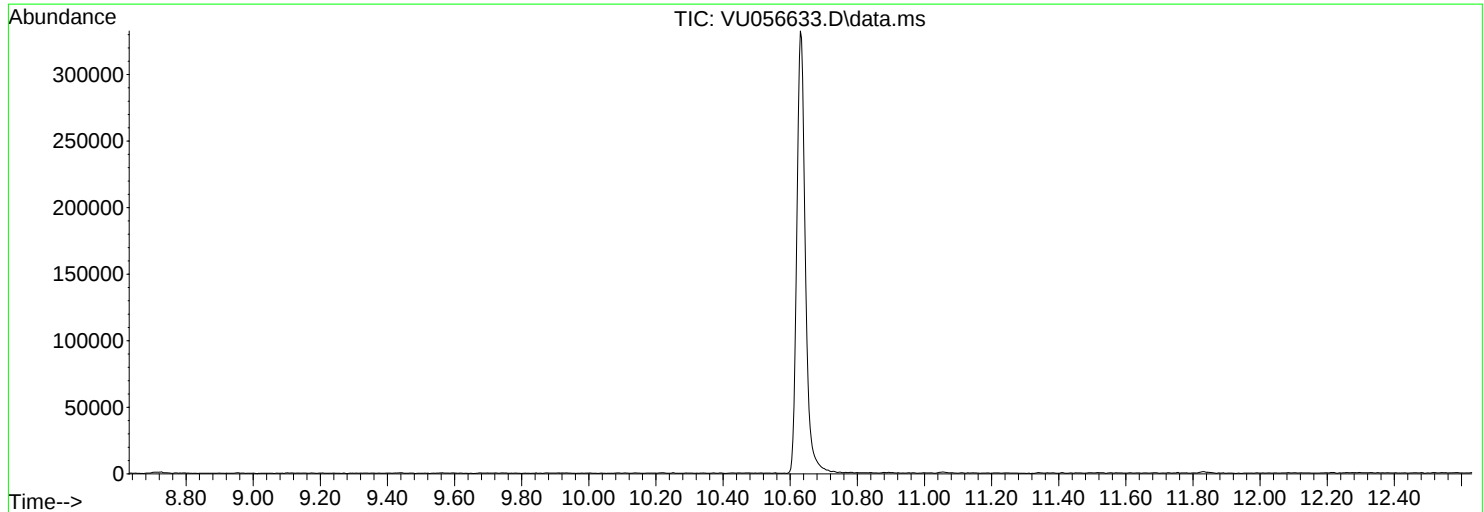

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	13014	PASS
75	95	30	80	51.7	35565	PASS
95	95	100	100	100.0	68765	PASS
96	95	5	9	6.9	4751	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.8	50032	PASS
175	174	5	9	7.0	3516	PASS
176	174	95	101	95.6	47813	PASS
177	176	5	9	6.1	2926	PASS

m/z	Abundance
39.80	132.0
43.90	412.0

Instrument :
MSVOA_U
ClientSampleId :
BFB084

m/z	Abundance
35.90	444.0
36.90	2448.0
38.00	2602.0
38.90	1006.0
40.00	231.0
43.80	753.0
44.80	651.0
46.00	134.0
46.90	895.0
48.00	380.0
48.90	2934.0
50.00	12826.0
50.90	3213.0
51.80	223.0
55.00	241.0
56.00	913.0
57.00	1620.0
59.80	678.0
60.90	2952.0
61.90	3431.0
63.00	2496.0
63.90	449.0
65.00	622.0
66.80	307.0
67.90	6692.0
69.00	7042.0
69.90	427.0
72.00	415.0
72.90	3444.0
74.00	11664.0
75.00	34984.0
75.90	3345.0
76.90	528.0
77.70	311.0
78.90	2536.0
80.00	656.0
80.80	2726.0
81.80	674.0
82.80	138.0
86.80	2762.0
87.80	2475.0
90.60	179.0
91.00	232.0
91.90	2157.0
92.90	3476.0
94.00	7871.0
95.00	65752.0
96.00	4596.0
103.80	216.0
105.90	312.0
110.60	155.0
115.80	300.0
116.80	345.0
117.80	278.0
118.80	407.0
127.90	325.0
130.00	412.0
131.00	144.0
134.80	159.0
136.70	147.0
140.90	809.0
142.90	827.0
144.80	317.0
145.90	101.0
154.80	208.0
156.80	140.0
171.90	478.0
173.90	47152.0
174.90	3356.0
175.90	45352.0
176.90	2737.0

Instrument :
MSVOA_U
ClientSampleId :
BFB084

m/z	Abundance
35.90	547.0
36.90	2559.0
38.00	2665.0
39.00	1017.0
39.90	235.0
43.90	833.0
44.80	594.0
46.00	168.0
46.90	946.0
48.00	413.0
49.00	3402.0
50.00	13476.0
50.90	3358.0
51.80	222.0
55.00	222.0
55.90	1079.0
56.90	1729.0
59.80	727.0
61.00	3309.0
61.90	3526.0
62.90	2660.0
63.90	426.0
65.00	662.0
66.80	273.0
68.00	6715.0
69.00	7394.0
70.10	417.0
72.00	497.0
72.90	3377.0
74.00	12388.0
75.00	36488.0
75.90	3546.0
76.90	475.0
77.70	376.0
78.80	2551.0
80.00	748.0
80.80	2838.0
81.80	682.0
86.80	2914.0
87.90	2605.0
90.90	212.0
91.90	1977.0
92.90	3704.0
94.00	8653.0
95.00	70416.0
96.00	4888.0
103.70	222.0
104.80	135.0
105.80	307.0
110.60	154.0
115.90	330.0
116.70	339.0
117.70	309.0
118.90	482.0
127.90	366.0
130.00	341.0
131.00	136.0
134.70	145.0
136.70	167.0
140.80	860.0
142.90	984.0
143.70	127.0
144.80	319.0
145.80	161.0
154.90	203.0
156.80	163.0
171.90	624.0
173.90	51040.0
174.90	3586.0
175.90	49152.0
176.90	2977.0
178.10	117.0

Instrument :
MSVOA_U
ClientSampleId :
BFB084

m/z	Abundance
35.90	533.0
36.90	2504.0
38.00	2426.0
38.90	998.0
39.90	215.0
43.90	833.0
44.90	485.0
46.10	162.0
47.00	863.0
48.00	366.0
49.00	3520.0
50.00	12740.0
51.00	3405.0
51.80	237.0
54.90	140.0
55.90	1116.0
56.90	1815.0
59.80	730.0
61.00	3353.0
61.90	3269.0
62.90	2746.0
63.90	375.0
65.10	690.0
66.90	208.0
68.00	6281.0
69.00	7047.0
70.00	459.0
72.00	469.0
72.90	3035.0
74.00	11670.0
75.00	35224.0
75.90	3392.0
76.90	381.0
77.80	346.0
78.80	2414.0
80.00	681.0
80.90	2692.0
81.80	573.0
85.80	134.0
86.90	2620.0
87.90	2580.0
90.80	246.0
91.90	1865.0
92.90	3398.0
94.00	8279.0
95.00	70128.0
96.00	4769.0
97.00	124.0
103.70	256.0
104.90	137.0
105.80	313.0
110.60	106.0
115.80	310.0
116.70	287.0
117.00	319.0
117.80	318.0
118.90	520.0
127.90	324.0
129.80	281.0
130.90	105.0
134.70	107.0
136.70	177.0
140.90	872.0
142.90	945.0
143.70	148.0
144.80	375.0
145.80	205.0
154.90	210.0
156.80	170.0
171.90	626.0
173.90	51904.0
174.90	3607.0
175.90	48936.0
176.90	3065.0
178.00	119.0

Instrument :
MSVOA_U
ClientSampleId :
BFB084