


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU113018\
 Data File : VU028407.D
 Acq On : 30 Nov 2018 08:27
 Operator : MD/SY
 Sample : BFB59
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB59

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM113018WMA.M
 Title : VOC Analysis
 Last Update : Fri Nov 30 23:11:27 2018

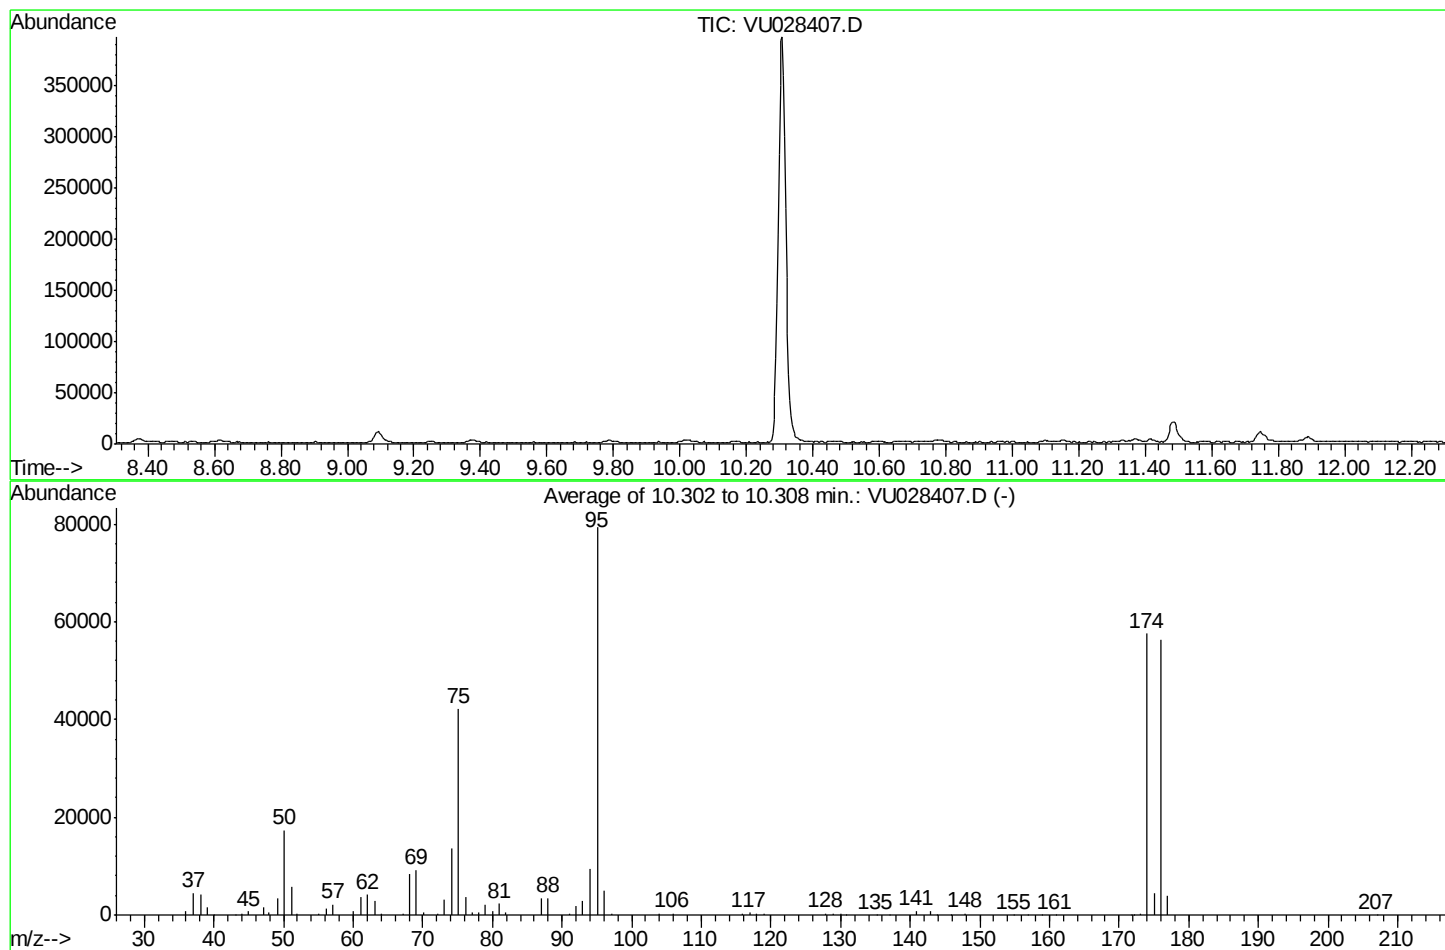

AutoFind: Scans 2839, 2840, 2841; Background Corrected with Scan 2827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	17320	PASS
75	95	30	80	53.3	42245	PASS
95	95	100	100	100.0	79314	PASS
96	95	5	9	6.3	4963	PASS
173	174	0.00	2	0.5	274	PASS
174	95	50	120	72.6	57554	PASS
175	174	5	9	7.7	4403	PASS
176	174	95	101	98.0	56392	PASS
177	176	5	9	6.9	3908	PASS

m/z	Abundance
36.00	851.0
37.10	4358.0
38.10	4041.0
39.00	1621.0
40.10	472.0
43.20	129.0
44.10	995.0
45.10	901.0
47.10	1407.0
48.00	475.0
49.10	3131.0
50.10	16672.0
51.10	5101.0
52.00	121.0
55.00	367.0
56.10	1219.0
57.10	2089.0
60.10	751.0
61.10	3397.0
62.00	3893.0
63.10	2719.0
64.00	221.0
67.10	211.0
68.10	7936.0
69.10	8690.0
70.10	552.0
72.00	481.0
73.10	3104.0
74.10	12152.0
75.10	38744.0
76.10	3545.0
77.10	512.0
78.10	544.0
78.90	1970.0
80.00	721.0
81.00	2076.0
81.90	428.0
87.00	3176.0
88.00	3189.0
91.00	308.0
92.00	1780.0
93.00	2631.0
94.10	8606.0
95.10	73488.0
96.10	4683.0
97.10	212.0
104.00	254.0
105.90	311.0
115.90	235.0
116.90	422.0
117.90	197.0
119.00	289.0
127.90	303.0
128.90	172.0
130.00	212.0
135.10	119.0
141.00	705.0
142.90	686.0
147.90	290.0
155.00	123.0
157.00	134.0
160.90	109.0
171.70	172.0
173.10	824.0
174.00	51080.0
175.00	4140.0
176.00	51168.0
177.00	3633.0
207.00	169.0

Instrument :
MSVOA_U
ClientSampleId :
BFB59

m/z	Abundance
39.90	406.0
41.00	169.0
42.10	101.0
43.10	111.0
44.00	859.0
45.00	108.0
207.00	184.0

Instrument :
MSVOA_U
ClientSampleId :
BFB59

m/z	Abundance
36.00	890.0
37.10	4586.0
38.10	4087.0
39.10	1802.0
40.00	426.0
41.00	115.0
43.00	138.0
44.00	1199.0
45.00	761.0
47.10	1750.0
47.90	643.0
49.10	3801.0
50.10	17216.0
51.10	6097.0
52.00	205.0
55.00	268.0
56.10	1543.0
57.10	2190.0
60.00	835.0
61.10	3954.0
62.10	4343.0
63.10	3033.0
64.00	263.0
67.10	303.0
68.10	8234.0
69.10	9517.0
70.00	657.0
72.10	313.0
73.10	3169.0
74.10	14524.0
75.10	44312.0
76.10	3778.0
77.10	739.0
78.10	320.0
79.00	2297.0
80.10	624.0
81.00	2381.0
82.00	594.0
87.00	3382.0
88.00	3557.0
91.10	345.0
92.00	1928.0
93.00	3112.0
94.10	9666.0
95.10	82112.0
96.10	5060.0
97.00	231.0
104.00	253.0
105.90	299.0
115.90	294.0
116.90	543.0
118.00	215.0
119.00	307.0
127.90	226.0
128.90	102.0
130.00	307.0
130.70	152.0
135.20	120.0
137.10	150.0
140.90	914.0
142.90	801.0
143.90	105.0
145.80	104.0
147.90	254.0
154.90	124.0
156.80	118.0
158.90	131.0
172.10	141.0
174.00	61728.0
175.00	4572.0
176.00	59872.0
177.00	4005.0
207.00	249.0

Instrument :
MSVOA_U
ClientSampleId :
BFB59

m/z	Abundance
36.00	975.0
37.10	4666.0
38.10	4298.0
39.10	1706.0
40.00	474.0
41.00	111.0
43.00	109.0
44.00	1094.0
45.00	853.0
47.10	1831.0
47.90	537.0
49.10	3623.0
50.10	18072.0
51.10	5874.0
52.00	149.0
55.00	315.0
56.10	1498.0
57.10	2200.0
60.00	810.0
61.10	3610.0
62.00	4336.0
63.10	2945.0
64.00	286.0
67.10	300.0
68.10	8631.0
69.10	9676.0
70.00	632.0
72.10	407.0
73.00	3136.0
74.10	13900.0
75.10	43680.0
76.10	3935.0
77.10	656.0
78.10	418.0
79.00	2262.0
80.00	760.0
81.00	2328.0
82.00	495.0
87.00	3486.0
88.00	3555.0
91.00	328.0
92.00	2005.0
93.00	2993.0
94.10	9658.0
95.10	82344.0
96.10	5148.0
97.00	264.0
104.00	262.0
105.90	325.0
115.90	316.0
116.90	493.0
118.00	227.0
119.00	286.0
127.90	283.0
128.90	167.0
130.00	275.0
130.70	105.0
135.20	128.0
137.10	145.0
141.00	833.0
142.90	773.0
143.90	127.0
145.90	117.0
147.90	293.0
155.00	123.0
157.00	115.0
160.90	113.0
171.80	132.0
172.10	136.0
174.00	59856.0
175.00	4498.0
176.00	58136.0
177.00	4088.0
207.00	242.0

Instrument :
MSVOA_U
ClientSampleId :
BFB59