


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU113020\
 Data File : VU041433.D
 Acq On : 30 Nov 2020 09:24
 Operator : SY/MD
 Sample : BFB35
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB135

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUTR113020WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Dec 01 01:39:43 2020

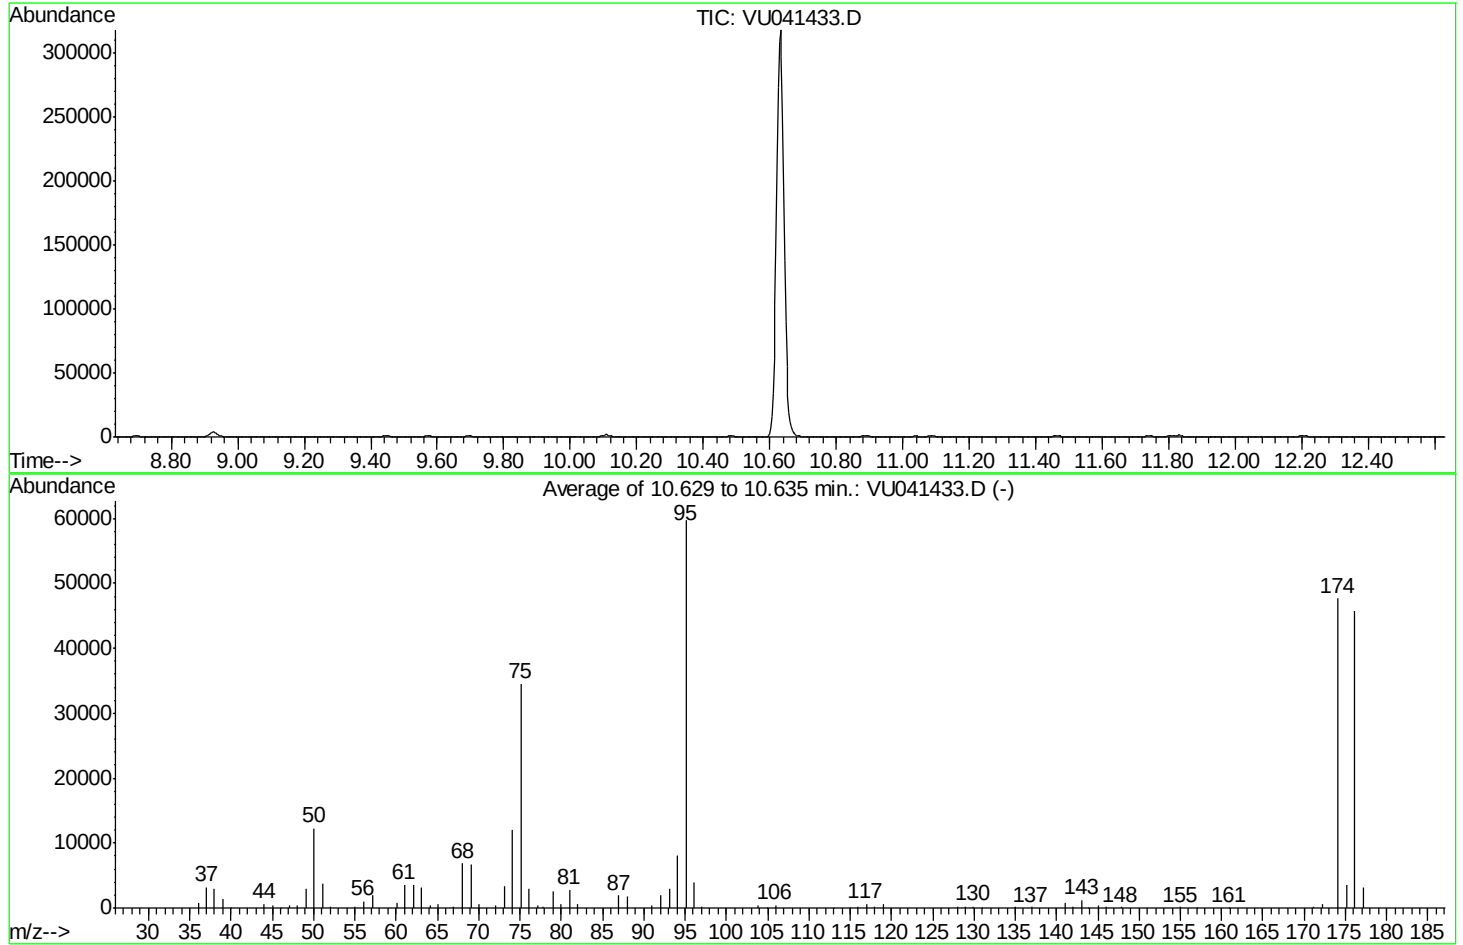

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	12275	PASS
75	95	30	80	57.9	34576	PASS
95	95	100	100	100.0	59728	PASS
96	95	5	9	6.7	4020	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	79.9	47693	PASS
175	174	5	9	7.6	3613	PASS
176	174	95	101	96.2	45858	PASS
177	176	5	9	6.9	3148	PASS

m/z Abundance

Instrument :
MSVOA_U
ClientSampleId :
BFB135

m/z	Abundance
36.00	664.0
37.00	3149.0
38.00	2898.0
39.00	1286.0
44.00	632.0
45.10	454.0
46.00	103.0
47.10	469.0
48.00	402.0
49.10	3043.0
50.10	12440.0
51.00	3829.0
52.00	169.0
55.00	219.0
56.00	1067.0
57.10	1927.0
60.10	719.0
61.00	3611.0
62.10	3624.0
63.10	3300.0
64.00	401.0
65.10	529.0
66.90	231.0
68.00	6937.0
69.10	6867.0
70.10	672.0
72.10	403.0
73.10	3272.0
74.10	12259.0
75.10	34976.0
76.10	3002.0
77.10	376.0
77.80	187.0
79.00	2516.0
80.00	689.0
81.00	2749.0
82.00	648.0
87.00	1989.0
88.10	1939.0
91.00	323.0
92.00	2047.0
93.10	3065.0
94.10	8179.0
95.10	60456.0
96.10	3993.0
96.90	138.0
103.90	390.0
106.00	353.0
115.00	131.0
115.90	277.0
117.00	621.0
118.00	248.0
119.00	566.0
128.00	251.0
129.00	132.0
129.90	243.0
130.90	142.0
135.00	170.0
137.00	191.0
141.00	808.0
142.00	141.0
143.10	1270.0
143.90	102.0
145.00	371.0
146.00	125.0
147.90	147.0
155.00	184.0
157.00	108.0
160.90	103.0
171.20	124.0
172.20	515.0
174.10	47016.0
175.10	3685.0
176.10	45440.0
177.10	3216.0

Instrument :
MSVOA_U
ClientSampleId :
BFB135

m/z	Abundance
36.00	744.0
37.00	3277.0
38.00	3030.0
39.00	1373.0
39.90	100.0
44.00	651.0
45.10	472.0
46.00	113.0
47.10	481.0
48.00	369.0
49.00	3070.0
50.10	12599.0
51.00	3928.0
52.00	199.0
55.00	273.0
56.00	1106.0
57.10	1968.0
60.10	785.0
61.00	3778.0
62.10	3709.0
63.10	3253.0
64.10	370.0
65.10	526.0
66.90	224.0
68.00	7025.0
69.10	6966.0
70.10	561.0
72.10	373.0
73.10	3590.0
74.10	12373.0
75.10	35752.0
76.10	3115.0
77.10	413.0
77.80	181.0
79.00	2562.0
80.00	705.0
81.00	2861.0
82.00	614.0
87.00	2020.0
88.10	1891.0
91.00	348.0
92.00	2015.0
93.10	3087.0
94.10	8245.0
95.10	61704.0
96.10	4173.0
97.00	178.0
103.90	401.0
104.90	107.0
106.00	415.0
115.00	119.0
115.90	272.0
117.00	636.0
118.00	299.0
119.00	559.0
128.00	216.0
129.00	143.0
130.00	243.0
130.90	128.0
135.00	155.0
137.00	177.0
141.00	834.0
142.00	159.0
143.10	1287.0
145.00	377.0
146.00	165.0
147.90	160.0
155.10	176.0
157.00	105.0
160.90	111.0
171.20	143.0
172.10	541.0
174.10	49216.0
175.10	3699.0
176.10	47184.0
177.10	3240.0

Instrument :
MSVOA_U
ClientSampleId :
BFB135

m/z	Abundance
36.00	686.0
37.10	3187.0
38.00	2885.0
39.00	1246.0
40.00	102.0
44.00	577.0
45.00	464.0
47.00	460.0
48.00	352.0
49.00	2779.0
50.10	11787.0
51.10	3770.0
52.00	177.0
55.00	270.0
56.00	1080.0
57.10	1821.0
60.00	721.0
61.00	3548.0
62.10	3472.0
63.10	2845.0
64.20	386.0
65.10	477.0
66.90	189.0
68.10	6583.0
69.10	6446.0
70.00	461.0
72.10	310.0
73.10	3478.0
74.10	11573.0
75.10	33000.0
76.10	2825.0
77.10	401.0
77.80	176.0
79.00	2393.0
80.00	665.0
81.00	2741.0
81.90	555.0
87.00	1912.0
88.00	1637.0
90.90	355.0
92.10	1866.0
93.10	2828.0
94.10	7617.0
95.10	57024.0
96.10	3894.0
97.00	148.0
103.90	335.0
104.90	108.0
106.00	425.0
113.00	100.0
115.90	219.0
117.00	635.0
118.00	303.0
119.00	514.0
128.00	195.0
128.90	110.0
130.00	214.0
135.00	119.0
137.00	139.0
141.00	807.0
142.00	122.0
143.10	1176.0
145.00	326.0
146.00	172.0
147.80	175.0
155.00	155.0
157.00	100.0
171.20	147.0
172.10	532.0
174.10	46848.0
175.10	3456.0
176.10	44952.0
177.10	2989.0

Instrument :
MSVOA_U
ClientSampleId :
BFB135