


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU113021\
 Data File : VU046023.D
 Acq On : 30 Nov 2021 09:05
 Operator : SY/MD
 Sample : BFB019
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB019

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis
 Last Update : Wed Dec 01 00:33:27 2021

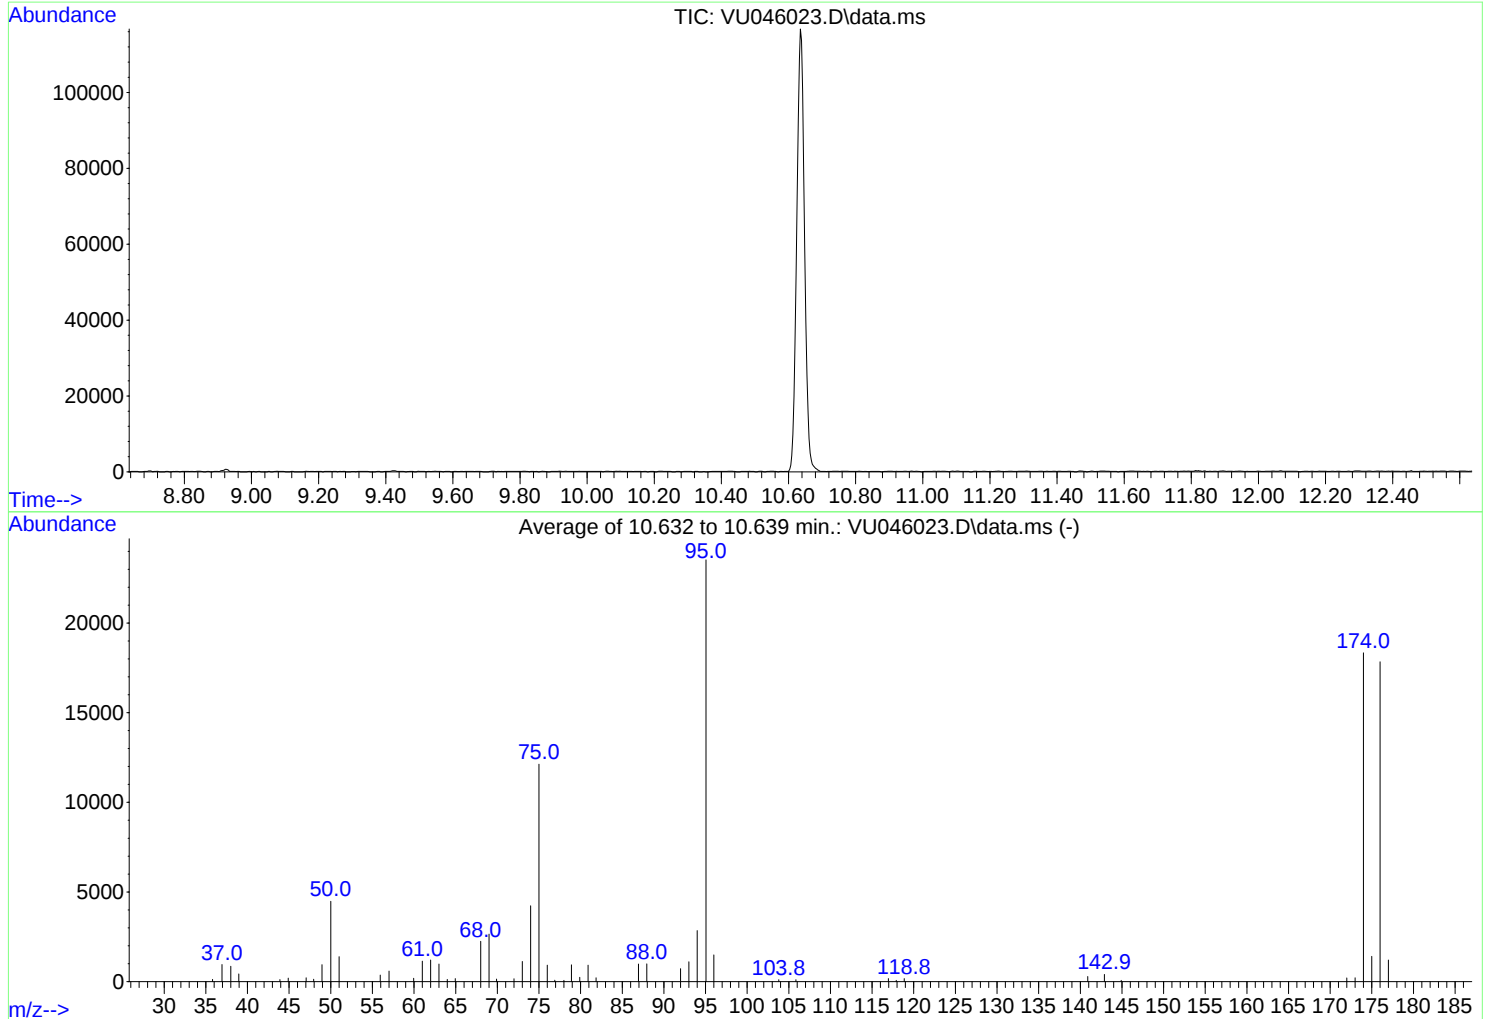

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	4483	PASS
75	95	30	80	51.6	12131	PASS
95	95	100	100	100.0	23525	PASS
96	95	5	9	6.3	1487	PASS
173	174	0.00	2	1.2	217	PASS
174	95	50	120	78.0	18341	PASS
175	174	5	9	7.7	1407	PASS
176	174	95	101	97.3	17837	PASS
177	176	5	9	6.7	1201	PASS

m/z	Abundance
35.00	103.0
37.00	865.0
38.00	904.0
39.00	463.0
43.00	248.0
44.00	173.0
47.00	201.0
47.00	128.0
48.00	921.0
50.00	4473.0
51.00	1344.0
56.00	385.0
57.00	578.0
60.00	188.0
61.00	1086.0
62.00	1244.0
63.00	953.0
64.00	105.0
65.00	154.0
68.00	2310.0
69.00	2629.0
69.00	142.0
72.00	114.0
73.00	1113.0
74.00	4165.0
75.00	12470.0
76.00	862.0
78.00	954.0
79.00	221.0
80.00	920.0
81.00	224.0
86.00	956.0
88.00	1059.0
92.00	766.0
93.00	1046.0
94.00	2797.0
95.00	23720.0
96.00	1456.0
103.00	118.0
105.00	100.0
117.00	163.0
118.00	183.0
140.00	267.0
142.00	418.0
144.00	100.0
172.00	210.0
173.00	228.0
174.00	18584.0
175.00	1478.0
176.00	18232.0
177.00	1203.0

Instrument :
MSVOA_U
ClientSampleId :
BFB019

m/z	Abundance
43.90	133.0

Instrument :
MSVOA_U
ClientSampleId :
BFB019

m/z	Abundance
35.80	142.0
36.90	1030.0
38.00	784.0
38.90	381.0
44.00	255.0
44.90	207.0
47.10	226.0
48.00	136.0
49.00	932.0
50.00	4312.0
51.00	1395.0
55.90	331.0
57.00	608.0
59.90	190.0
61.00	1140.0
62.00	1163.0
63.00	994.0
64.00	145.0
64.90	189.0
68.00	2123.0
69.00	2573.0
69.90	142.0
72.00	216.0
73.00	1101.0
74.00	4115.0
75.00	11443.0
76.00	961.0
76.90	149.0
78.00	108.0
78.90	915.0
79.90	250.0
80.90	901.0
81.90	197.0
87.00	962.0
87.90	896.0
92.00	650.0
93.00	1111.0
94.00	2835.0
95.00	22568.0
96.00	1491.0
103.80	102.0
105.80	113.0
116.90	170.0
117.90	111.0
118.80	153.0
140.90	286.0
142.90	377.0
172.00	191.0
173.00	208.0
174.00	17480.0
175.00	1293.0
176.00	16904.0
177.00	1189.0

Instrument :
MSVOA_U
ClientSampleId :
BFB019

m/z	Abundance
35.00	124.0
37.00	973.0
38.00	891.0
39.00	445.0
44.00	253.0
44.90	199.0
47.00	225.0
47.90	132.0
48.90	973.0
50.00	4663.0
51.00	1445.0
55.90	388.0
57.00	585.0
60.00	179.0
61.00	1191.0
62.00	1219.0
63.00	1010.0
64.00	119.0
65.00	177.0
68.00	2312.0
69.00	2752.0
69.90	141.0
72.00	166.0
73.00	1150.0
74.00	4399.0
75.00	12481.0
76.00	935.0
76.90	103.0
78.00	107.0
78.90	955.0
79.90	246.0
80.90	930.0
81.80	219.0
87.00	1029.0
88.00	1028.0
92.00	763.0
93.00	1161.0
94.00	2903.0
95.10	24288.0
96.00	1514.0
103.80	110.0
105.90	108.0
116.90	177.0
117.90	110.0
118.90	177.0
140.90	299.0
142.90	415.0
144.90	103.0
172.00	206.0
173.00	214.0
174.00	18960.0
175.00	1449.0
176.00	18376.0
177.00	1211.0

Instrument :
MSVOA_U
ClientSampleId :
BFB019