

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU113023\
 Data File : VU056643.D
 Acq On : 30 Nov 2023 10:47
 Operator : MD/SY
 Sample : VU1130WBL02
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK089

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU056643.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	107	rVB	124772	144915	15.58%	1.836%
2	1.911	184	193	207	rVB	93485	129490	13.92%	1.640%
3	2.461	355	364	370	rBV	5522	11275	1.21%	0.143%
4	2.564	385	396	409	rBV	200104	324135	34.85%	4.106%
5	3.043	537	545	553	rBV3	13603	22799	2.45%	0.289%
6	4.621	1022	1036	1058	rBV	131867	347987	37.42%	4.408%
7	5.059	1155	1172	1190	rBV	190482	430417	46.28%	5.452%
8	5.721	1359	1378	1397	rBV2	353695	930002	100.00%	11.781%
9	6.245	1527	1541	1563	rBV	331950	659593	70.92%	8.355%
10	6.686	1663	1678	1696	rBV	225471	445145	47.86%	5.639%
11	7.563	1941	1951	1971	rVB2	106169	195385	21.01%	2.475%
12	7.895	2041	2054	2075	rBV	405612	738396	79.40%	9.354%
13	8.177	2130	2142	2153	rBV2	64490	116677	12.55%	1.478%
14	8.631	2270	2283	2311	rBV	468986	912295	98.10%	11.556%
15	9.415	2515	2527	2547	rBV	472239	828256	89.06%	10.492%
16	10.753	2931	2943	2955	rVB	155731	255861	27.51%	3.241%
17	10.891	2976	2986	2993	rVB3	6663	11780	1.27%	0.149%
18	11.808	3258	3271	3290	rVV	455062	746932	80.32%	9.462%
19	12.190	3378	3390	3408	rBV	371400	630872	67.84%	7.992%
20	14.566	4115	4129	4131	rBV	6592	12048	1.30%	0.153%




Sum of corrected areas: 7894260

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU113023\
Data File : VU056643.D
Acq On : 30 Nov 2023 10:47
Operator : MD/SY
Sample : VU1130WBL02
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK089

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

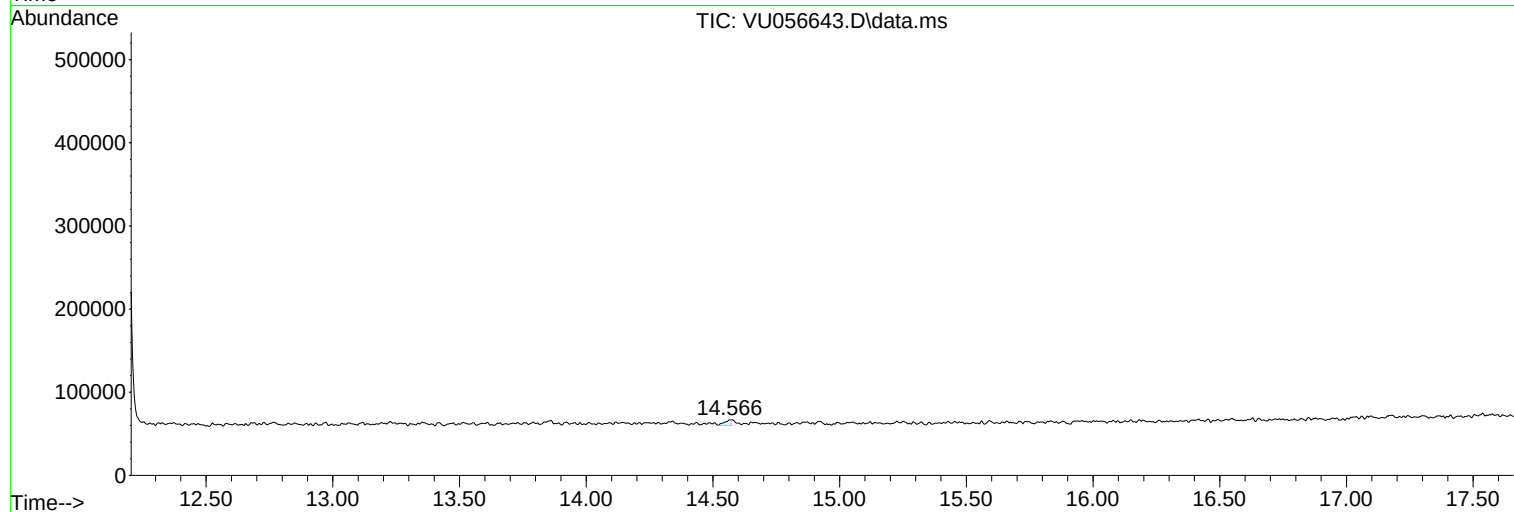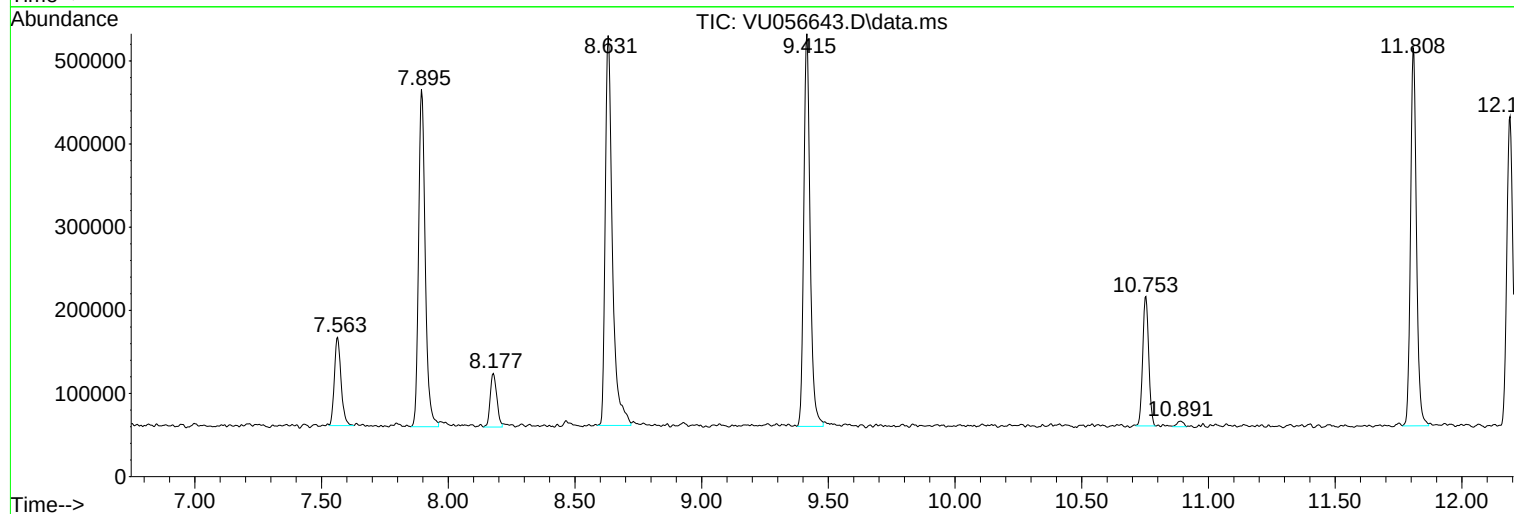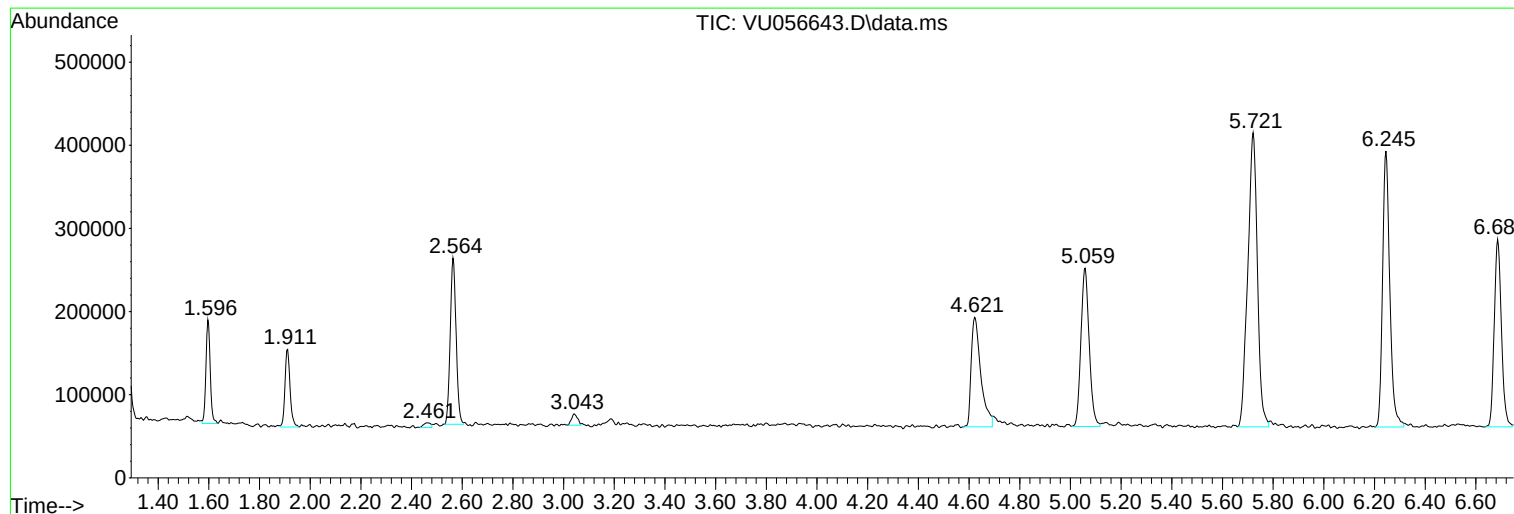

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU113023\
Data File : VU056643.D
Acq On : 30 Nov 2023 10:47
Operator : MD/SY
Sample : VU1130WBL02
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK089

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU113023\
Data File : VU056643.D
Acq On : 30 Nov 2023 10:47
Operator : MD/SY
Sample : VU1130WBL02
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK089

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc