
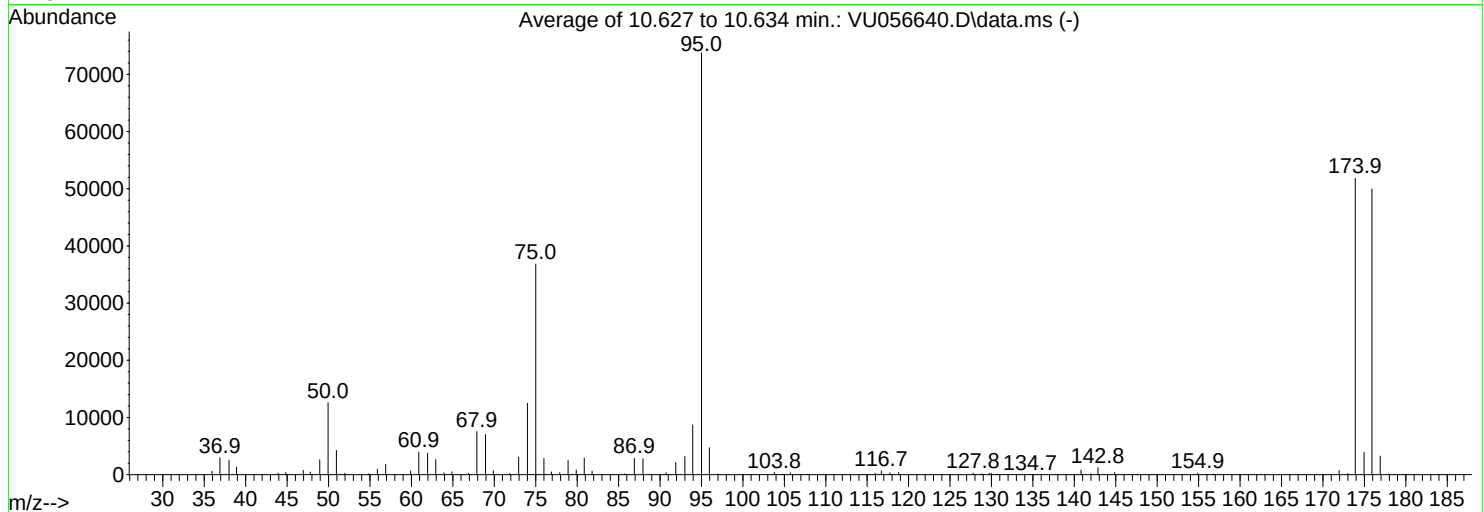


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU113023\
Data File : VU056640.D
Acq On : 30 Nov 2023 09:00
Operator : MD/SY
Sample : BFB085
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB085

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Nov 30 22:25:57 2023

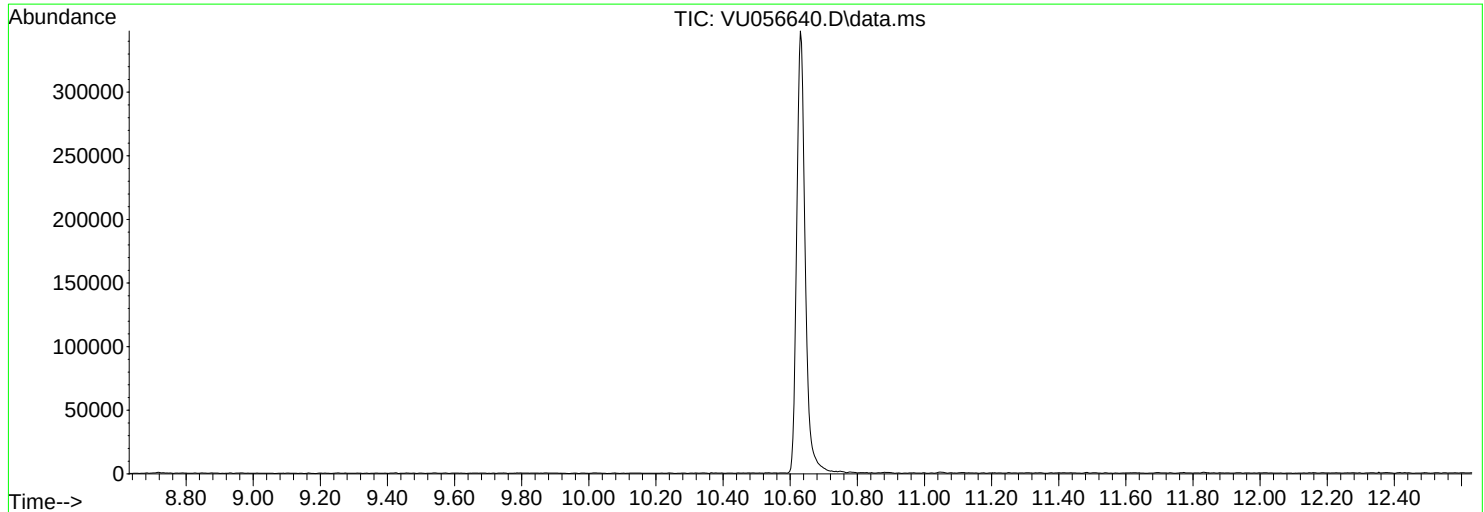

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	12596	PASS
75	95	30	80	49.9	36816	PASS
95	95	100	100	100.0	73765	PASS
96	95	5	9	6.4	4715	PASS
173	174	0.00	2	0.4	187	PASS
174	95	50	120	70.3	51832	PASS
175	174	5	9	7.5	3896	PASS
176	174	95	101	96.4	49989	PASS
177	176	5	9	6.5	3242	PASS

m/z	Abundance
39.90	228.0
43.90	550.0

Instrument :
MSVOA_U
ClientSampleId :
BFB085

m/z	Abundance
36.00	667.0
36.90	2852.0
38.00	2531.0
38.90	1224.0
39.80	218.0
43.90	817.0
44.90	397.0
46.90	709.0
47.80	367.0
48.90	2608.0
50.00	12470.0
51.00	4120.0
52.00	175.0
54.90	153.0
55.90	985.0
56.90	1921.0
59.90	737.0
60.90	3974.0
61.90	3637.0
63.00	2772.0
64.00	319.0
64.90	556.0
66.90	240.0
67.90	7082.0
69.00	6921.0
69.90	656.0
71.90	322.0
73.00	2927.0
74.00	11841.0
75.00	35480.0
76.00	3063.0
76.90	467.0
77.90	295.0
78.90	2633.0
79.90	721.0
80.90	2989.0
81.80	590.0
85.70	139.0
86.90	2839.0
87.90	3137.0
90.80	269.0
91.90	1996.0
93.00	3104.0
94.00	8736.0
95.00	71280.0
95.90	4666.0
97.00	216.0
103.80	382.0
104.80	132.0
105.70	262.0
112.90	129.0
115.90	271.0
116.70	646.0
117.70	325.0
118.80	339.0
127.80	241.0
128.80	138.0
129.70	315.0
130.00	302.0
140.80	764.0
142.00	116.0
142.90	1308.0
144.90	374.0
146.70	109.0
147.10	104.0
154.90	233.0
156.80	219.0
170.90	108.0
172.00	549.0
173.90	49408.0
175.00	3619.0
175.90	47824.0
176.90	3245.0
178.00	121.0

Instrument :
MSVOA_U
ClientSampleId :
BFB085

m/z	Abundance
36.00	592.0
36.90	3074.0
38.00	2605.0
38.90	1418.0
39.70	198.0
43.90	819.0
44.80	386.0
46.90	781.0
47.80	473.0
48.90	2600.0
49.90	12914.0
51.00	4415.0
51.90	244.0
54.90	128.0
55.90	983.0
56.90	1846.0
59.90	684.0
60.90	4088.0
62.00	3947.0
62.90	2718.0
63.90	333.0
64.90	492.0
66.90	213.0
67.90	7743.0
68.90	7149.0
69.90	747.0
71.80	286.0
72.90	3197.0
74.00	12751.0
75.00	37736.0
76.00	2935.0
76.90	476.0
77.90	342.0
78.90	2526.0
79.90	879.0
80.90	3026.0
81.80	653.0
85.70	135.0
86.90	2958.0
87.90	2885.0
90.70	337.0
91.90	2156.0
93.00	3307.0
94.00	8895.0
95.00	76176.0
95.90	4848.0
97.00	178.0
103.80	386.0
104.80	112.0
105.80	321.0
112.90	114.0
116.00	259.0
116.70	659.0
117.70	303.0
118.80	405.0
127.80	310.0
128.80	134.0
130.00	347.0
130.70	103.0
140.80	888.0
141.90	144.0
142.80	1248.0
144.00	121.0
144.80	372.0
147.20	106.0
147.60	112.0
154.90	323.0
156.80	140.0
172.00	731.0
173.90	53216.0
174.90	4025.0
175.90	51376.0
176.90	3386.0
177.90	146.0

Instrument :
MSVOA_U
ClientSampleId :
BFB085

m/z	Abundance
35.90	503.0
36.90	2896.0
38.00	2421.0
38.90	1352.0
39.60	183.0
43.90	800.0
44.90	404.0
47.00	765.0
47.80	494.0
49.00	2580.0
49.90	12405.0
50.90	4225.0
51.90	289.0
54.80	105.0
55.90	866.0
56.90	1594.0
59.90	546.0
60.90	3755.0
62.00	3777.0
62.90	2441.0
63.90	342.0
64.90	461.0
66.90	224.0
67.90	7759.0
68.90	7019.0
69.90	702.0
72.90	3135.0
74.00	12846.0
75.00	37232.0
76.00	2577.0
76.90	452.0
77.90	360.0
78.90	2294.0
79.90	861.0
80.80	2747.0
81.80	607.0
85.80	135.0
86.90	2794.0
88.00	2412.0
90.70	366.0
91.90	2222.0
93.00	3047.0
93.90	8370.0
95.00	73840.0
96.00	4630.0
103.80	387.0
105.80	370.0
107.80	138.0
116.00	213.0
116.70	618.0
117.80	358.0
118.80	401.0
127.80	290.0
128.90	111.0
129.80	361.0
130.80	125.0
134.70	112.0
136.60	106.0
140.80	823.0
141.90	156.0
142.90	1084.0
144.00	139.0
144.80	320.0
147.60	122.0
154.90	304.0
171.90	874.0
173.00	561.0
173.90	52872.0
174.90	4044.0
175.90	50768.0
176.90	3096.0
177.90	151.0

Instrument :
MSVOA_U
ClientSampleId :
BFB085