

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120121\
 Data File : VU046035.D
 Acq On : 01 Dec 2021 11:04
 Operator : SY/MD
 Sample : VU1201WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK042

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046035.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	95	rVB	98486	110879	14.86%	1.896%
2	1.919	171	180	194	rBV	75166	96910	12.99%	1.657%
3	2.144	248	250	253	rBV	280	184	0.02%	0.003%
4	2.202	266	268	270	rVB	283	113	0.02%	0.002%
5	2.391	323	327	333	rBV	171	235	0.03%	0.004%
6	2.517	362	366	370	rVB3	378	348	0.05%	0.006%
7	2.571	370	383	416	rBV	158888	269258	36.08%	4.603%
8	2.716	426	428	433	rVB2	278	184	0.02%	0.003%
9	2.793	447	452	454	rBV	438	335	0.04%	0.006%
10	2.877	473	478	481	rBB	145	165	0.02%	0.003%
11	3.044	526	530	531	rBV2	966	704	0.09%	0.012%
12	3.215	581	583	586	rBV	150	118	0.02%	0.002%
13	3.260	592	597	599	rBB	168	138	0.02%	0.002%
14	3.472	660	663	666	rBB	132	114	0.02%	0.002%
15	3.514	673	676	679	rBB	129	112	0.02%	0.002%
16	3.623	706	710	713	rBV	132	157	0.02%	0.003%
17	3.887	789	792	795	rBV	147	145	0.02%	0.002%
18	3.957	812	814	819	rBB	146	144	0.02%	0.002%
19	4.359	935	939	941	rBB	153	125	0.02%	0.002%
20	4.645	1011	1028	1063	rBV2	56834	196307	26.31%	3.356%
21	4.835	1084	1087	1091	rVB	402	269	0.04%	0.005%
22	4.854	1091	1093	1096	rVV2	293	148	0.02%	0.003%
23	4.880	1097	1101	1105	rVB2	215	189	0.03%	0.003%
24	4.906	1105	1109	1110	rBV	169	129	0.02%	0.002%
25	5.067	1142	1159	1181	rBV	128162	292017	39.13%	4.992%
26	5.163	1185	1189	1194	rVB3	318	285	0.04%	0.005%
27	5.186	1194	1196	1199	rBV2	253	191	0.03%	0.003%
28	5.729	1343	1365	1390	rBV2	276627	746220	100.00%	12.758%
29	5.957	1433	1436	1438	rBV2	181	150	0.02%	0.003%
30	6.041	1460	1462	1465	rBV	170	141	0.02%	0.002%
31	6.115	1482	1485	1488	rBV2	218	155	0.02%	0.003%
32	6.253	1513	1528	1546	rBV	232378	437825	58.67%	7.485%
33	6.346	1555	1557	1567	rVB2	766	768	0.10%	0.013%
34	6.488	1598	1601	1605	rBB	254	172	0.02%	0.003%
35	6.536	1606	1616	1631	rBV3	5825	13538	1.81%	0.231%
36	6.694	1651	1665	1685	rBV	172506	332990	44.62%	5.693%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120121\
 Data File : VU046035.D
 Acq On : 01 Dec 2021 11:04
 Operator : SY/MD
 Sample : VU1201WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK042

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	6.803	1696	1699	1703	rBV2	443	443	0.06%	0.008%
38	6.903	1728	1730	1734	rBB	151	123	0.02%	0.002%
39	7.041	1770	1773	1774	rBV2	221	157	0.02%	0.003%
40	7.108	1791	1794	1798	rBV	166	187	0.03%	0.003%
41	7.182	1810	1817	1828	rBB2	1410	2254	0.30%	0.039%
42	7.237	1831	1834	1838	rBB	164	156	0.02%	0.003%
43	7.433	1892	1895	1898	rBB	135	114	0.02%	0.002%
44	7.488	1909	1912	1915	rBB	158	124	0.02%	0.002%
45	7.568	1922	1937	1956	rBV	93124	162195	21.74%	2.773%
46	7.652	1960	1963	1967	rVV	265	244	0.03%	0.004%
47	7.687	1967	1974	1983	rVB5	959	1367	0.18%	0.023%
48	7.835	2017	2020	2022	rBV	137	116	0.02%	0.002%
49	7.899	2027	2040	2058	rBV	345489	606960	81.34%	10.377%
50	8.179	2116	2127	2142	rVV	64548	107423	14.40%	1.837%
51	8.401	2194	2196	2201	rBB	137	140	0.02%	0.002%
52	8.574	2247	2250	2253	rVB	178	143	0.02%	0.002%
53	8.636	2256	2269	2302	rBV	212130	397723	53.30%	6.800%
54	8.790	2313	2317	2321	rVB	164	188	0.03%	0.003%
55	8.812	2321	2324	2327	rBV	152	145	0.02%	0.002%
56	8.835	2327	2331	2337	rVB	207	266	0.04%	0.005%
57	8.867	2337	2341	2347	rBB	143	201	0.03%	0.003%
58	8.899	2348	2351	2353	rBV	170	145	0.02%	0.002%
59	8.986	2374	2378	2381	rBV	145	177	0.02%	0.003%
60	9.147	2425	2428	2430	rBV	156	128	0.02%	0.002%
61	9.163	2430	2433	2436	rVV	233	140	0.02%	0.002%
62	9.230	2451	2454	2459	rVB	213	227	0.03%	0.004%
63	9.256	2459	2462	2464	rBV	161	131	0.02%	0.002%
64	9.420	2500	2513	2543	rBV	334936	556944	74.64%	9.522%
65	9.523	2543	2545	2548	rVB	271	128	0.02%	0.002%
66	9.571	2556	2560	2565	rBV	241	288	0.04%	0.005%
67	9.690	2593	2597	2607	rVB3	688	961	0.13%	0.016%
68	9.735	2608	2611	2614	rBV	146	149	0.02%	0.003%
69	9.767	2617	2621	2623	rBV	136	125	0.02%	0.002%
70	9.867	2649	2652	2655	rBV	138	147	0.02%	0.003%
71	10.497	2844	2848	2851	rVB2	159	119	0.02%	0.002%
72	10.565	2866	2869	2872	rBV	155	161	0.02%	0.003%
73	10.635	2888	2891	2896	rVB	297	266	0.04%	0.005%
74	10.677	2896	2904	2911	rBV3	1769	2528	0.34%	0.043%
75	10.758	2916	2929	2949	rVV	240264	385707	51.69%	6.594%
76	11.089	3029	3032	3034	rBV2	195	124	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120121\
 Data File : VU046035.D
 Acq On : 01 Dec 2021 11:04
 Operator : SY/MD
 Sample : VU1201WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK042

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.459	3139	3147	3148	rBV3	890	945	0.13%	0.016%
78	11.520	3163	3166	3172	rVB	155	125	0.02%	0.002%
79	11.639	3200	3203	3207	rBV	101	116	0.02%	0.002%
80	11.697	3213	3221	3225	rBV3	619	811	0.11%	0.014%
81	11.748	3233	3237	3244	rVB	463	454	0.06%	0.008%
82	11.812	3244	3257	3277	rBV	351340	548226	73.47%	9.373%
83	11.944	3291	3298	3301	rBV2	517	608	0.08%	0.010%
84	11.973	3302	3307	3315	rVB4	901	1100	0.15%	0.019%
85	12.195	3363	3376	3392	rBV	344852	559852	75.03%	9.571%
86	13.224	3691	3696	3702	rBV2	499	682	0.09%	0.012%
87	13.709	3844	3847	3857	rVB	150	177	0.02%	0.003%
88	13.844	3884	3889	3894	rVB2	730	735	0.10%	0.013%
89	13.870	3894	3897	3901	rBV	142	116	0.02%	0.002%
90	14.095	3956	3967	3975	rBV	887	1653	0.22%	0.028%
91	14.301	4028	4031	4036	rBV	133	152	0.02%	0.003%
92	14.336	4036	4042	4047	rVV2	805	814	0.11%	0.014%
93	14.532	4101	4103	4111	rVB	254	205	0.03%	0.004%
94	14.571	4111	4115	4119	rBV	154	149	0.02%	0.003%
95	14.889	4211	4214	4219	rBV	207	129	0.02%	0.002%
96	15.172	4298	4302	4305	rBV2	252	245	0.03%	0.004%
97	15.336	4349	4353	4356	rBV2	243	234	0.03%	0.004%
98	15.545	4415	4418	4420	rBV2	209	136	0.02%	0.002%
99	15.606	4435	4437	4441	rBV	332	240	0.03%	0.004%
100	16.767	4795	4798	4800	rBV2	378	183	0.02%	0.003%




Sum of corrected areas: 5849213

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120121\
Data File : VU046035.D
Acq On : 01 Dec 2021 11:04
Operator : SY/MD
Sample : VU1201WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK042

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

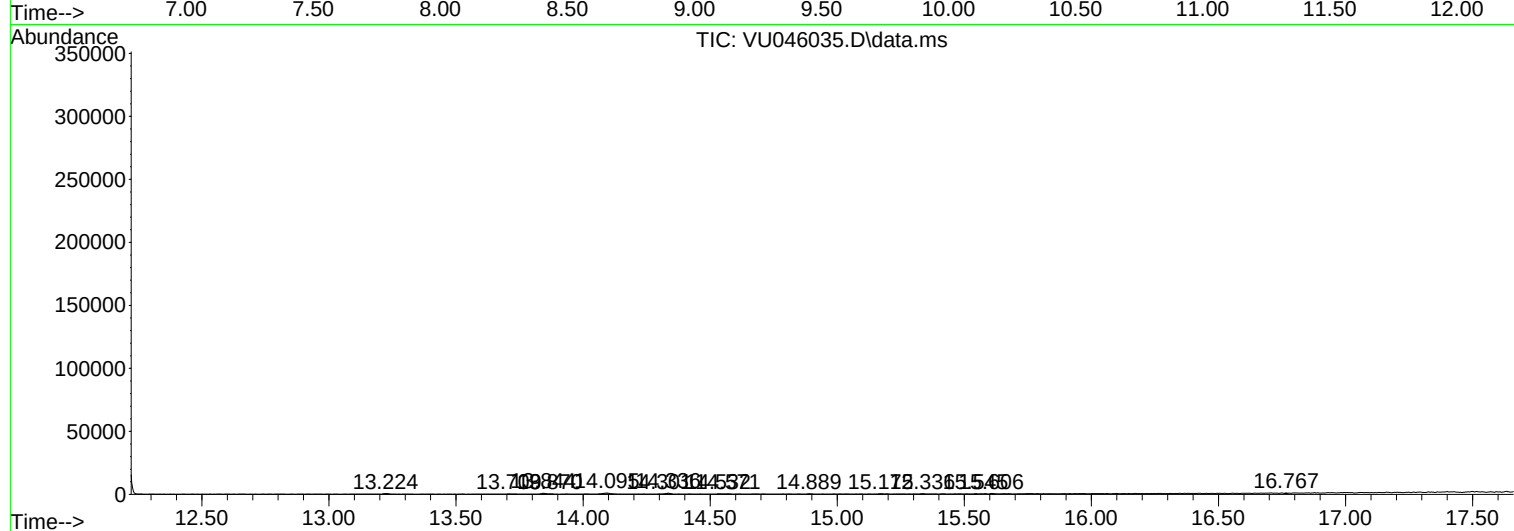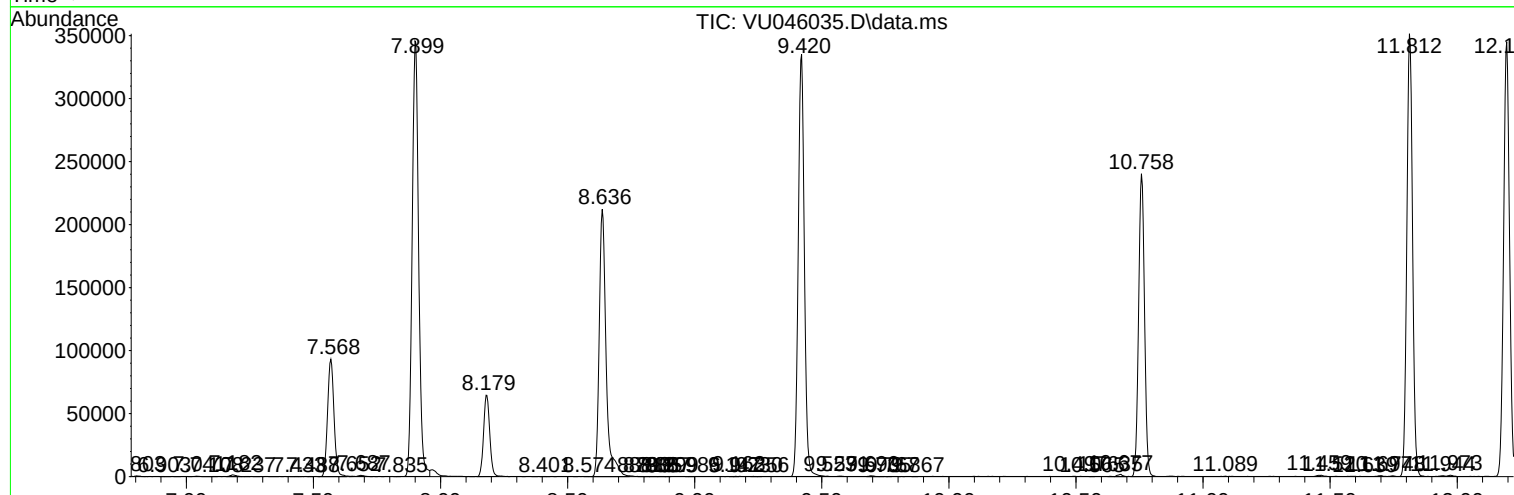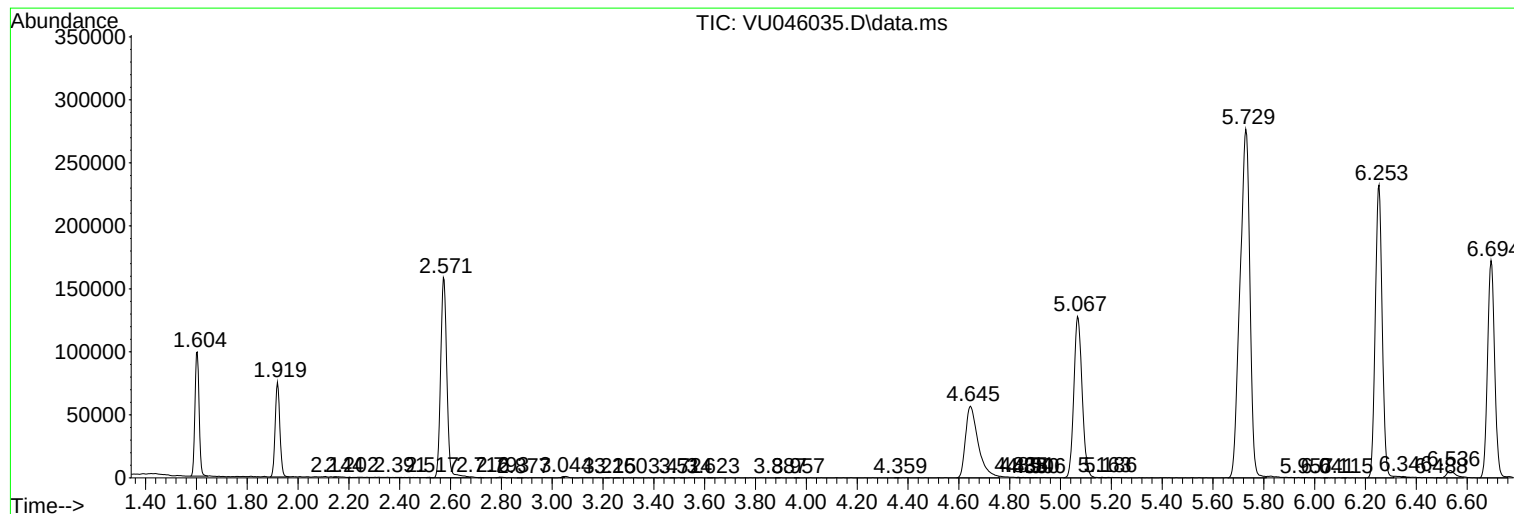

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120121\
Data File : VU046035.D
Acq On : 01 Dec 2021 11:04
Operator : SY/MD
Sample : VU1201WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK042

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120121\
Data File : VU046035.D
Acq On : 01 Dec 2021 11:04
Operator : SY/MD
Sample : VU1201WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK042

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------