

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120121\
 Data File : VU046038.D
 Acq On : 01 Dec 2021 16:49
 Operator : SY/MD
 Sample : M4878-01 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0G20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046038.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.363	3	7	17	rVB	22235	20608	2.77%	0.340%
2	1.601	74	81	93	rBV	96661	106903	14.36%	1.766%
3	1.919	170	180	192	rBV	75523	96397	12.95%	1.592%
4	2.002	201	206	210	rBV3	723	710	0.10%	0.012%
5	2.205	265	269	275	rVB2	534	532	0.07%	0.009%
6	2.427	336	338	344	rVB2	295	231	0.03%	0.004%
7	2.572	371	383	403	rBV	155080	256129	34.40%	4.231%
8	2.800	450	454	459	rVB2	198	195	0.03%	0.003%
9	2.967	501	506	508	rBB2	296	236	0.03%	0.004%
10	2.983	508	511	515	rBV	141	171	0.02%	0.003%
11	3.044	526	530	531	rBV	587	352	0.05%	0.006%
12	3.089	539	544	553	rVB4	644	734	0.10%	0.012%
13	3.189	564	575	587	rVB2	1914	3754	0.50%	0.062%
14	3.356	625	627	628	rBV	441	205	0.03%	0.003%
15	3.700	730	734	737	rBV2	587	581	0.08%	0.010%
16	4.539	992	995	1003	rVB2	495	640	0.09%	0.011%
17	4.642	1011	1027	1059	rBV	60736	204592	27.48%	3.379%
18	5.070	1144	1160	1184	rVV	126782	289799	38.92%	4.787%
19	5.227	1205	1209	1211	rBV2	285	222	0.03%	0.004%
20	5.292	1227	1229	1232	rVB	224	146	0.02%	0.002%
21	5.388	1253	1259	1267	rBV4	748	1316	0.18%	0.022%
22	5.729	1343	1365	1396	rBV2	274194	744633	100.00%	12.299%
23	5.861	1404	1406	1410	rVB2	298	177	0.02%	0.003%
24	5.925	1423	1426	1433	rVV2	323	334	0.04%	0.006%
25	5.970	1437	1440	1441	rVB	322	156	0.02%	0.003%
26	6.253	1513	1528	1545	rBV	252920	478076	64.20%	7.897%
27	6.542	1606	1618	1632	rBV5	8848	20556	2.76%	0.340%
28	6.697	1651	1666	1681	rBV	169304	326916	43.90%	5.400%
29	6.806	1698	1700	1702	rBV	424	199	0.03%	0.003%
30	6.922	1733	1736	1739	rBB	206	164	0.02%	0.003%
31	7.054	1770	1777	1781	rBB	360	428	0.06%	0.007%
32	7.124	1796	1799	1803	rBB	196	171	0.02%	0.003%
33	7.186	1809	1818	1827	rBB3	1839	2552	0.34%	0.042%
34	7.507	1915	1918	1921	rBV	249	182	0.02%	0.003%
35	7.568	1925	1937	1956	rBV	92427	160541	21.56%	2.652%
36	7.690	1969	1975	1984	rVB4	1026	1649	0.22%	0.027%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120121\
 Data File : VU046038.D
 Acq On : 01 Dec 2021 16:49
 Operator : SY/MD
 Sample : M4878-01 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0G20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.796	2001	2008	2010	rBV	164	236	0.03%	0.004%
38	7.903	2026	2041	2057	rBV	339986	596664	80.13%	9.855%
39	8.057	2085	2089	2094	rVB2	315	420	0.06%	0.007%
40	8.137	2111	2114	2117	rVB2	374	228	0.03%	0.004%
41	8.182	2117	2128	2147	rBV	64373	106894	14.36%	1.766%
42	8.253	2148	2150	2152	rVV	307	161	0.02%	0.003%
43	8.288	2158	2161	2166	rVB2	325	328	0.04%	0.005%
44	8.337	2170	2176	2179	rBB	160	204	0.03%	0.003%
45	8.478	2215	2220	2223	rVV2	390	402	0.05%	0.007%
46	8.555	2235	2244	2255	rVB3	15679	26135	3.51%	0.432%
47	8.636	2257	2269	2302	rBV	203091	379426	50.95%	6.267%
48	8.915	2350	2356	2364	rBV2	927	1584	0.21%	0.026%
49	9.070	2400	2404	2409	rBV	170	259	0.03%	0.004%
50	9.166	2430	2434	2438	rBB	178	195	0.03%	0.003%
51	9.214	2444	2449	2451	rBV2	345	311	0.04%	0.005%
52	9.340	2482	2488	2495	rVB	465	734	0.10%	0.012%
53	9.420	2500	2513	2537	rBV	361757	610176	81.94%	10.079%
54	9.571	2554	2560	2572	rBV3	1310	2056	0.28%	0.034%
55	9.693	2590	2598	2609	rVB	3268	4873	0.65%	0.080%
56	9.745	2609	2614	2619	rBV3	473	448	0.06%	0.007%
57	9.832	2638	2641	2646	rBV	169	199	0.03%	0.003%
58	10.105	2720	2726	2731	rBV3	469	568	0.08%	0.009%
59	10.163	2741	2744	2750	rBV	190	247	0.03%	0.004%
60	10.256	2768	2773	2776	rBV2	279	311	0.04%	0.005%
61	10.430	2822	2827	2829	rBV	198	214	0.03%	0.004%
62	10.484	2840	2844	2849	rBV	188	228	0.03%	0.004%
63	10.636	2886	2891	2894	rBV2	272	186	0.02%	0.003%
64	10.652	2894	2896	2897	rVV2	361	190	0.03%	0.003%
65	10.674	2897	2903	2909	rVV2	1890	2717	0.36%	0.045%
66	10.761	2917	2930	2947	rVB	231303	377144	50.65%	6.229%
67	10.867	2961	2963	2968	rVB2	270	221	0.03%	0.004%
68	10.906	2968	2975	2984	rVB5	1185	1726	0.23%	0.029%
69	10.999	2996	3004	3010	rBV3	2857	4089	0.55%	0.068%
70	11.095	3023	3034	3037	rBV	1341	2017	0.27%	0.033%
71	11.211	3067	3070	3073	rVB	317	224	0.03%	0.004%
72	11.230	3073	3076	3078	rBV	183	151	0.02%	0.002%
73	11.298	3088	3097	3106	rBV	1623	2268	0.30%	0.037%
74	11.472	3140	3151	3160	rBV2	9127	13590	1.83%	0.224%
75	11.574	3180	3183	3188	rBV2	178	182	0.02%	0.003%
76	11.693	3214	3220	3227	rVB4	817	842	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120121\
 Data File : VU046038.D
 Acq On : 01 Dec 2021 16:49
 Operator : SY/MD
 Sample : M4878-01 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0G20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.816	3245	3258	3273	rBV	382421	610031	81.92%	10.076%
78	11.870	3273	3275	3278	rVV3	613	414	0.06%	0.007%
79	11.896	3278	3283	3293	rVV2	1762	2459	0.33%	0.041%
80	11.951	3297	3300	3302	rVV2	486	404	0.05%	0.007%
81	11.976	3303	3308	3315	rVV2	1305	1637	0.22%	0.027%
82	12.009	3316	3318	3328	rVB2	241	208	0.03%	0.003%
83	12.099	3339	3346	3351	rBV3	1044	1314	0.18%	0.022%
84	12.127	3351	3355	3361	rVB	417	496	0.07%	0.008%
85	12.195	3361	3376	3394	rBV	352568	566303	76.05%	9.354%
86	12.333	3411	3419	3426	rVB3	1057	1438	0.19%	0.024%
87	12.375	3427	3432	3437	rVB2	263	329	0.04%	0.005%
88	12.404	3437	3441	3444	rBV2	282	191	0.03%	0.003%
89	12.468	3456	3461	3465	rBV2	380	490	0.07%	0.008%
90	12.574	3487	3494	3502	rVV2	788	1082	0.15%	0.018%
91	12.635	3510	3513	3518	rVB2	212	200	0.03%	0.003%
92	12.681	3521	3527	3539	rVV3	1012	1456	0.20%	0.024%
93	12.976	3613	3619	3624	rBV3	467	571	0.08%	0.009%
94	13.028	3629	3635	3641	rVB2	738	883	0.12%	0.015%
95	13.291	3713	3717	3725	rVB2	285	411	0.06%	0.007%
96	13.436	3755	3762	3763	rBV2	549	509	0.07%	0.008%
97	13.459	3764	3769	3776	rVB3	1195	1392	0.19%	0.023%
98	13.944	3916	3920	3924	rBV2	251	270	0.04%	0.004%
99	14.089	3957	3965	3974	rVB2	826	1334	0.18%	0.022%
100	14.944	4229	4231	4236	rVB2	211	150	0.02%	0.002%




Sum of corrected areas: 6054207

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120121\
Data File : VU046038.D
Acq On : 01 Dec 2021 16:49
Operator : SY/MD
Sample : M4878-01 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0G20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

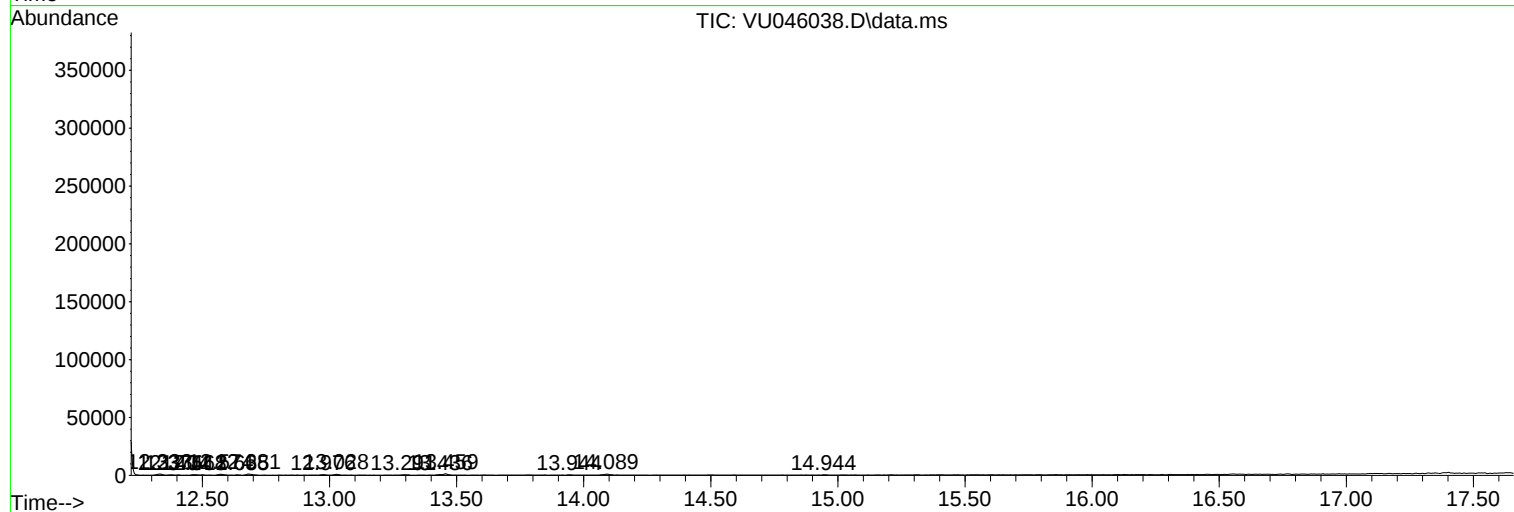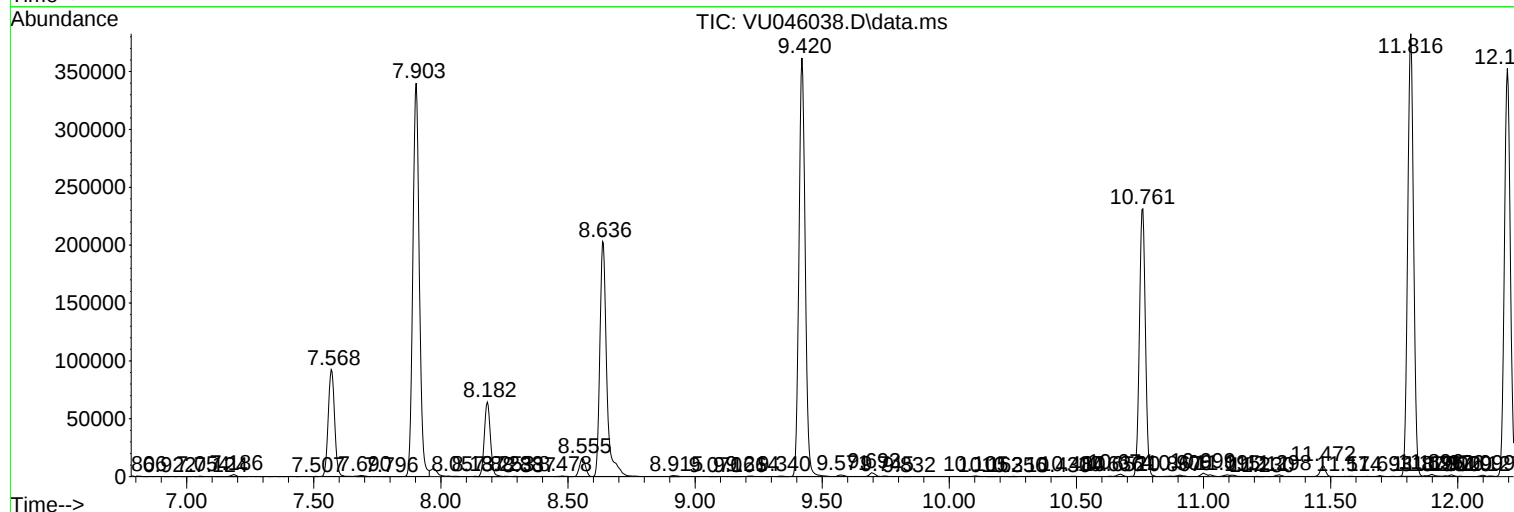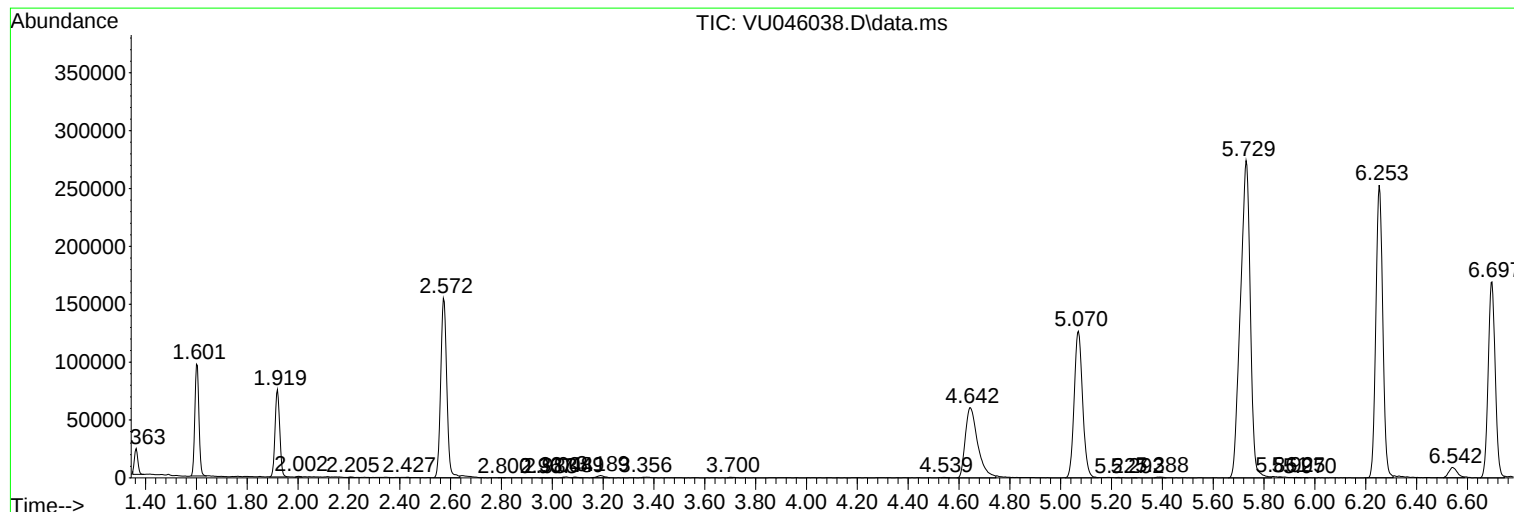

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120121\
Data File : VU046038.D
Acq On : 01 Dec 2021 16:49
Operator : SY/MD
Sample : M4878-01 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0G20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120121\
Data File : VU046038.D
Acq On : 01 Dec 2021 16:49
Operator : SY/MD
Sample : M4878-01 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0G20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc