

m/z	Abundance
43.90	161.0

Instrument :
MSVOA_U
ClientSampleId :
BFB020

m/z	Abundance
36.00	183.0
37.00	1044.0
38.00	1060.0
39.00	440.0
44.00	260.0
44.90	191.0
47.00	289.0
48.10	141.0
49.00	1116.0
50.00	4570.0
51.00	1435.0
56.00	394.0
57.00	674.0
59.90	276.0
61.00	1381.0
62.00	1236.0
63.00	1172.0
64.00	151.0
65.00	188.0
68.00	2638.0
69.00	2706.0
70.00	259.0
71.90	166.0
73.00	1306.0
74.00	4998.0
75.00	13801.0
76.00	1227.0
76.90	143.0
78.10	152.0
78.90	1015.0
79.90	314.0
80.90	917.0
81.90	219.0
87.00	1114.0
88.00	1104.0
90.90	148.0
91.90	755.0
93.00	1164.0
94.00	3125.0
95.00	27136.0
96.00	1801.0
103.90	127.0
105.90	102.0
116.90	221.0
119.00	168.0
127.90	112.0
140.90	254.0
143.00	360.0
172.00	325.0
173.10	204.0
174.00	20808.0
175.00	1623.0
176.00	19880.0
177.00	1318.0

Instrument :
MSVOA_U
ClientSampleId :
BFB020

m/z	Abundance
36.00	172.0
37.00	976.0
38.00	897.0
39.00	429.0
44.00	252.0
44.90	145.0
47.00	310.0
49.00	941.0
50.00	4523.0
51.00	1502.0
56.00	387.0
57.00	823.0
59.90	261.0
61.00	1246.0
62.00	1286.0
63.00	1080.0
64.00	167.0
65.00	220.0
68.00	2754.0
69.00	2652.0
70.00	251.0
71.90	155.0
73.00	1220.0
74.00	4767.0
75.00	13810.0
76.00	1301.0
76.90	121.0
77.90	139.0
78.90	1086.0
79.90	285.0
80.90	850.0
81.90	218.0
86.90	1149.0
88.00	1065.0
92.00	763.0
93.00	1171.0
94.00	3286.0
95.00	26768.0
96.00	1793.0
96.90	112.0
103.80	118.0
116.90	226.0
117.90	123.0
119.00	138.0
127.90	110.0
140.90	297.0
143.00	376.0
172.00	378.0
173.00	225.0
174.00	21616.0
175.00	1554.0
176.00	20704.0
177.00	1360.0

Instrument :
MSVOA_U
ClientSampleId :
BFB020

m/z	Abundance
36.00	183.0
37.00	1060.0
38.00	1023.0
39.00	447.0
44.00	270.0
44.90	156.0
47.00	323.0
48.10	112.0
49.00	1116.0
50.00	4812.0
51.00	1538.0
56.00	405.0
57.00	789.0
59.90	282.0
61.00	1364.0
62.00	1310.0
63.00	1181.0
64.00	169.0
64.90	201.0
68.00	2872.0
69.00	2864.0
70.00	291.0
71.90	163.0
73.00	1289.0
74.00	5153.0
75.00	14466.0
76.00	1311.0
76.90	124.0
78.00	147.0
78.90	1086.0
79.90	321.0
80.90	895.0
81.90	233.0
87.00	1161.0
88.00	1181.0
90.90	117.0
92.00	782.0
93.00	1227.0
94.00	3333.0
95.00	28280.0
96.00	1874.0
103.90	121.0
116.90	229.0
117.90	114.0
119.00	156.0
127.90	116.0
140.90	285.0
143.00	383.0
172.00	393.0
173.00	223.0
174.00	22112.0
175.00	1686.0
176.00	21464.0
177.00	1420.0



Instrument :
MSVOA_U
ClientSampleId :
BFB020

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120121\
 Data File : VU046032.D
 Acq On : 01 Dec 2021 09:29
 Operator : SY/MD
 Sample : BFB020
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB020

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis
 Last Update : Fri Dec 03 05:08:36 2021

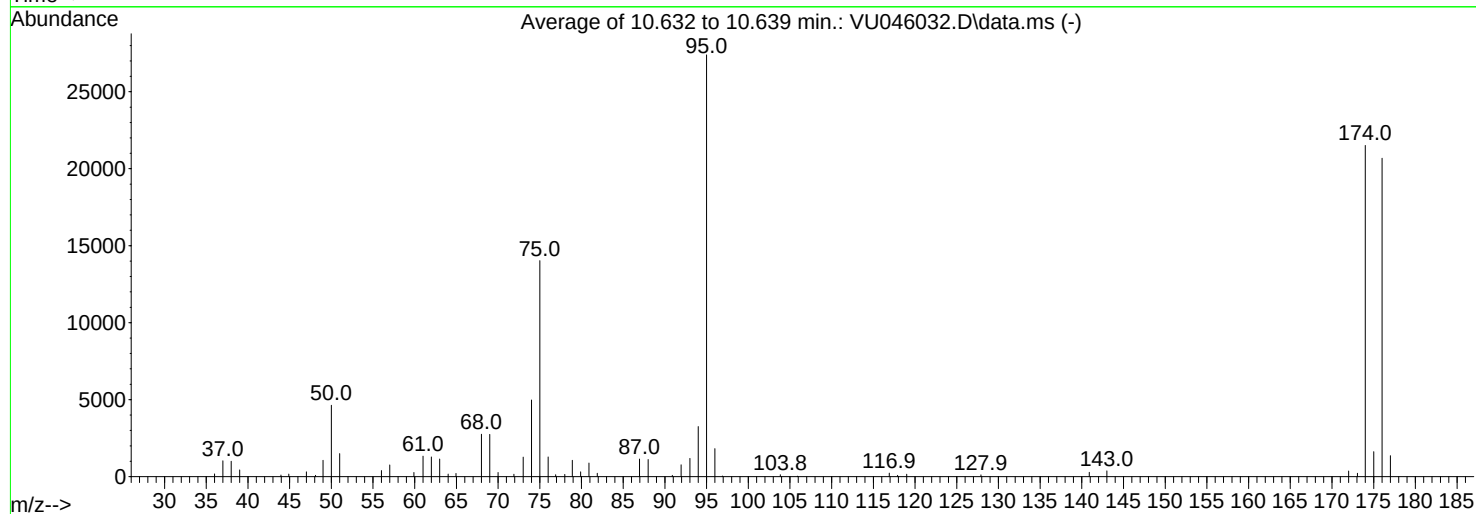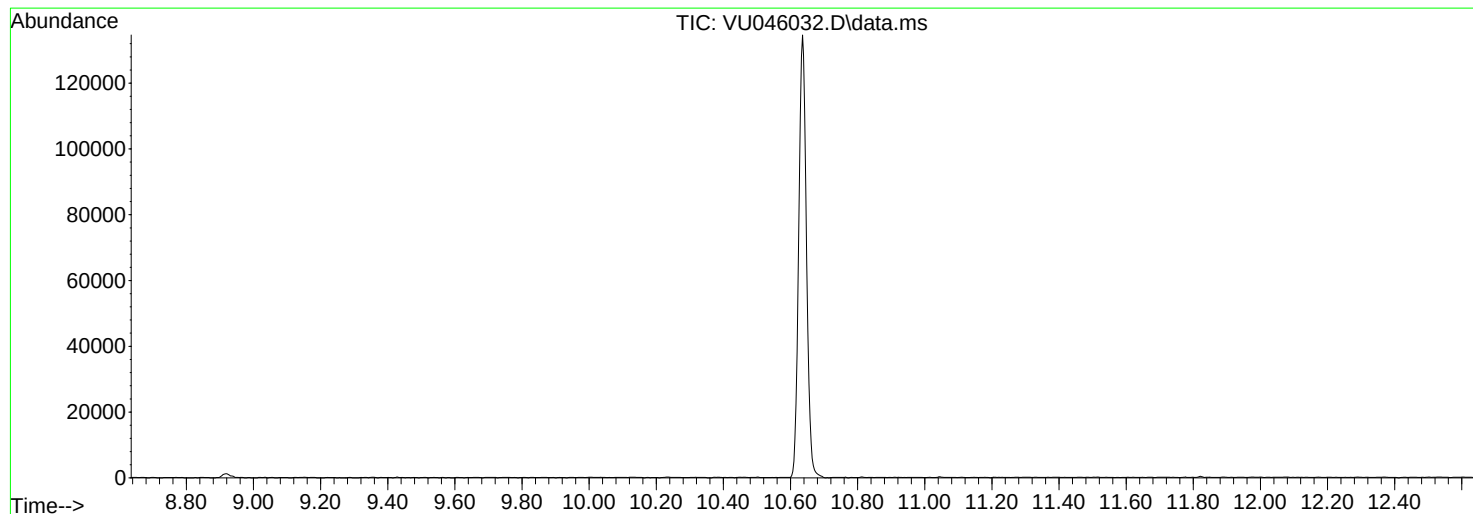

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	4635	PASS
75	95	30	80	51.2	14026	PASS
95	95	100	100	100.0	27395	PASS
96	95	5	9	6.7	1823	PASS
173	174	0.00	2	1.0	217	PASS
174	95	50	120	78.5	21512	PASS
175	174	5	9	7.5	1621	PASS
176	174	95	101	96.1	20683	PASS
177	176	5	9	6.6	1366	PASS