
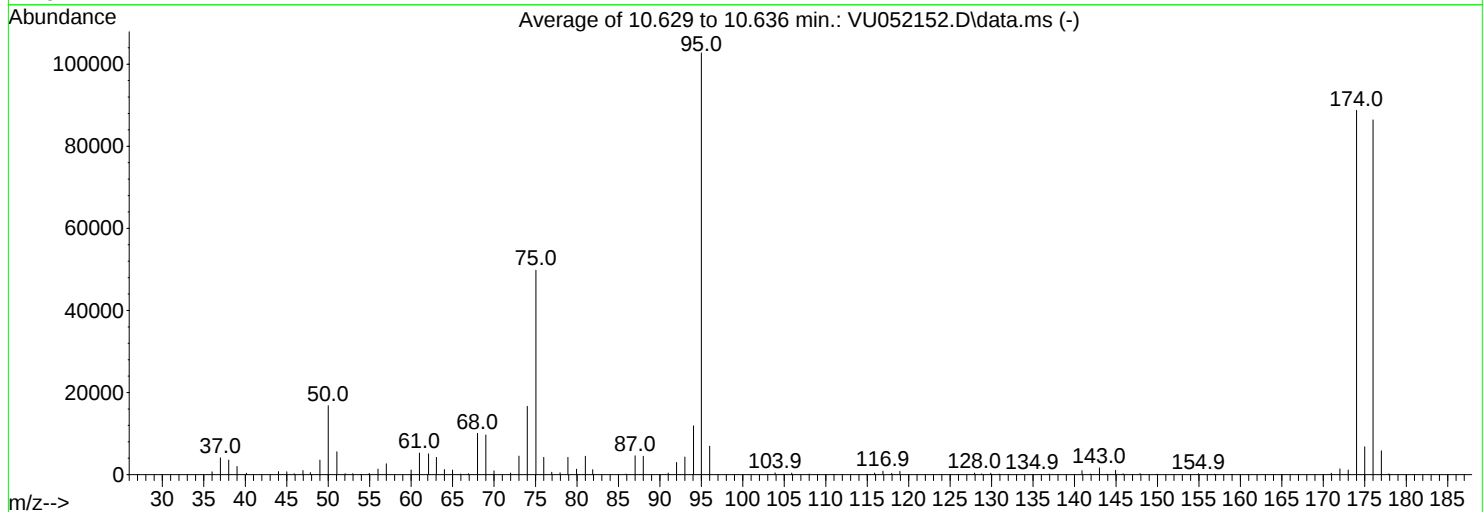


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120122\
Data File : VU052152.D
Acq On : 01 Dec 2022 09:31
Operator : JC/MD
Sample : BFB007
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB007

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
Title : TRACE VOA SOM01.0
Last Update : Fri Dec 02 00:27:38 2022

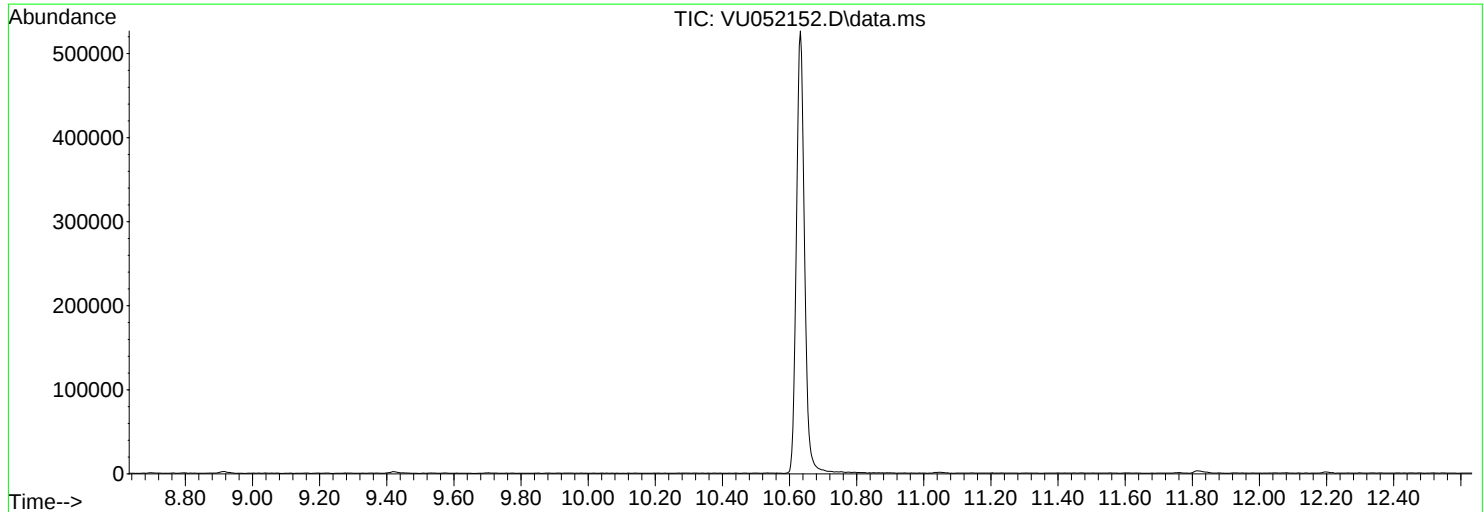

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	16791	PASS
75	95	30	80	48.5	49813	PASS
95	95	100	100	100.0	102768	PASS
96	95	5	9	6.8	6950	PASS
173	174	0.00	2	1.3	1131	PASS
174	95	50	120	86.4	88752	PASS
175	174	5	9	7.7	6796	PASS
176	174	95	101	97.4	86408	PASS
177	176	5	9	6.7	5822	PASS

m/z	Abundance
39.90	166.0
44.00	469.0

Instrument :
MSVOA_U
ClientSampleId :
BFB007

m/z	Abundance
36.00	800.0
37.00	4123.0
38.00	3594.0
39.00	1920.0
40.20	327.0
44.00	1131.0
45.00	735.0
45.90	256.0
47.00	1091.0
47.80	529.0
49.00	3514.0
50.00	16872.0
51.10	5626.0
52.10	312.0
52.90	254.0
53.90	101.0
54.90	299.0
56.00	1526.0
57.00	2692.0
60.00	1145.0
61.00	5450.0
62.10	5125.0
63.00	4064.0
64.00	1366.0
65.00	1089.0
66.00	157.0
66.90	223.0
68.00	10135.0
69.00	9729.0
70.00	938.0
72.00	398.0
73.00	4711.0
74.00	16592.0
75.00	49992.0
76.00	4276.0
76.90	576.0
78.00	466.0
78.90	4340.0
80.00	1313.0
81.00	4519.0
81.90	1166.0
85.90	161.0
87.00	4775.0
88.00	4547.0
91.00	369.0
92.00	2934.0
93.00	4420.0
94.00	12082.0
95.00	103544.0
96.00	7242.0
103.90	451.0
104.90	122.0
105.90	443.0
108.00	196.0
111.00	133.0
114.90	103.0
115.90	398.0
116.90	831.0
118.00	333.0
119.00	776.0
128.00	434.0
128.80	198.0
129.90	353.0
130.90	162.0
134.90	171.0
136.90	117.0
140.90	1003.0
141.80	137.0
143.00	1660.0
143.90	118.0
145.00	1099.0
145.80	230.0
147.80	279.0
150.00	109.0
154.90	185.0
156.90	123.0
159.00	143.0
170.90	355.0
172.00	1263.0
173.00	1129.0
174.00	86176.0
175.00	6671.0
176.00	83992.0
177.00	5594.0
177.90	235.0

Instrument :
MSVOA_U
ClientSampleId :
BFB007

m/z	Abundance
36.00	720.0
37.00	4249.0
38.00	3717.0
39.00	2085.0
40.10	352.0
44.00	1212.0
45.00	741.0
45.90	231.0
46.90	1092.0
47.90	529.0
49.00	3635.0
50.00	17240.0
51.10	5722.0
52.10	244.0
53.00	247.0
55.00	324.0
56.00	1396.0
57.00	2747.0
60.00	1179.0
61.00	5459.0
62.10	5236.0
63.00	4308.0
64.00	1340.0
65.00	1189.0
65.90	156.0
66.90	269.0
68.00	10313.0
69.00	9962.0
70.00	975.0
72.00	409.0
73.00	4659.0
74.00	17088.0
75.00	51160.0
76.00	4383.0
76.90	587.0
78.00	466.0
78.90	4400.0
80.00	1341.0
81.00	4602.0
81.90	1238.0
85.90	155.0
87.00	4730.0
88.00	4643.0
91.00	401.0
92.00	3044.0
93.00	4347.0
94.10	12240.0
95.00	105768.0
96.00	7147.0
103.90	420.0
105.00	141.0
105.90	391.0
108.00	167.0
111.00	121.0
115.90	402.0
116.90	887.0
117.90	344.0
118.90	866.0
128.00	403.0
128.80	237.0
129.90	359.0
130.90	163.0
134.90	121.0
136.90	149.0
140.90	989.0
141.90	163.0
143.00	1649.0
143.90	100.0
145.00	1073.0
145.80	221.0
147.90	280.0
149.90	102.0
154.90	229.0
156.90	112.0
159.00	106.0
160.90	101.0
171.00	365.0
172.00	1453.0
173.00	1142.0
174.00	91408.0
175.00	7021.0
176.00	89264.0
177.00	6024.0
177.90	209.0

Instrument :
MSVOA_U
ClientSampleId :
BFB007

m/z	Abundance
36.00	612.0
37.00	3957.0
38.00	3352.0
39.00	1947.0
40.10	380.0
44.00	1239.0
45.00	647.0
45.90	179.0
47.00	909.0
47.90	489.0
49.00	3473.0
50.00	16260.0
51.00	5365.0
51.90	193.0
53.00	197.0
55.00	331.0
56.00	1167.0
57.00	2565.0
60.00	1086.0
61.00	4917.0
62.10	4873.0
63.10	4235.0
64.00	1106.0
65.00	1132.0
65.90	170.0
66.90	263.0
68.00	9687.0
69.00	9346.0
70.00	884.0
72.00	407.0
73.00	4250.0
74.00	16233.0
75.10	48288.0
76.00	4034.0
77.00	616.0
77.90	444.0
78.90	3937.0
79.90	1310.0
81.00	4353.0
81.90	1217.0
85.90	138.0
87.00	4315.0
88.00	4318.0
91.00	397.0
92.00	2952.0
93.00	4054.0
94.00	11379.0
95.00	98992.0
96.00	6460.0
103.90	404.0
104.90	139.0
105.90	342.0
108.00	163.0
114.90	111.0
115.90	380.0
116.90	884.0
117.90	319.0
118.90	839.0
127.90	363.0
128.80	211.0
129.90	328.0
130.90	160.0
137.00	165.0
140.90	992.0
142.00	181.0
143.00	1657.0
143.90	113.0
144.90	1035.0
145.90	197.0
148.00	276.0
149.90	111.0
155.00	264.0
156.90	127.0
170.90	394.0
172.00	1519.0
173.00	1122.0
174.00	88672.0
175.00	6697.0
176.00	85968.0
177.00	5847.0
177.90	169.0

Instrument :
MSVOA_U
ClientSampleId :
BFB007