

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U120219\
 Data File : VU035934.D
 Acq On : 02 Dec 2019 15:20
 Operator : JC/SP
 Sample : K6003-04
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Quant Time: Dec 02 18:23:41 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR112119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Dec 02 18:11:23 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	244536	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.45	117	282903	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.84	152	107635	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	186780	5.85	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	117.00%
7) Chloroethane-d5	1.93	69	153217	5.54	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	110.80%
11) 1,1-Dichloroethene-d2	2.59	63	201570	3.39	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.80%
20) 2-Butanone-d5	4.70	46	320378	43.34	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	86.68%
24) Chloroform-d	5.11	84	250694	4.63	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.60%
26) 1,2-Dichloroethane-d4	5.75	65	134913	4.44	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.80%
32) Benzene-d6	5.77	84	490969	4.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.00%
36) 1,2-Dichloropropane-d6	6.73	67	163093	4.48	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.60%
41) Toluene-d8	7.93	98	390734	3.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.40%
43) trans-1,3-Dichloropropene-	8.21	79	59856	4.23	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.60%
46) 2-Hexanone-d5	8.68	63	231548	40.71	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.42%
57) 1,1,2,2-Tetrachloroethane-	10.78	84	126746	4.14	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	82.80%
64) 1,2-Dichlorobenzene-d4	12.22	152	117818	5.04	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.80%


Target Compounds				Ovalue
13) Acetone	2.68	43	15942	2.455 ug/L 93
16) Methylene chloride	3.08	84	15490	0.504 ug/L 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU120219\
Data File : VU035934.D
Acq On : 02 Dec 2019 15:20
Operator : JC/SP
Sample : K6003-04
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Time: Dec 02 18:23:41 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR112119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Dec 02 18:11:23 2019
Response via : Initial Calibration

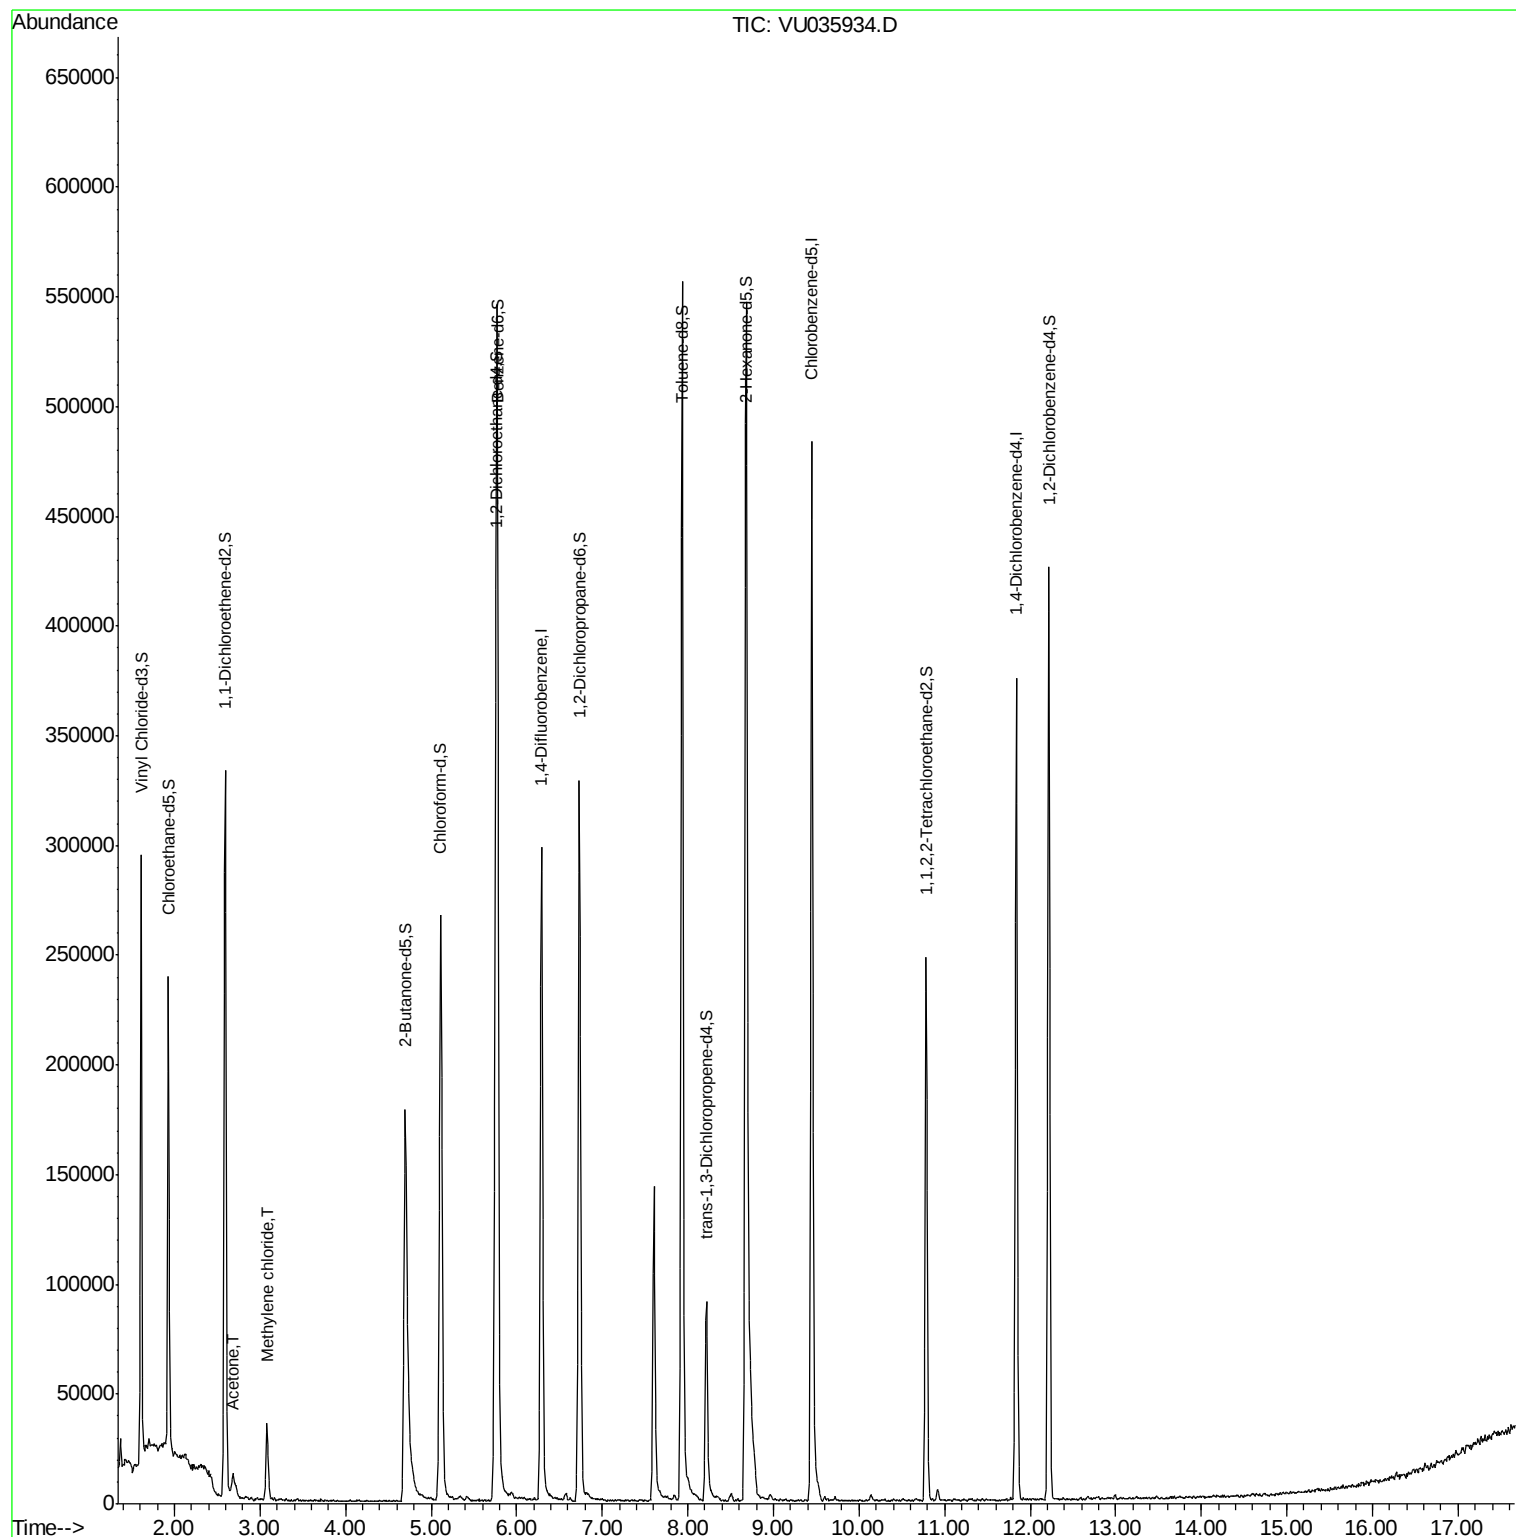

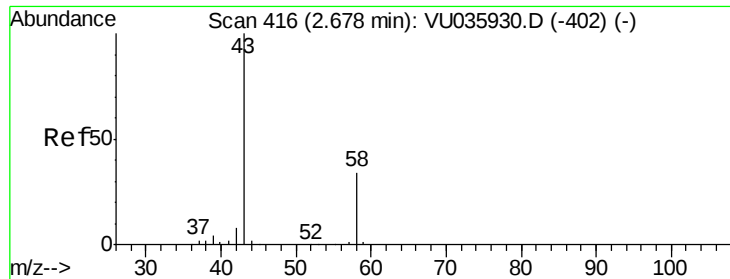

#13

Acetone

Concen: 2.455 ug/L

RT: 2.68 min Scan# 418

Delta R.T. 0.02 min

Lab File: VU035934.D

Acq: 02 Dec 2019 15:20

Instrument :

MSVOA_U

ClientSampleId :


VHBLK01

Tot Ion: 43 Resp: 15942




Ion Ratio Lower Upper

43 100

58 34.5 0.0 61.2

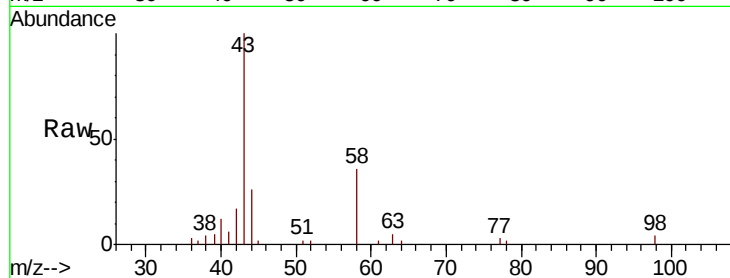

Abundance Ion 43.05 (42.75 to 43.75): VU035934.D (-319) (-)

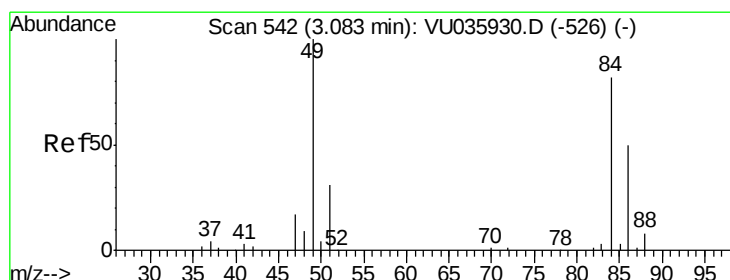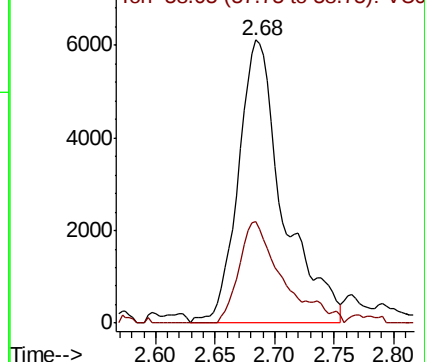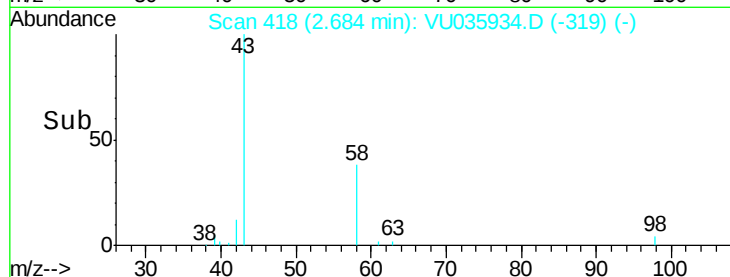

#16

Methylene chloride

Concen: 0.504 ug/L

RT: 3.08 min Scan# 542

Delta R.T. 0.00 min

Lab File: VU035934.D

Acq: 02 Dec 2019 15:20


Tgt Ion: 84 Resp: 15490

Ion Ratio Lower Upper

84 100

86 69.6 44.4 82.5

49 126.0 94.0 174.6

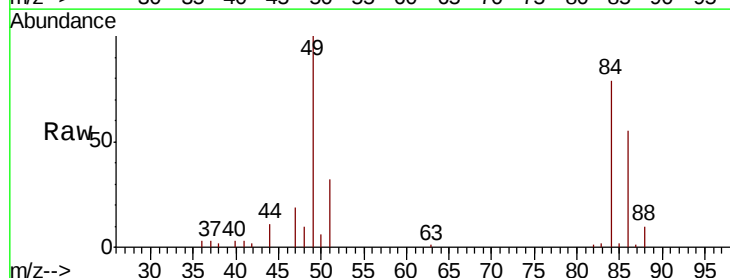

Abundance Ion 84.05 (83.75 to 84.75): VU035934.D (-448) (-)

