


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU120219\
 Data File : VU035929.D
 Acq On : 02 Dec 2019 10:17
 Operator : JC/SP
 Sample : BFB09
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB09

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR112119WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Dec 04 10:53:38 2019

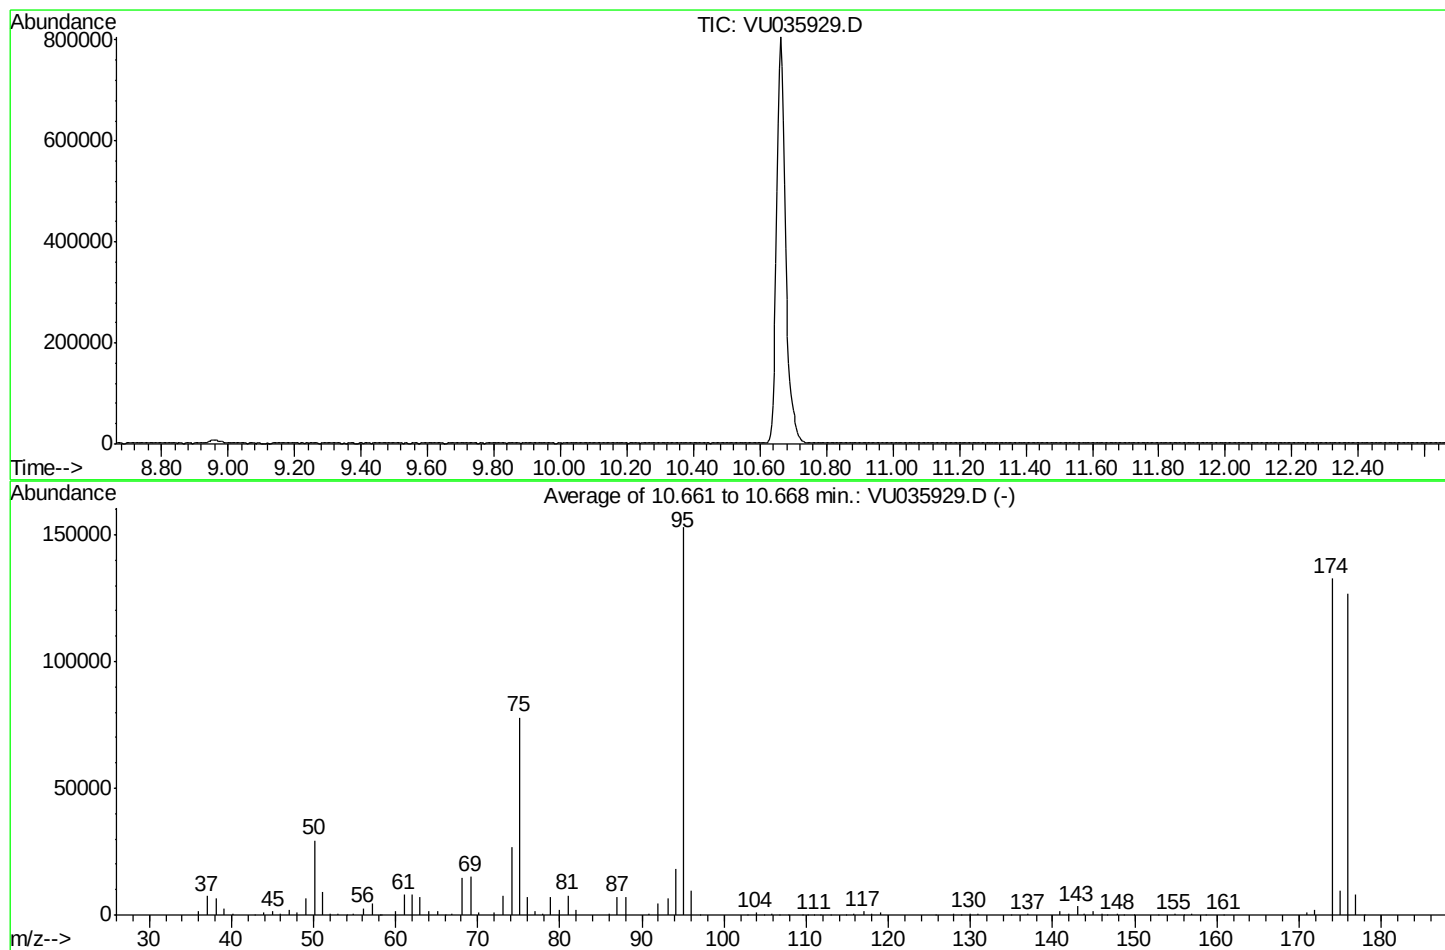

AutoFind: Scans 2899, 2900, 2901; Background Corrected with Scan 2883

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	29450	PASS
75	95	30	80	50.9	77888	PASS
95	95	100	100	100.0	152917	PASS
96	95	5	9	6.4	9794	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	86.8	132696	PASS
175	174	5	9	7.3	9626	PASS
176	174	95	101	95.3	126504	PASS
177	176	5	9	6.5	8163	PASS

m/z	Abundance
36.00	1461.0
37.10	7544.0
38.10	6989.0
39.10	2865.0
39.80	442.0
40.30	459.0
42.90	187.0
44.00	1954.0
45.10	1323.0
46.00	380.0
47.10	2173.0
48.00	935.0
49.00	6911.0
50.10	29688.0
51.10	9853.0
51.90	387.0
53.00	289.0
54.10	289.0
54.90	477.0
56.10	2827.0
57.10	4618.0
58.30	126.0
60.00	1802.0
61.10	8634.0
62.00	8184.0
63.00	7180.0
64.10	1491.0
65.10	1426.0
66.10	133.0
66.90	515.0
68.10	15704.0
69.10	15190.0
70.00	1223.0
72.00	941.0
73.00	7934.0
74.10	26848.0
75.10	81360.0
76.10	7313.0
77.00	1383.0
77.90	812.0
78.90	7400.0
79.90	2086.0
81.00	8278.0
82.00	1986.0
86.10	332.0
87.00	7522.0
88.00	6791.0
90.80	555.0
92.00	4674.0
93.10	6796.0
94.00	18864.0
95.10	155968.0
96.00	10019.0
97.10	358.0
102.90	104.0
103.90	837.0
104.80	205.0
105.90	632.0
106.80	187.0
107.70	181.0
109.60	123.0
110.10	129.0
111.00	132.0
112.90	100.0
114.90	148.0
115.90	537.0
116.90	1373.0
117.90	454.0
119.00	1231.0
125.80	104.0
128.00	522.0
128.80	235.0
129.90	494.0
130.90	276.0
135.00	164.0
137.00	340.0
140.90	1538.0
141.90	293.0
143.00	3209.0
143.90	357.0
145.00	1731.0
146.00	256.0
146.70	162.0
147.90	467.0
150.00	256.0
152.90	122.0
154.90	519.0
156.00	119.0
157.00	333.0
158.60	117.0
160.80	121.0
171.00	923.0

Instrument :
MSVOA_U
ClientSampleId :
BFB09

172.00	2019.0
174.00	133888.0
175.00	10237.0
176.00	128248.0
177.00	8671.0
177.90	240.0

Instrument :
MSVOA_U
ClientSampleId :
BFB09

m/z	Abundance
36.00	1485.0
37.00	7605.0
38.10	6634.0
39.10	2874.0
39.80	524.0
40.20	477.0
42.90	193.0
44.00	2063.0
45.00	1410.0
46.00	333.0
47.10	2137.0
48.10	935.0
49.00	6644.0
50.10	30136.0
51.10	9363.0
51.90	413.0
53.00	298.0
54.10	237.0
54.90	510.0
56.00	2818.0
57.10	4430.0
58.00	124.0
60.00	1732.0
61.00	8189.0
62.10	8037.0
63.00	7330.0
64.10	1532.0
65.00	1426.0
66.10	146.0
66.90	558.0
68.10	14669.0
69.10	15270.0
70.00	1109.0
72.00	991.0
73.00	7742.0
74.10	27280.0
75.10	79680.0
76.00	7214.0
77.00	1499.0
77.80	761.0
78.90	7523.0
79.90	2026.0
81.00	7978.0
81.90	2042.0
86.10	388.0
87.00	7153.0
88.00	7394.0
90.90	590.0
92.00	4449.0
93.10	6769.0
94.00	18680.0
95.10	156544.0
96.00	10072.0
97.20	250.0
102.80	133.0
103.90	870.0
104.80	218.0
105.80	632.0
106.80	217.0
107.80	192.0
109.60	154.0
110.90	196.0
111.70	131.0
113.00	160.0
114.90	137.0
115.90	672.0
117.00	1441.0
117.90	596.0
119.00	1115.0
125.80	102.0
128.00	593.0
128.80	249.0
129.90	606.0
130.80	311.0
135.00	230.0
137.10	334.0
140.90	1626.0
141.90	335.0
143.00	3424.0
143.90	338.0
145.00	1546.0
146.00	287.0
146.70	139.0
148.00	499.0
149.90	208.0
152.90	141.0
154.90	465.0
156.00	129.0
157.00	383.0
158.60	134.0
160.80	173.0
171.00	826.0

Instrument :
MSVOA_U
ClientSampleId :
BFB09

172.00	1763.0
174.00	136704.0
175.00	9834.0
176.00	130456.0
177.00	8208.0
178.00	249.0

Instrument :
MSVOA_U
ClientSampleId :
BFB09

m/z	Abundance
36.00	1323.0
37.00	7103.0
38.10	5658.0
39.10	2365.0
39.80	624.0
42.90	146.0
44.00	2125.0
45.10	1341.0
46.00	258.0
47.00	1903.0
48.10	877.0
49.00	5999.0
50.10	28528.0
51.10	8254.0
52.00	432.0
53.00	316.0
54.10	158.0
54.90	496.0
56.00	2382.0
57.10	4026.0
58.10	157.0
60.00	1463.0
61.00	7190.0
62.10	7434.0
63.00	6597.0
64.10	1548.0
65.00	1422.0
66.00	165.0
66.90	502.0
68.00	13561.0
69.10	14979.0
70.10	1165.0
71.90	899.0
73.00	7214.0
74.10	25520.0
75.00	72624.0
76.00	6538.0
77.00	1399.0
77.90	638.0
78.90	6764.0
80.00	1899.0
81.00	7194.0
81.90	2006.0
86.00	485.0
87.00	6768.0
88.00	7074.0
91.00	608.0
92.00	4234.0
93.10	6076.0
94.10	17368.0
95.00	146240.0
96.00	9293.0
97.20	185.0
102.80	111.0
103.90	793.0
104.80	242.0
105.80	562.0
106.80	168.0
107.80	155.0
109.60	138.0
110.90	175.0
111.70	103.0
113.00	173.0
114.90	116.0
115.80	727.0
117.00	1367.0
117.90	672.0
119.00	961.0
125.80	111.0
128.00	544.0
128.80	234.0
130.00	646.0
130.80	275.0
134.90	304.0
137.10	251.0
140.90	1470.0
142.00	331.0
143.00	3527.0
143.90	264.0
145.00	1242.0
146.00	333.0
148.00	441.0
148.70	100.0
149.90	191.0
153.00	112.0
154.80	365.0
156.00	118.0
157.00	433.0
158.70	101.0
160.90	172.0
170.90	670.0
171.90	1805.0

Instrument :
MSVOA_U
ClientSampleId :
BFB09

174.00	127496.0
175.00	8808.0
176.00	120808.0
176.90	7612.0
178.00	190.0

Instrument :
MSVOA_U
ClientSampleId :
BFB09

Scan 2883 (10.610 min): VU035929.D
BFB09

m/z	Abundance
39.90	578.0
41.90	165.0
43.90	1099.0

Instrument :
MSVOA_U
ClientSampleId :
BFB09