

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120221\
 Data File : VU046053.D
 Acq On : 02 Dec 2021 15:34
 Operator : SY/MD
 Sample : M4868-02ME
 Misc : 6.84g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGKN9ME

Quant Time: Dec 03 05:11:40 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 03 05:08:36 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	244901	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.427	117	238612	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	120169	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	70511	34.952	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	69.900%
7) Chloroethane-d5	1.916	69	47789	30.853	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	61.700%#
11) 1,1-Dichloroethene-d2	2.543	63	95629	26.406	ug/L	-0.03
Spiked Amount	50.000	Range	60 - 125	Recovery	=	52.820%#
21) 2-Butanone-d5	4.652	46	121729	75.905	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	75.900%
24) Chloroform-d	5.067	84	126713	37.613	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	75.220%
26) 1,2-Dichloroethane-d4	5.703	65	90664	40.101	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	80.200%
32) Benzene-d6	5.723	84	284549	41.607	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.220%
36) 1,2-Dichloropropane-d6	6.690	67	90058	42.489	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	84.980%
41) Toluene-d8	7.899	98	258561	41.523	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	83.040%
43) trans-1,3-Dichloroprop...	8.186	79	44231	43.229	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.460%
47) 2-Hexanone-d5	8.678	63	88501	88.065	ug/L	0.04
Spiked Amount	100.000	Range	45 - 130	Recovery	=	88.070%
56) 1,1,2,2-Tetrachloroeth...	10.771	84	122969	38.256	ug/L	0.01
Spiked Amount	50.000	Range	65 - 120	Recovery	=	76.520%
66) 1,2-Dichlorobenzene-d4	12.198	152	100235	43.312	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.620%
Target Compounds						
					Qvalue	
15) Methyl Acetate	2.967	43	1967	0.842	ug/L #	80
52) Ethylbenzene	9.575	91	24071	2.886	ug/L	99
53) m,p-Xylene	9.697	106	28600	8.793	ug/L	99
54) o-xylene	10.108	106	8100	2.567	ug/L	98
63) 1,2,4-Trimethylbenzene	11.472	105	17760	2.724	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120221\
Data File : VU046053.D
Acq On : 02 Dec 2021 15:34
Operator : SY/MD
Sample : M4868-02ME
Misc : 6.84g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGKN9ME

Quant Time: Dec 03 05:11:40 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 03 05:08:36 2021
Response via : Initial Calibration




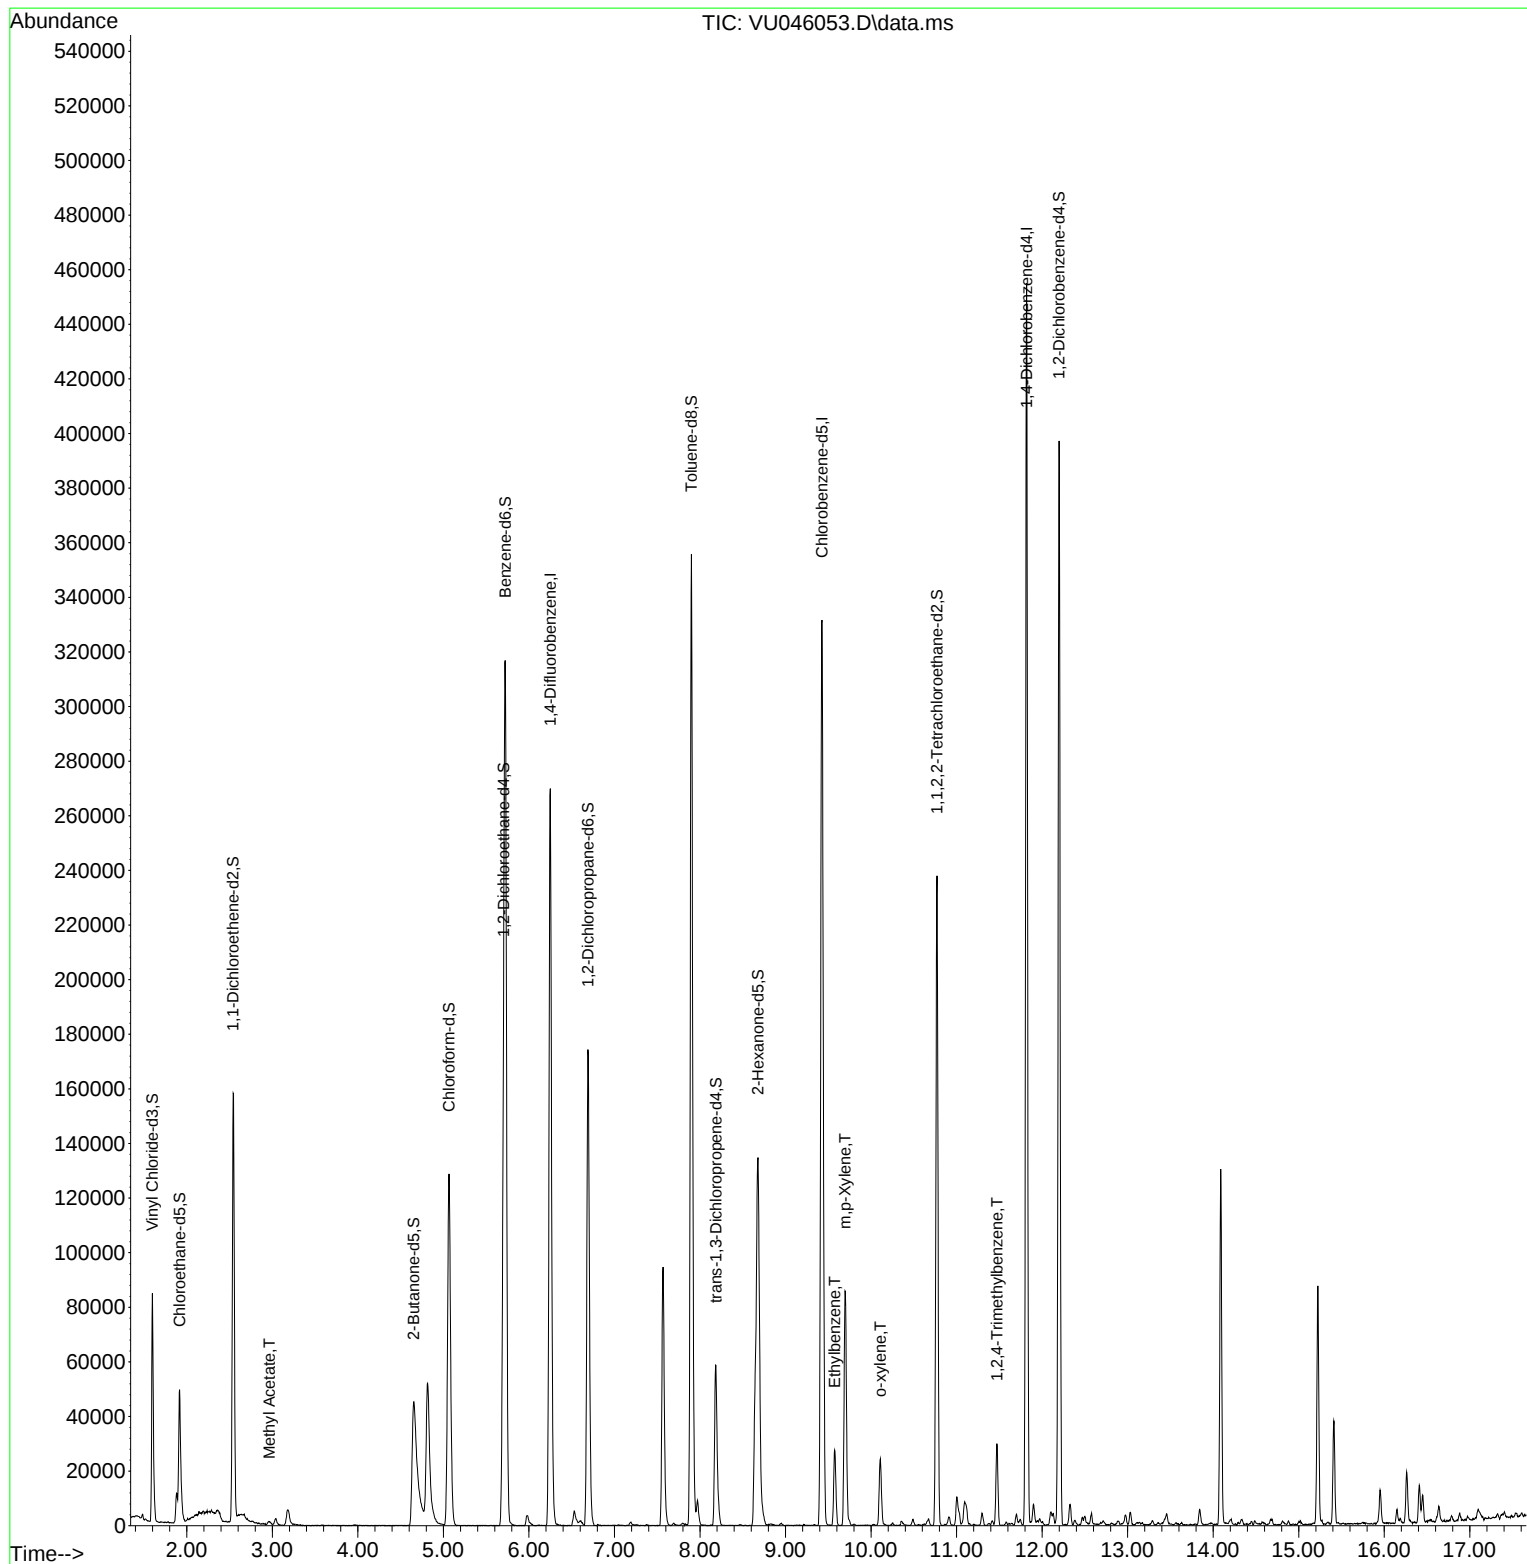


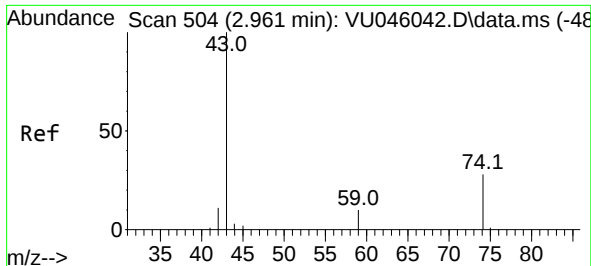

#15
Methyl Acetate
Concen: 0.842 ug/L
RT: 2.967 min Scan# 504
Delta R.T. 0.007 min
Lab File: VU046053.D
Acq: 02 Dec 2021 15:34




Instrument :
MSVOA_U
ClientSampleId :
BGKN9ME


Tgt Ion: 43 Resp: 1967
Ion Ratio Lower Upper
43 100
74 16.0 20.8 31.2#

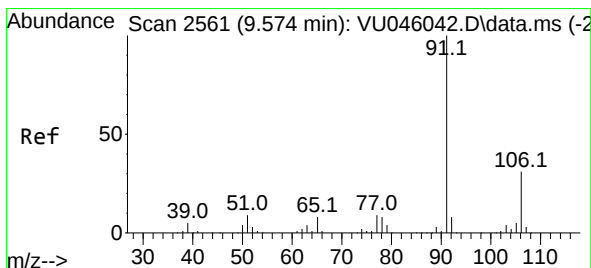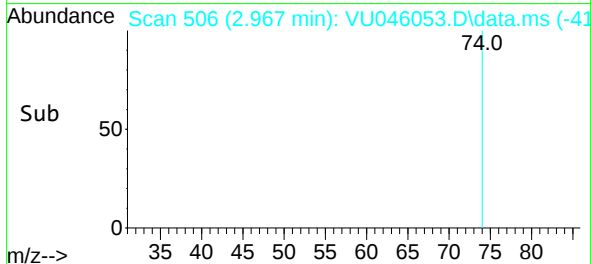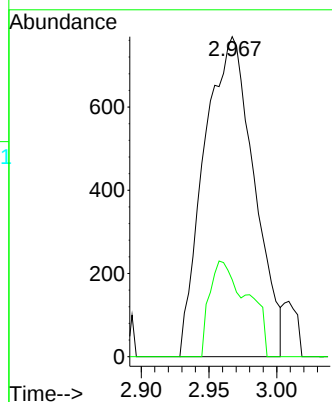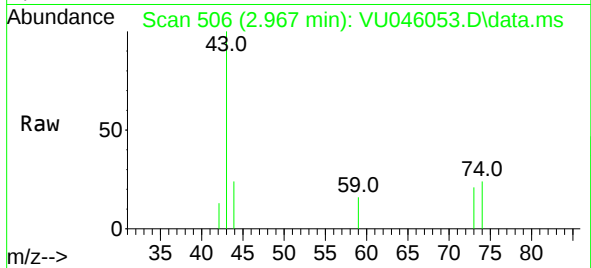

#52
Ethylbenzene
Concen: 2.886 ug/L
RT: 9.575 min Scan# 2561
Delta R.T. 0.000 min
Lab File: VU046053.D
Acq: 02 Dec 2021 15:34

Tgt Ion: 91 Resp: 24071
Ion Ratio Lower Upper
91 100
106 29.5 21.1 39.3


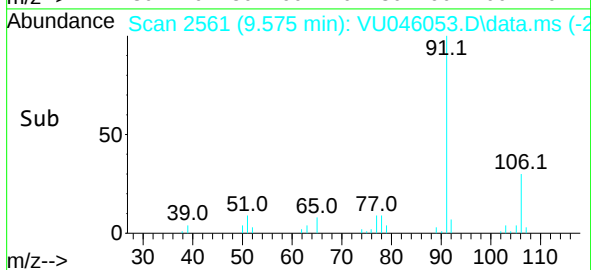
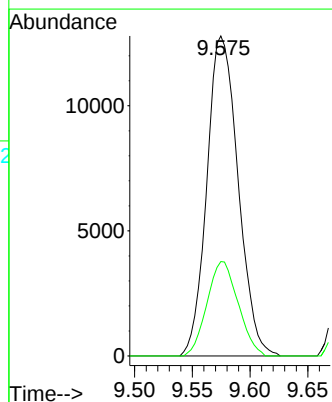
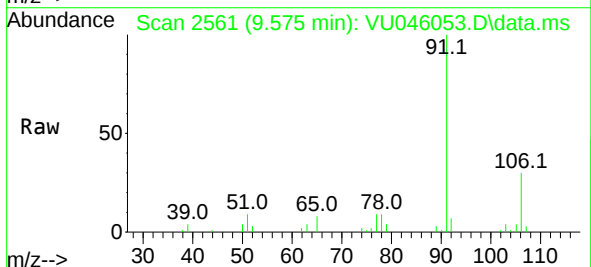


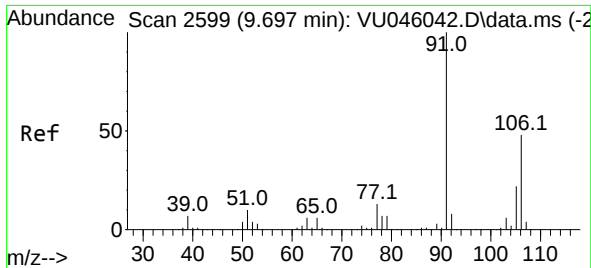

#53
m,p-Xylene
Concen: 8.793 ug/L
RT: 9.697 min Scan# 21
Delta R.T. 0.000 min
Lab File: VU046053.D
Acq: 02 Dec 2021 15:34




Instrument :
MSVOA_U
ClientSampleId :
BGKN9ME


Tgt Ion:106 Resp: 28600
Ion Ratio Lower Upper
106 100
91 204.5 144.3 268.1

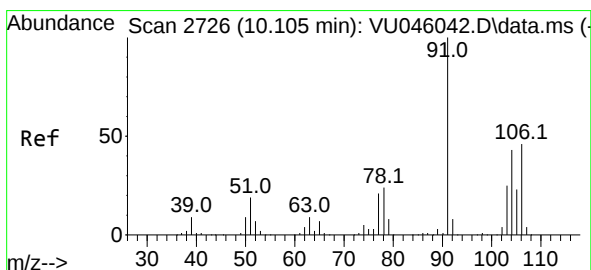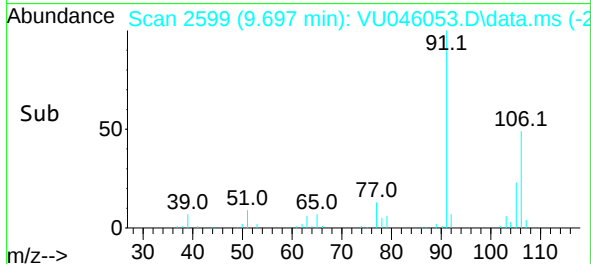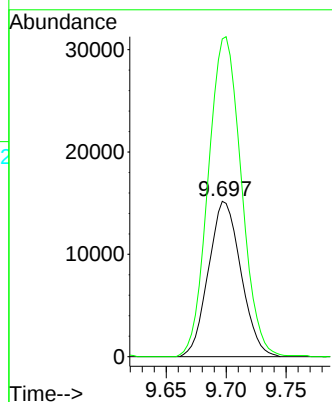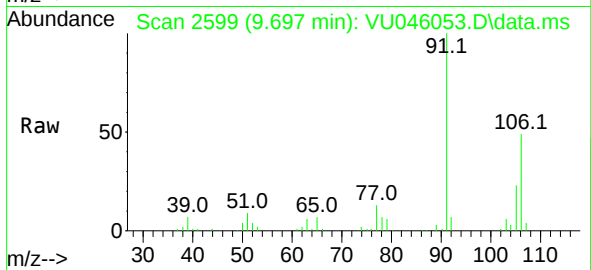

#54
o-xylene
Concen: 2.567 ug/L
RT: 10.108 min Scan# 2727
Delta R.T. 0.003 min
Lab File: VU046053.D
Acq: 02 Dec 2021 15:34

Tgt Ion:106 Resp: 8100
Ion Ratio Lower Upper
106 100
91 223.1 154.2 286.4

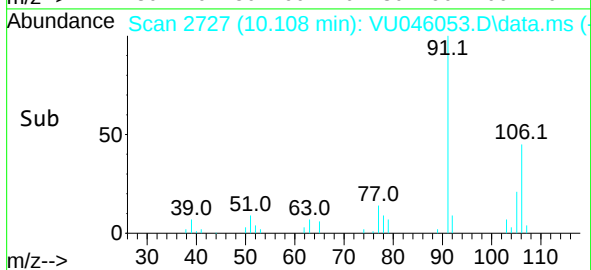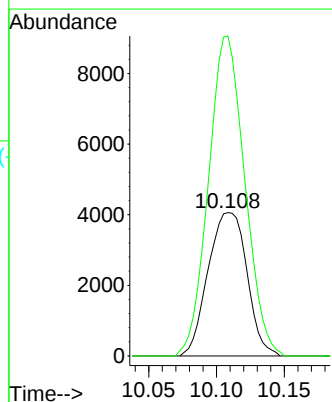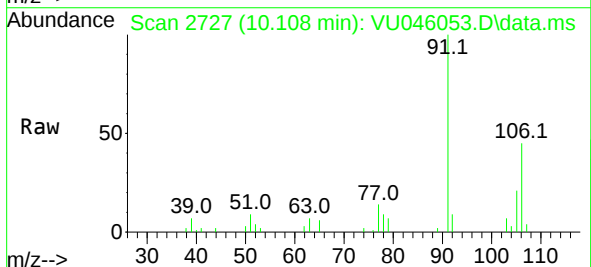

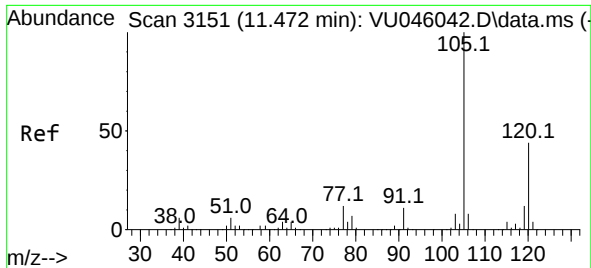

#63

1,2,4-Trimethylbenzene

Concen: 2.724 ug/L

RT: 11.472 min Scan# 31

Delta R.T. 0.000 min

Lab File: VU046053.D

Acq: 02 Dec 2021 15:34

Instrument :

MSVOA_U

ClientSampleId :

BGKN9ME

Tgt Ion:105 Resp: 17760

Ion Ratio Lower Upper

105 100

120 45.7 35.2 52.8

