

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120221\
 Data File : VU046054.D
 Acq On : 02 Dec 2021 15:57
 Operator : SY/MD
 Sample : M4870-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGKN9

Quant Time: Dec 03 05:11:53 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 03 05:08:36 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	219111	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	215985	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	112829	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	61698	34.183	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	68.360%		
7) Chloroethane-d5	1.916	69	49414	35.657	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	71.320%		
11) 1,1-Dichloroethene-d2	2.568	63	88645	27.358	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	54.720%#		
21) 2-Butanone-d5	4.633	46	130385	90.872	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	90.870%		
24) Chloroform-d	5.067	84	127332	42.245	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	84.500%		
26) 1,2-Dichloroethane-d4	5.703	65	84568	41.807	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	83.620%		
32) Benzene-d6	5.729	84	267398	43.195	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.380%		
36) 1,2-Dichloropropane-d6	6.694	67	84732	44.165	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	88.320%		
41) Toluene-d8	7.899	98	244155	43.317	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	86.640%		
43) trans-1,3-Dichloroprop...	8.182	79	39448	42.594	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	85.180%		
47) 2-Hexanone-d5	8.632	63	89960	98.895	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	98.890%		
56) 1,1,2,2-Tetrachloroeth...	10.758	84	122867	42.229	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	84.460%		
66) 1,2-Dichlorobenzene-d4	12.195	152	98188	45.188	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	90.380%		
Target Compounds					Qvalue	
13) Acetone	2.649	43	25419	14.175	ug/L	92
20) cis-1,2-Dichloroethene	4.671	96	7252	4.169	ug/L	99
22) 2-Butanone	4.716	43	6218	3.185	ug/L	96
33) Benzene	5.780	78	4306	0.659	ug/L	100
40) 4-Methyl-2-pentanone	7.793	43	4567	1.815	ug/L	96
42) Toluene	7.973	91	19027	2.713	ug/L	96
52) Ethylbenzene	9.571	91	76843	10.179	ug/L	100
53) m,p-Xylene	9.693	106	75796	25.746	ug/L	95
54) o-xylene	10.102	106	31490	11.023	ug/L	96
62) 1,3,5-Trimethylbenzene	11.089	105	6319	1.033	ug/L	100
63) 1,2,4-Trimethylbenzene	11.468	105	22792	3.723	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120221\
Data File : VU046054.D
Acq On : 02 Dec 2021 15:57
Operator : SY/MD
Sample : M4870-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGKN9

Quant Time: Dec 03 05:11:53 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 03 05:08:36 2021
Response via : Initial Calibration




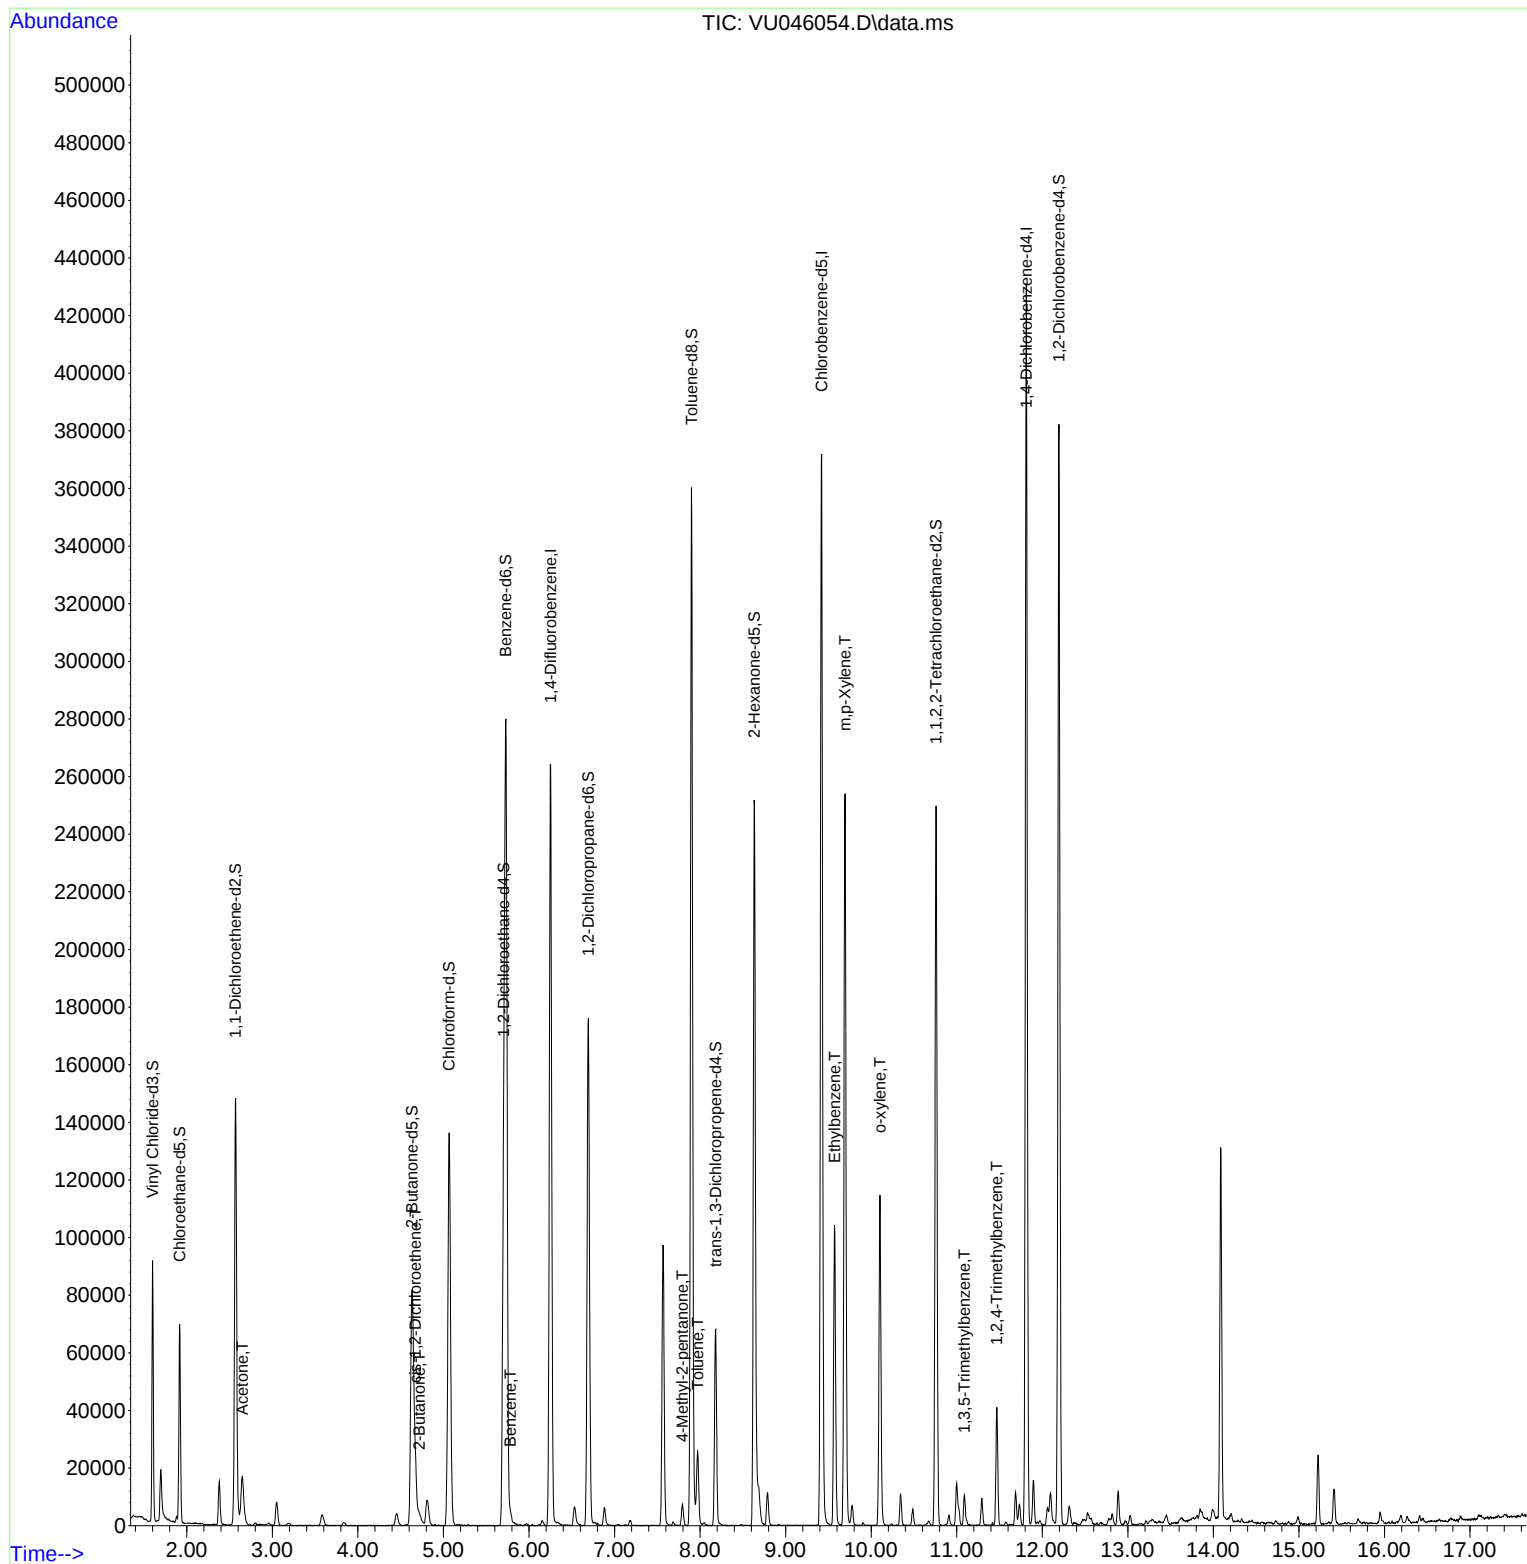


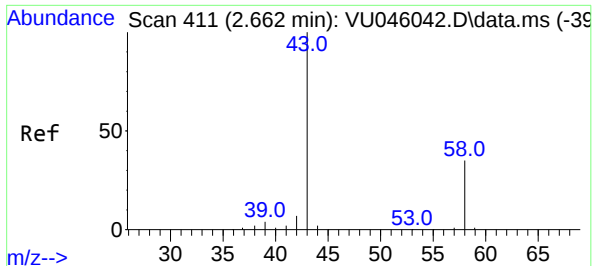

#13
Acetone
Concen: 14.175 ug/L
RT: 2.649 min Scan# 407
Delta R.T. -0.013 min
Lab File: VU046054.D
Acq: 02 Dec 2021 15:57




Instrument :
MSVOA_U
ClientSampleId :
BGKN9


Tgt Ion: 43 Resp: 25419
Ion Ratio Lower Upper
43 100
58 37.7 0.0 66.8

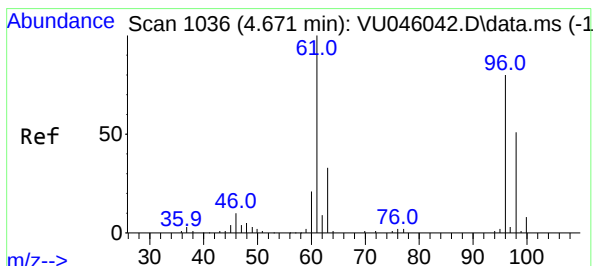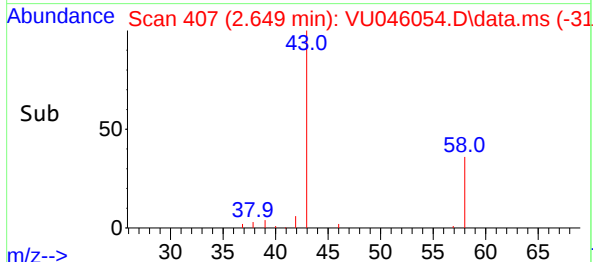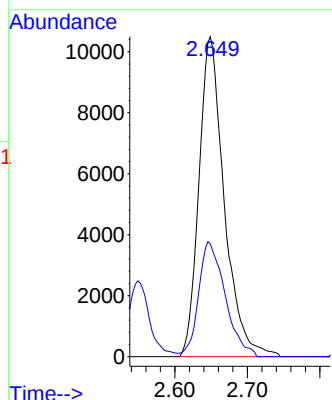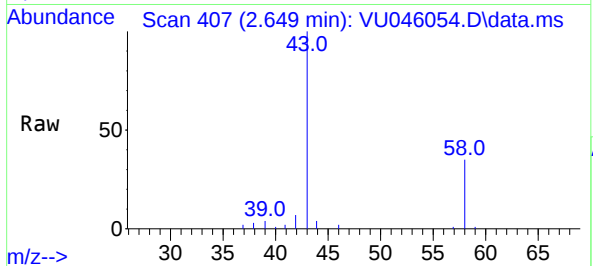

#20
cis-1,2-Dichloroethene
Concen: 4.169 ug/L
RT: 4.671 min Scan# 1036
Delta R.T. 0.000 min
Lab File: VU046054.D
Acq: 02 Dec 2021 15:57

Tgt Ion: 96 Resp: 7252
Ion Ratio Lower Upper
96 100
61 122.6 86.8 161.2
68 0.0 0.0 0.0


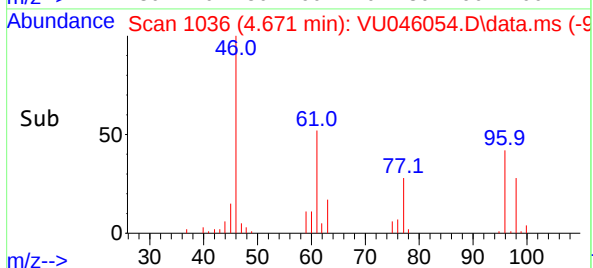
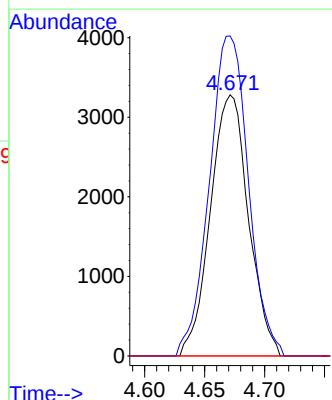
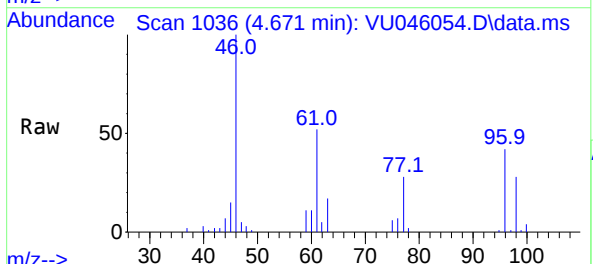


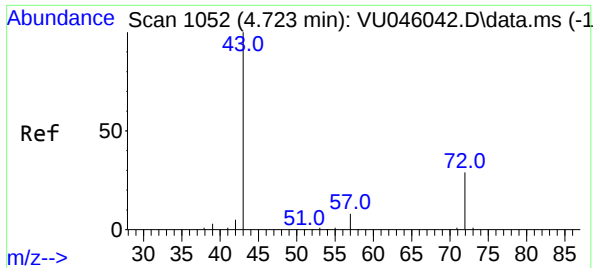

#22
2-Butanone
Concen: 3.185 ug/L
RT: 4.716 min Scan# 1050
Delta R.T. -0.006 min
Lab File: VU046054.D
Acq: 02 Dec 2021 15:57




Instrument :
MSVOA_U
ClientSampleId :
BGKN9


Tgt Ion: 43 Resp: 6218
Ion Ratio Lower Upper
43 100
72 31.4 14.5 43.6

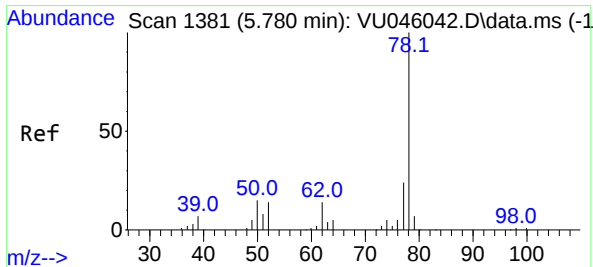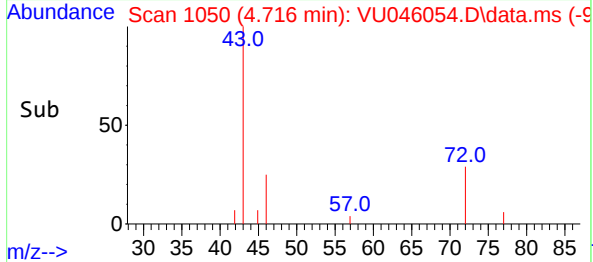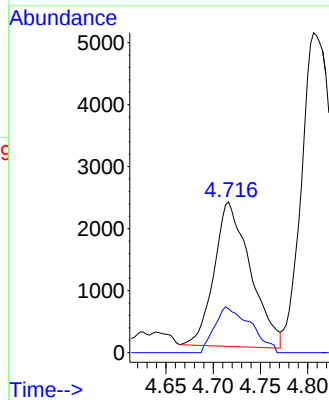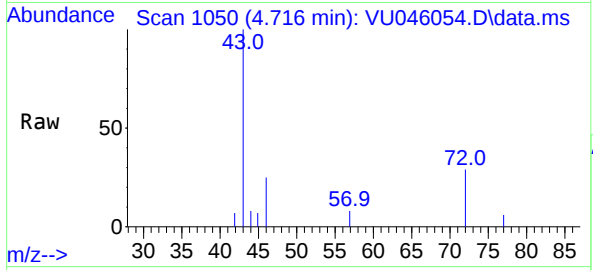

#33
Benzene
Concen: 0.659 ug/L
RT: 5.780 min Scan# 1381
Delta R.T. 0.000 min
Lab File: VU046054.D
Acq: 02 Dec 2021 15:57

Tgt Ion: 78 Resp: 4306

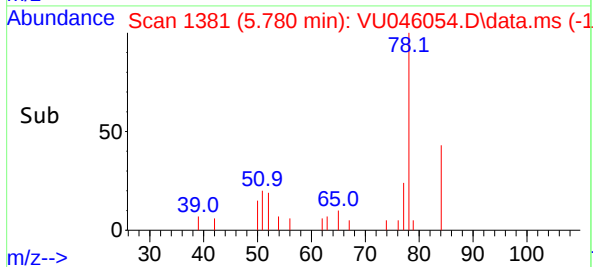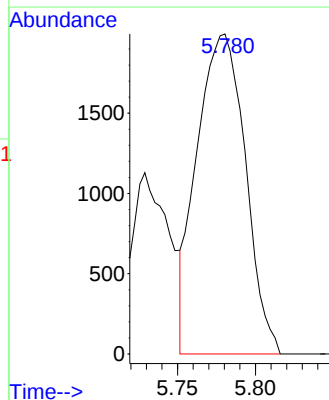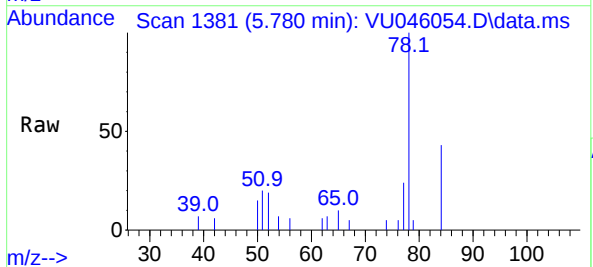

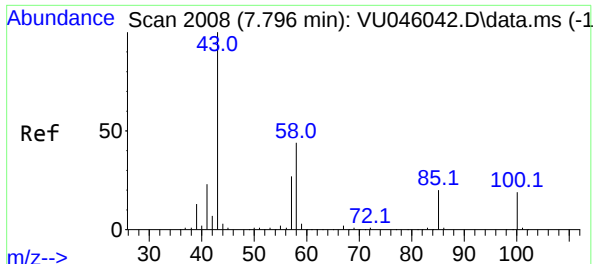

#40

4-Methyl-2-pentanone

Concen: 1.815 ug/L

RT: 7.793 min Scan# 2007

Delta R.T. -0.003 min

Lab File: VU046054.D

Acq: 02 Dec 2021 15:57

Instrument :

MSVOA_U

ClientSampleId :

BGKN9





Tgt Ion: 43 Resp: 4567

Ion Ratio Lower Upper

43 100

58 45.1 34.2 51.4

100 16.2 14.5 21.7

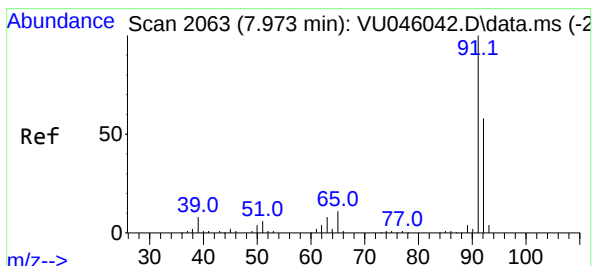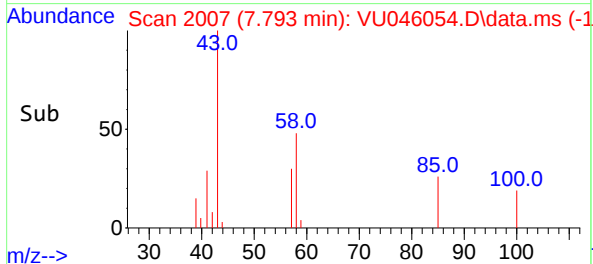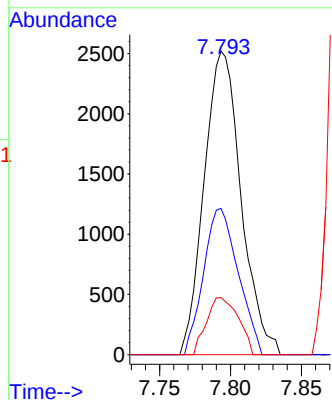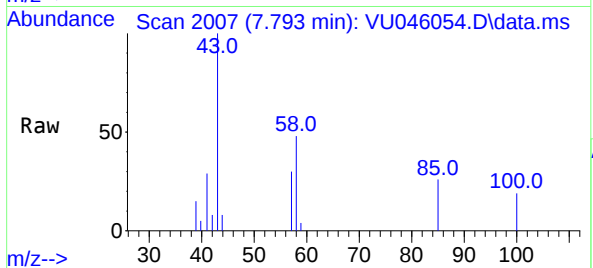

#42

Toluene

Concen: 2.713 ug/L

RT: 7.973 min Scan# 2063

Delta R.T. 0.000 min

Lab File: VU046054.D




Acq: 02 Dec 2021 15:57


Tgt Ion: 91 Resp: 19027

Ion Ratio Lower Upper

91 100

92 57.1 41.9 77.7


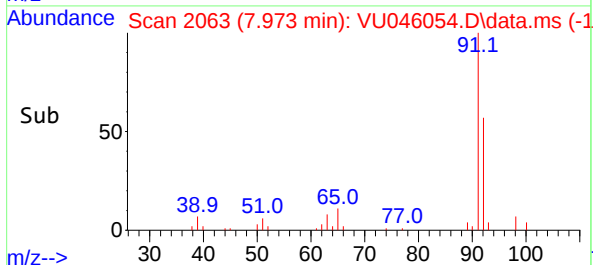
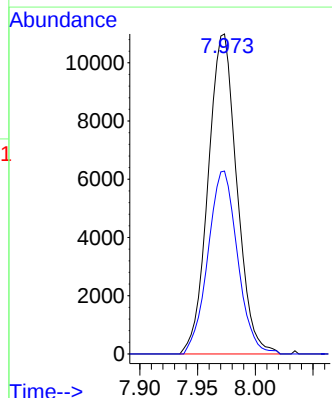
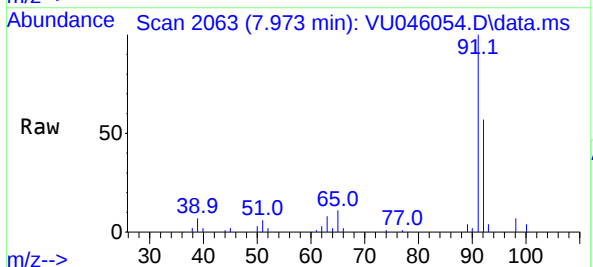


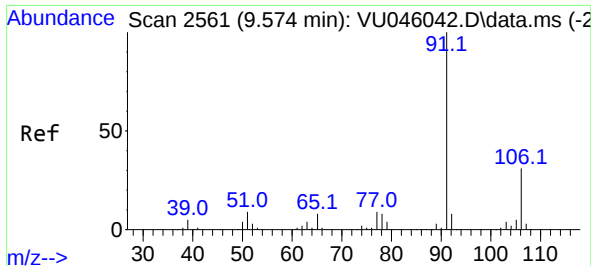

#52
Ethylbenzene
Concen: 10.179 ug/L
RT: 9.571 min Scan# 2561
Delta R.T. -0.003 min
Lab File: VU046054.D
Acq: 02 Dec 2021 15:57




Instrument :
MSVOA_U
ClientSampleId :
BGKN9


Tgt Ion: 91 Resp: 76843
Ion Ratio Lower Upper
91 100
106 30.2 21.1 39.3

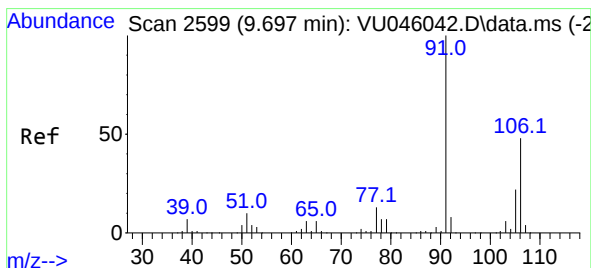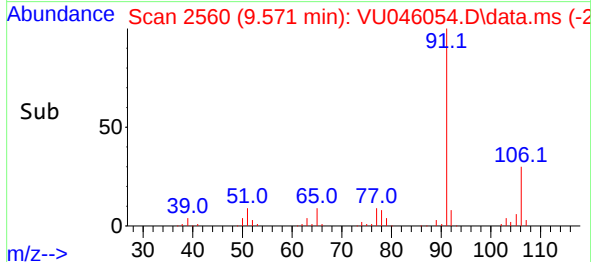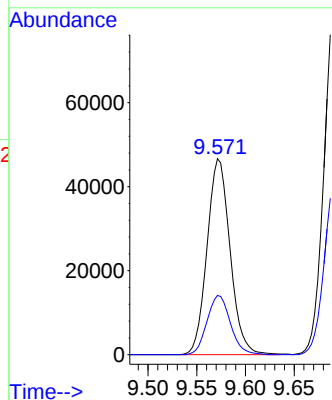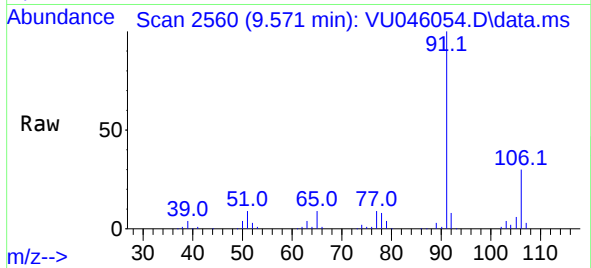

#53
m,p-Xylene
Concen: 25.746 ug/L
RT: 9.693 min Scan# 2598
Delta R.T. -0.003 min
Lab File: VU046054.D
Acq: 02 Dec 2021 15:57

Tgt Ion:106 Resp: 75796
Ion Ratio Lower Upper
106 100
91 198.0 144.3 268.1


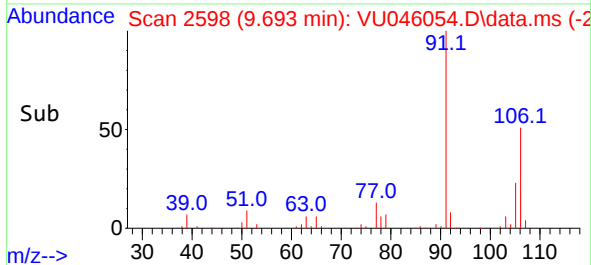
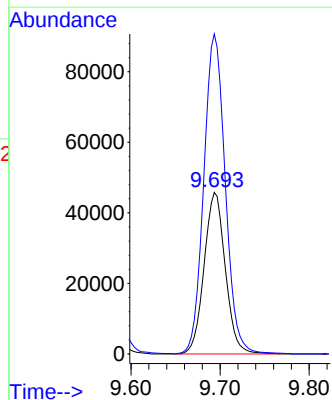
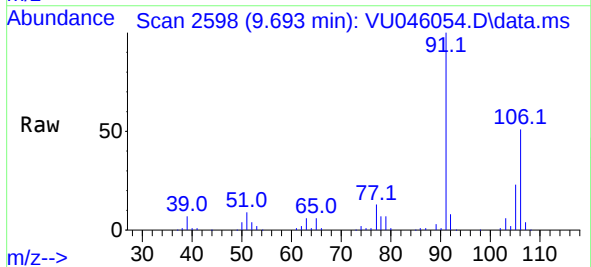


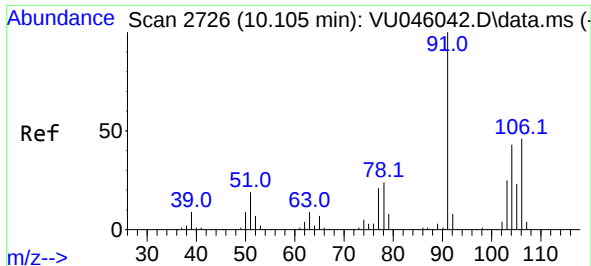

#54
o-xylene
Concen: 11.023 ug/L
RT: 10.102 min Scan# 21
Delta R.T. -0.003 min
Lab File: VU046054.D
Acq: 02 Dec 2021 15:57




Instrument :
MSVOA_U
ClientSampleId :
BGKN9


Tgt Ion:106 Resp: 31490
Ion Ratio Lower Upper
106 100
91 214.2 154.2 286.4

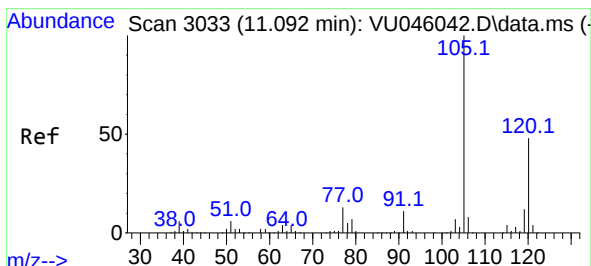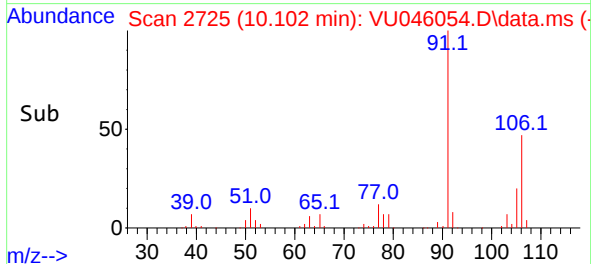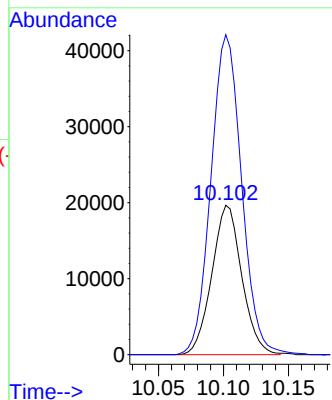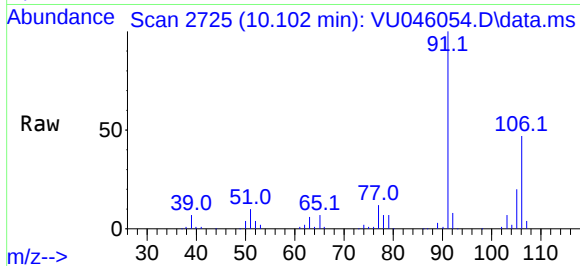

#62
1,3,5-Trimethylbenzene
Concen: 1.033 ug/L
RT: 11.089 min Scan# 3032
Delta R.T. -0.003 min
Lab File: VU046054.D
Acq: 02 Dec 2021 15:57

Tgt Ion:105 Resp: 6319
Ion Ratio Lower Upper
105 100
120 47.0 37.8 56.6

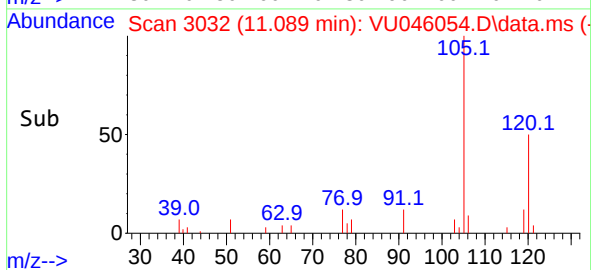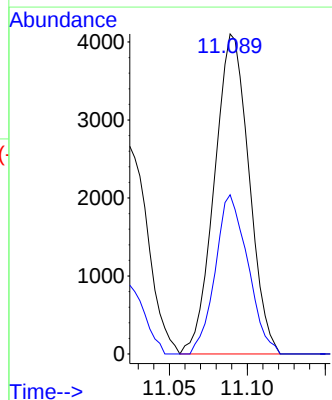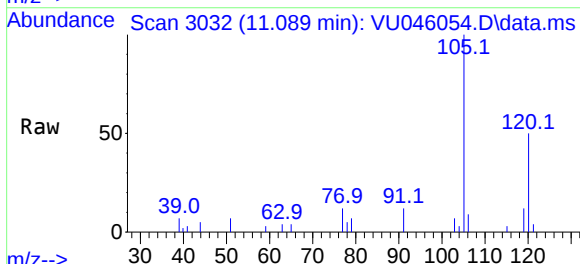

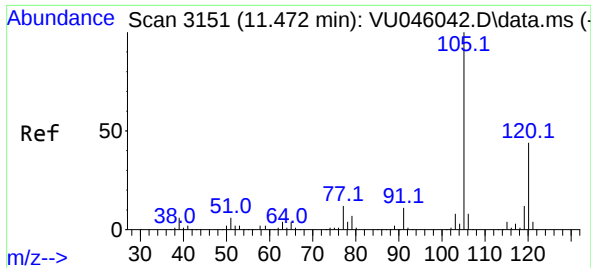

#63
1,2,4-Trimethylbenzene
Concen: 3.723 ug/L
RT: 11.468 min Scan# 31
Delta R.T. -0.003 min
Lab File: VU046054.D
Acq: 02 Dec 2021 15:57

Instrument :
MSVOA_U
ClientSampleId :
BGKN9

Tgt Ion:105 Resp: 22792
Ion Ratio Lower Upper
105 100
120 43.2 35.2 52.8

