

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120221\
 Data File : VU046044.D
 Acq On : 02 Dec 2021 10:44
 Operator : SY/MD
 Sample : VU1202WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK044

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046044.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	94	rBV	92678	101284	14.04%	1.810%
2	1.919	171	180	191	rBV	72040	91909	12.74%	1.643%
3	2.327	303	307	309	rBV2	300	168	0.02%	0.003%
4	2.511	361	364	369	rVB2	227	225	0.03%	0.004%
5	2.572	370	383	411	rBV	149510	248651	34.47%	4.444%
6	2.755	436	440	443	rBV	198	202	0.03%	0.004%
7	2.800	446	454	459	rVV	526	797	0.11%	0.014%
8	2.874	474	477	481	rBV	177	193	0.03%	0.003%
9	3.019	516	522	527	rBV	173	303	0.04%	0.005%
10	3.051	527	532	538	rVV3	584	692	0.10%	0.012%
11	3.154	560	564	566	rBV	140	120	0.02%	0.002%
12	3.208	576	581	584	rBV	142	175	0.02%	0.003%
13	3.305	607	611	614	rBB	152	149	0.02%	0.003%
14	3.375	630	633	635	rBV	147	123	0.02%	0.002%
15	3.507	669	674	677	rBV	201	229	0.03%	0.004%
16	3.662	716	722	725	rBB	161	214	0.03%	0.004%
17	3.845	776	779	783	rBB	145	142	0.02%	0.003%
18	3.916	798	801	805	rBV	168	200	0.03%	0.004%
19	3.964	814	816	822	rBB	156	175	0.02%	0.003%
20	4.006	826	829	833	rBB	145	125	0.02%	0.002%
21	4.276	911	913	916	rBV	145	123	0.02%	0.002%
22	4.330	924	930	933	rBB	147	198	0.03%	0.004%
23	4.353	934	937	940	rBB	142	121	0.02%	0.002%
24	4.565	1001	1003	1006	rBV	143	124	0.02%	0.002%
25	4.639	1011	1026	1065	rVV	59574	184987	25.65%	3.306%
26	4.874	1096	1099	1104	rVB2	192	135	0.02%	0.002%
27	5.067	1142	1159	1180	rVV	123364	283126	39.25%	5.061%
28	5.160	1185	1188	1191	rVB2	280	203	0.03%	0.004%
29	5.179	1191	1194	1198	rBV2	325	280	0.04%	0.005%
30	5.227	1206	1209	1213	rBV2	146	147	0.02%	0.003%
31	5.279	1221	1225	1228	rBB	138	115	0.02%	0.002%
32	5.298	1228	1231	1233	rBV	216	164	0.02%	0.003%
33	5.588	1317	1321	1325	rBB	178	207	0.03%	0.004%
34	5.729	1343	1365	1385	rBV2	268356	721308	100.00%	12.893%
35	5.951	1432	1434	1438	rVB2	304	213	0.03%	0.004%
36	5.977	1439	1442	1446	rBV2	274	284	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120221\
 Data File : VU046044.D
 Acq On : 02 Dec 2021 10:44
 Operator : SY/MD
 Sample : VU1202WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK044

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	6.047	1460	1464	1467	rVB2	280	201	0.03%	0.004%
38	6.147	1491	1495	1498	rBB	138	119	0.02%	0.002%
39	6.253	1513	1528	1547	rBV	231149	433896	60.15%	7.755%
40	6.436	1582	1585	1587	rVB	185	123	0.02%	0.002%
41	6.462	1587	1593	1595	rBV2	138	151	0.02%	0.003%
42	6.533	1603	1615	1634	rBV5	7183	17166	2.38%	0.307%
43	6.694	1651	1665	1686	rBV	167733	322416	44.70%	5.763%
44	6.864	1710	1718	1724	rBB	168	330	0.05%	0.006%
45	6.896	1724	1728	1735	rBV	152	283	0.04%	0.005%
46	7.089	1785	1788	1791	rVB	170	130	0.02%	0.002%
47	7.144	1803	1805	1809	rBB	184	147	0.02%	0.003%
48	7.182	1809	1817	1830	rBV3	1539	2600	0.36%	0.046%
49	7.295	1847	1852	1853	rBV	148	129	0.02%	0.002%
50	7.414	1886	1889	1893	rBB	155	147	0.02%	0.003%
51	7.436	1893	1896	1899	rBB	142	119	0.02%	0.002%
52	7.568	1924	1937	1955	rBV	90422	154334	21.40%	2.759%
53	7.684	1968	1973	1982	rVB5	856	1398	0.19%	0.025%
54	7.768	1993	1999	2002	rBV	159	226	0.03%	0.004%
55	7.899	2026	2040	2057	rBV	333357	578843	80.25%	10.346%
56	8.179	2116	2127	2141	rBV2	61166	101438	14.06%	1.813%
57	8.292	2161	2162	2166	rVB	229	127	0.02%	0.002%
58	8.366	2182	2185	2189	rBV	198	206	0.03%	0.004%
59	8.443	2206	2209	2211	rBV	163	128	0.02%	0.002%
60	8.462	2211	2215	2219	rVV	106	126	0.02%	0.002%
61	8.533	2234	2237	2241	rBB	172	159	0.02%	0.003%
62	8.568	2246	2248	2252	rVB	209	165	0.02%	0.003%
63	8.636	2252	2269	2301	rBV	200385	371260	51.47%	6.636%
64	9.054	2396	2399	2402	rBV	139	144	0.02%	0.003%
65	9.301	2473	2476	2478	rBV	171	144	0.02%	0.003%
66	9.417	2499	2512	2541	rBV	329572	552251	76.56%	9.871%
67	9.578	2555	2562	2566	rVB2	347	366	0.05%	0.007%
68	9.697	2594	2599	2606	rVB2	558	730	0.10%	0.013%
69	9.954	2674	2679	2685	rBV	136	139	0.02%	0.002%
70	10.044	2705	2707	2711	rVB	175	149	0.02%	0.003%
71	10.066	2712	2714	2717	rBV	198	160	0.02%	0.003%
72	10.092	2718	2722	2724	rBV	196	129	0.02%	0.002%
73	10.481	2840	2843	2847	rBV2	161	164	0.02%	0.003%
74	10.674	2893	2903	2912	rVV3	1551	2017	0.28%	0.036%
75	10.758	2916	2929	2946	rBV	225933	360393	49.96%	6.442%
76	10.893	2969	2971	2974	rBV	237	163	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120221\
 Data File : VU046044.D
 Acq On : 02 Dec 2021 10:44
 Operator : SY/MD
 Sample : VU1202WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK044

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.089	3028	3032	3035	rVB2	269	159	0.02%	0.003%
78	11.455	3140	3146	3148	rBV	659	583	0.08%	0.010%
79	11.690	3215	3219	3223	rBV2	336	296	0.04%	0.005%
80	11.738	3231	3234	3235	rBV	290	159	0.02%	0.003%
81	11.812	3245	3257	3273	rBV	330955	520935	72.22%	9.311%
82	11.947	3291	3299	3301	rBV	284	333	0.05%	0.006%
83	11.976	3304	3308	3311	rVB	601	396	0.05%	0.007%
84	12.195	3361	3376	3392	rBV	325829	523898	72.63%	9.364%
85	12.603	3499	3503	3507	rBV	111	122	0.02%	0.002%
86	12.639	3512	3514	3518	rVB	181	130	0.02%	0.002%
87	13.227	3690	3697	3701	rBV2	494	635	0.09%	0.011%
88	13.648	3825	3828	3833	rBV	151	162	0.02%	0.003%
89	13.848	3883	3890	3897	rVB2	1060	1313	0.18%	0.023%
90	14.092	3958	3966	3973	rVB2	1120	1511	0.21%	0.027%
91	14.304	4026	4032	4035	rBV	168	209	0.03%	0.004%
92	14.330	4035	4040	4046	rVV3	828	957	0.13%	0.017%
93	15.211	4311	4314	4318	rVB2	204	164	0.02%	0.003%
94	15.372	4362	4364	4367	rBV2	221	140	0.02%	0.003%
95	15.481	4396	4398	4403	rBV2	296	247	0.03%	0.004%
96	15.513	4405	4408	4410	rBV	201	145	0.02%	0.003%
97	15.648	4448	4450	4452	rBV	232	118	0.02%	0.002%
98	16.841	4818	4821	4823	rBV2	381	248	0.03%	0.004%
99	16.876	4829	4832	4834	rBV2	479	363	0.05%	0.006%
100	17.015	4872	4875	4878	rBV3	508	395	0.05%	0.007%




Sum of corrected areas: 5594745

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120221\
Data File : VU046044.D
Acq On : 02 Dec 2021 10:44
Operator : SY/MD
Sample : VU1202WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK044

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

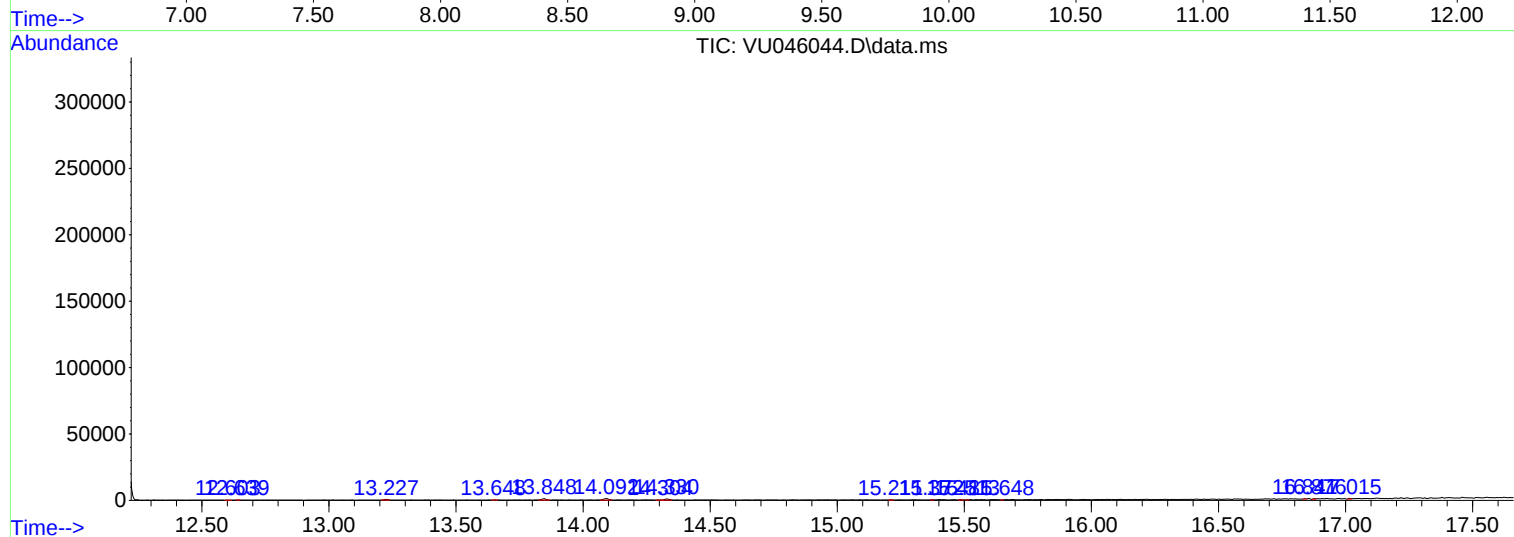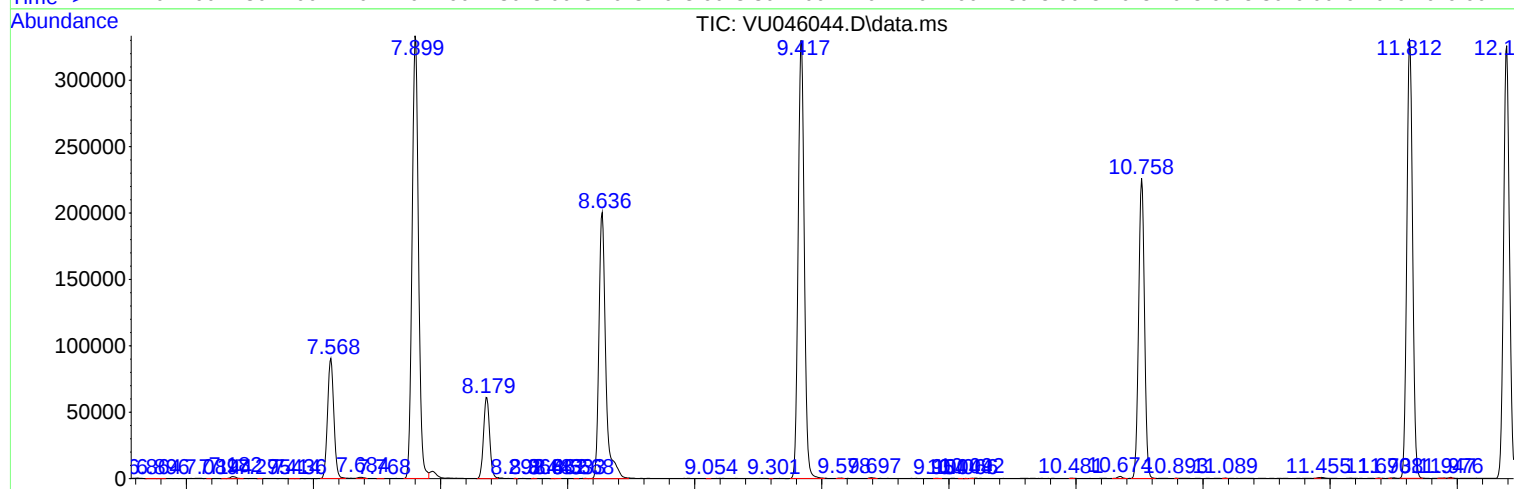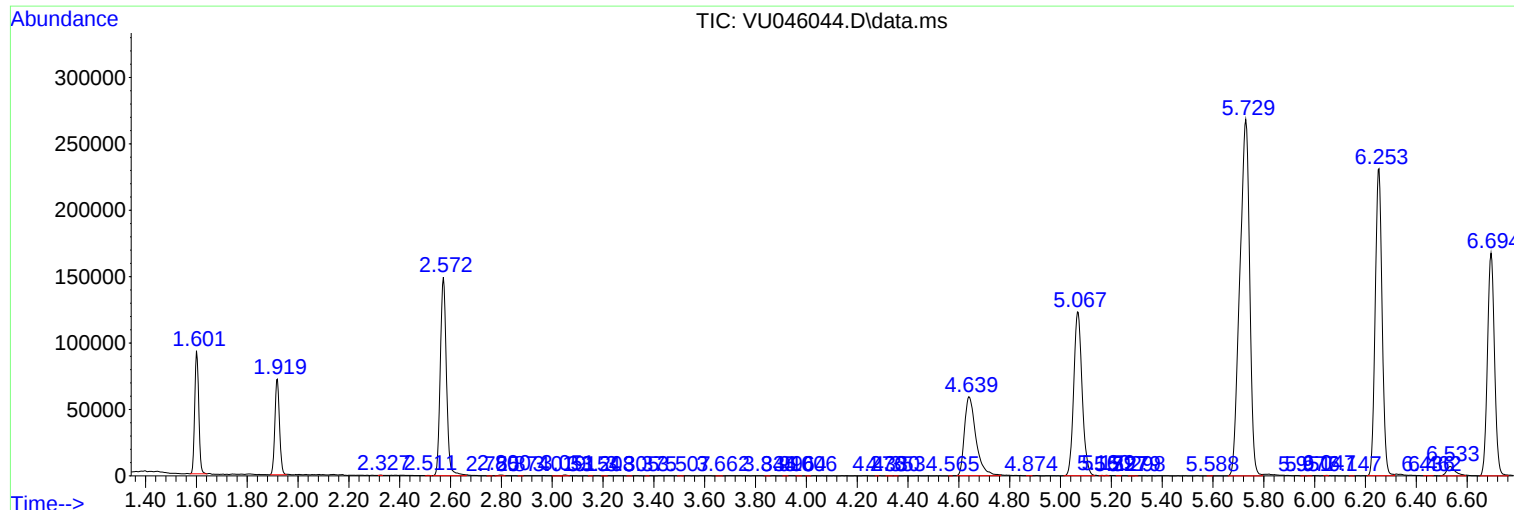

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120221\
Data File : VU046044.D
Acq On : 02 Dec 2021 10:44
Operator : SY/MD
Sample : VU1202WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK044

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120221\
Data File : VU046044.D
Acq On : 02 Dec 2021 10:44
Operator : SY/MD
Sample : VU1202WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK044

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc