

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120221\
 Data File : VU046059.D
 Acq On : 02 Dec 2021 17:49
 Operator : SY/MD
 Sample : M4878-01 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0G20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046059.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.363	3	7	13	rVB2	3949	3814	0.45%	0.054%
2	1.600	73	81	100	rBV	100499	111243	12.98%	1.577%
3	1.916	170	179	193	rVB	75849	96686	11.28%	1.371%
4	2.440	338	342	345	rVB3	528	450	0.05%	0.006%
5	2.571	371	383	402	rBV	172050	288952	33.72%	4.096%
6	3.047	522	531	539	rBV5	1126	2009	0.23%	0.028%
7	3.086	539	543	546	rVB2	199	183	0.02%	0.003%
8	3.186	565	574	585	rVB2	1361	2837	0.33%	0.040%
9	3.366	626	630	637	rVB2	688	802	0.09%	0.011%
10	3.543	678	685	688	rBV	207	297	0.03%	0.004%
11	3.774	754	757	761	rBV	194	221	0.03%	0.003%
12	3.838	773	777	781	rBV	187	232	0.03%	0.003%
13	4.063	842	847	850	rBV	164	209	0.02%	0.003%
14	4.346	929	935	939	rBV	175	294	0.03%	0.004%
15	4.536	991	994	997	rBV2	403	334	0.04%	0.005%
16	4.633	1008	1024	1049	rBV	83578	234265	27.33%	3.321%
17	4.845	1088	1090	1098	rVB	257	282	0.03%	0.004%
18	4.880	1099	1101	1108	rVB2	180	181	0.02%	0.003%
19	4.944	1115	1121	1125	rBV2	381	402	0.05%	0.006%
20	5.067	1142	1159	1180	rBV	146792	332890	38.84%	4.719%
21	5.198	1196	1200	1205	rBV2	202	204	0.02%	0.003%
22	5.292	1225	1229	1239	rVB3	602	835	0.10%	0.012%
23	5.391	1253	1260	1267	rVB4	873	1303	0.15%	0.018%
24	5.513	1291	1298	1302	rBB	163	248	0.03%	0.004%
25	5.542	1303	1307	1311	rBV	179	225	0.03%	0.003%
26	5.729	1343	1365	1390	rVV2	313804	857035	100.00%	12.149%
27	6.044	1457	1463	1468	rVV2	278	341	0.04%	0.005%
28	6.112	1481	1484	1488	rBV2	236	189	0.02%	0.003%
29	6.253	1512	1528	1547	rBV	298642	564485	65.86%	8.002%
30	6.539	1605	1617	1630	rBV7	10334	22710	2.65%	0.322%
31	6.694	1651	1665	1684	rBV	199025	382350	44.61%	5.420%
32	6.806	1695	1700	1706	rVB3	659	754	0.09%	0.011%
33	7.047	1767	1775	1781	rBV	446	584	0.07%	0.008%
34	7.179	1810	1816	1828	rBV4	1916	3093	0.36%	0.044%
35	7.398	1880	1884	1888	rBV	197	247	0.03%	0.004%
36	7.568	1924	1937	1954	rBV	111131	190575	22.24%	2.702%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120221\
 Data File : VU046059.D
 Acq On : 02 Dec 2021 17:49
 Operator : SY/MD
 Sample : M4878-01 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0G20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.684	1967	1973	1986	rVB3	1440	2224	0.26%	0.032%
38	7.790	2003	2006	2010	rBV2	285	176	0.02%	0.002%
39	7.899	2027	2040	2057	rBV	394745	692966	80.86%	9.823%
40	8.054	2086	2088	2094	rVV	256	244	0.03%	0.003%
41	8.179	2116	2127	2145	rBV	74406	124591	14.54%	1.766%
42	8.304	2160	2166	2169	rBV	173	267	0.03%	0.004%
43	8.343	2176	2178	2182	rBV	258	194	0.02%	0.003%
44	8.555	2234	2244	2255	rVB2	20217	33673	3.93%	0.477%
45	8.632	2255	2268	2303	rBV	254923	457821	53.42%	6.490%
46	8.909	2349	2354	2356	rBV	886	808	0.09%	0.011%
47	9.070	2400	2404	2409	rVV2	190	174	0.02%	0.002%
48	9.420	2500	2513	2536	rBV	420698	702984	82.03%	9.965%
49	9.571	2552	2560	2573	rVB	2405	3476	0.41%	0.049%
50	9.693	2589	2598	2610	rBV3	6085	9379	1.09%	0.133%
51	9.745	2610	2614	2616	rBV	344	231	0.03%	0.003%
52	10.102	2717	2725	2732	rVB2	712	1080	0.13%	0.015%
53	10.253	2766	2772	2778	rVB3	842	934	0.11%	0.013%
54	10.491	2840	2846	2852	rVB2	345	419	0.05%	0.006%
55	10.619	2883	2886	2887	rBV	354	186	0.02%	0.003%
56	10.674	2892	2903	2911	rVB5	1922	3899	0.45%	0.055%
57	10.758	2916	2929	2948	rBV	277277	442541	51.64%	6.273%
58	10.857	2956	2960	2965	rVV2	320	362	0.04%	0.005%
59	10.906	2969	2975	2983	rVV3	1107	1626	0.19%	0.023%
60	10.999	2995	3004	3009	rBV2	4236	5953	0.69%	0.084%
61	11.089	3023	3032	3034	rBV2	2485	2583	0.30%	0.037%
62	11.147	3048	3050	3054	rVB2	345	252	0.03%	0.004%
63	11.295	3088	3096	3106	rBV3	2385	3405	0.40%	0.048%
64	11.372	3115	3120	3127	rBV2	669	832	0.10%	0.012%
65	11.417	3127	3134	3141	rVV3	2236	3145	0.37%	0.045%
66	11.468	3141	3150	3165	rVB2	12600	20143	2.35%	0.286%
67	11.574	3175	3183	3192	rVB3	854	1225	0.14%	0.017%
68	11.642	3200	3204	3206	rBV	317	222	0.03%	0.003%
69	11.697	3211	3221	3230	rBV4	1873	3034	0.35%	0.043%
70	11.812	3245	3257	3272	rBV	457214	731389	85.34%	10.368%
71	11.899	3276	3284	3292	rVV3	2656	4729	0.55%	0.067%
72	11.944	3295	3298	3302	rVV3	1183	1153	0.13%	0.016%
73	11.973	3304	3307	3313	rVB3	1554	1592	0.19%	0.023%
74	12.095	3339	3345	3346	rBV3	1392	1172	0.14%	0.017%
75	12.195	3361	3376	3398	rVB	410496	664486	77.53%	9.420%
76	12.327	3410	3417	3425	rVB5	4294	5967	0.70%	0.085%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120221\
 Data File : VU046059.D
 Acq On : 02 Dec 2021 17:49
 Operator : SY/MD
 Sample : M4878-01 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0G20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	12.407	3439	3442	3447	rVB4	709	687	0.08%	0.010%
78	12.465	3455	3460	3464	rBV3	476	539	0.06%	0.008%
79	12.529	3478	3480	3486	rVB3	541	508	0.06%	0.007%
80	12.574	3486	3494	3500	rVB4	1362	1611	0.19%	0.023%
81	12.941	3606	3608	3613	rBV2	385	371	0.04%	0.005%
82	12.976	3613	3619	3624	rVB3	823	991	0.12%	0.014%
83	13.008	3624	3629	3630	rBV	237	197	0.02%	0.003%
84	13.031	3630	3636	3645	rVB5	964	1483	0.17%	0.021%
85	13.298	3714	3719	3725	rVB4	453	550	0.06%	0.008%
86	13.433	3756	3761	3762	rBV3	726	622	0.07%	0.009%
87	13.455	3765	3768	3776	rVB2	2024	1872	0.22%	0.027%
88	14.089	3957	3965	3977	rBV2	2568	3750	0.44%	0.053%
89	14.192	3995	3997	4002	rBV2	318	181	0.02%	0.003%
90	14.449	4074	4077	4080	rVB2	441	318	0.04%	0.005%
91	14.494	4088	4091	4095	rVB2	262	197	0.02%	0.003%
92	14.577	4112	4117	4120	rBV2	319	397	0.05%	0.006%
93	14.835	4194	4197	4202	rBV2	207	240	0.03%	0.003%
94	15.012	4249	4252	4254	rBV2	252	184	0.02%	0.003%
95	15.066	4266	4269	4272	rVB	270	173	0.02%	0.002%
96	15.092	4272	4277	4280	rBV2	279	260	0.03%	0.004%
97	15.227	4312	4319	4327	rBV2	2419	3653	0.43%	0.052%
98	15.327	4348	4350	4355	rBV2	221	190	0.02%	0.003%
99	15.413	4369	4377	4384	rBV3	1159	1776	0.21%	0.025%
100	16.217	4625	4627	4630	rBV2	343	176	0.02%	0.002%




Sum of corrected areas: 7054224

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120221\
Data File : VU046059.D
Acq On : 02 Dec 2021 17:49
Operator : SY/MD
Sample : M4878-01 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0G20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

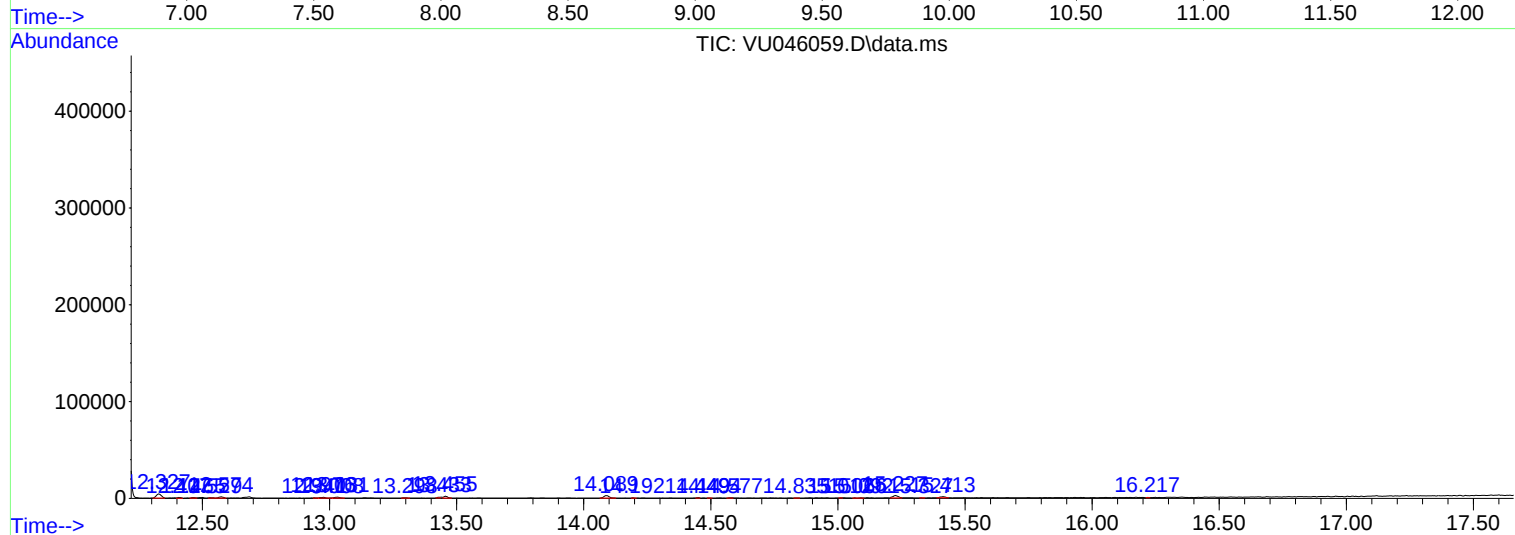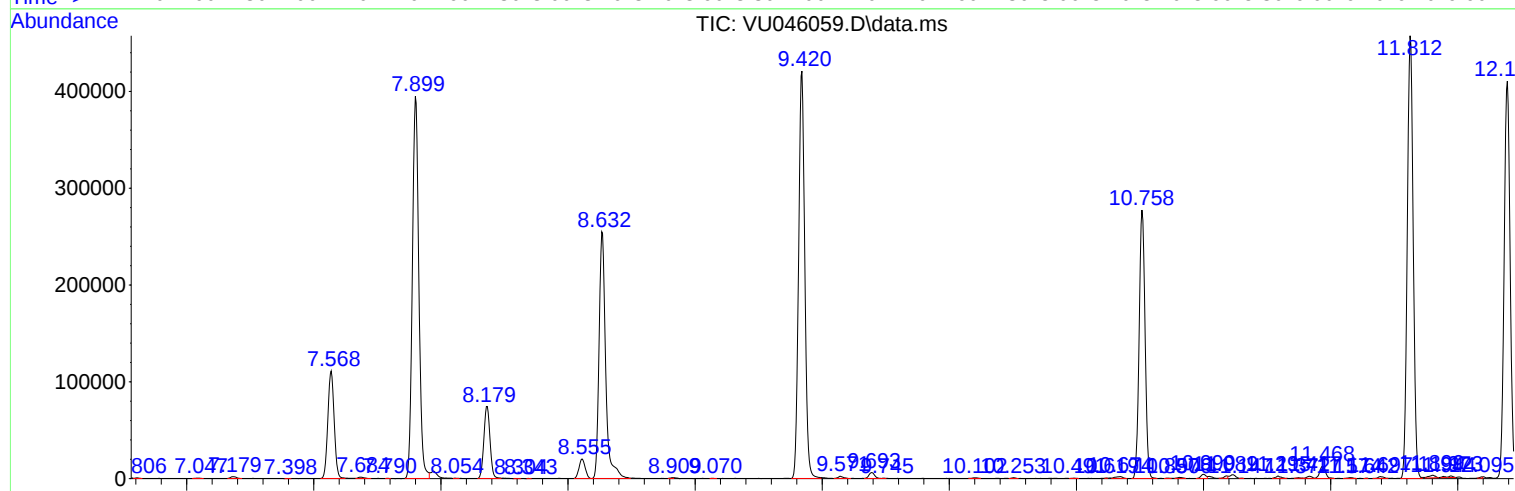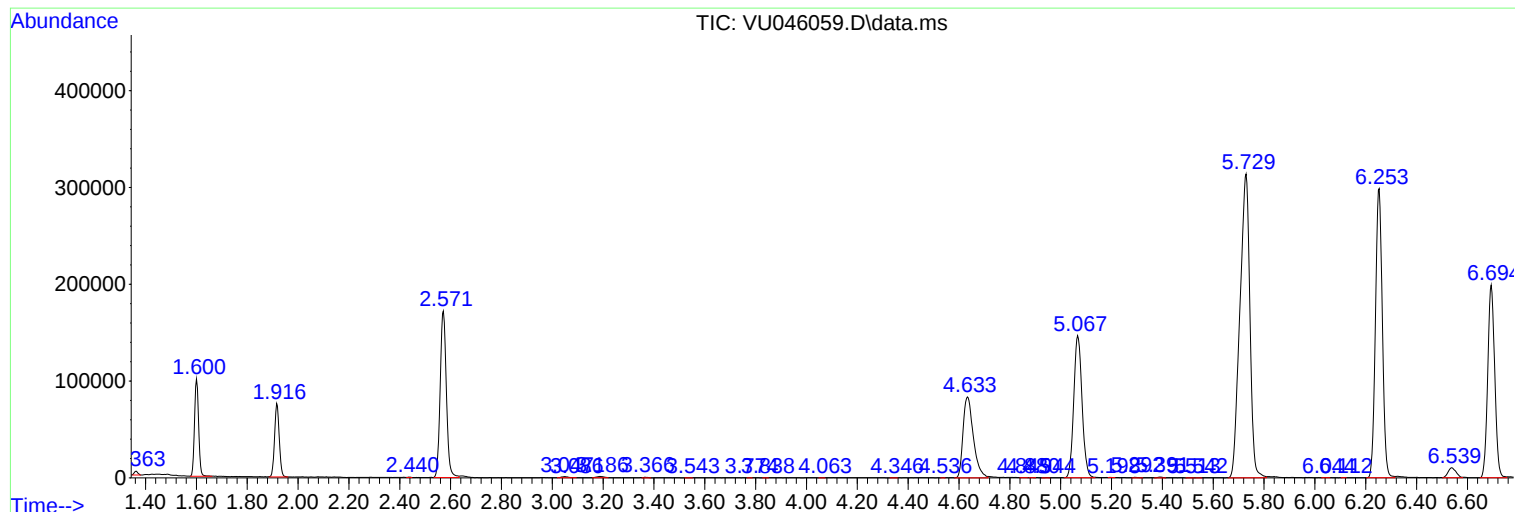

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120221\
Data File : VU046059.D
Acq On : 02 Dec 2021 17:49
Operator : SY/MD
Sample : M4878-01 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0G20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120221\
Data File : VU046059.D
Acq On : 02 Dec 2021 17:49
Operator : SY/MD
Sample : M4878-01 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0G20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc