


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120221\
 Data File : VU046041.D
 Acq On : 02 Dec 2021 09:18
 Operator : SY/MD
 Sample : BFB021
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB021

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis
 Last Update : Fri Dec 03 05:08:36 2021

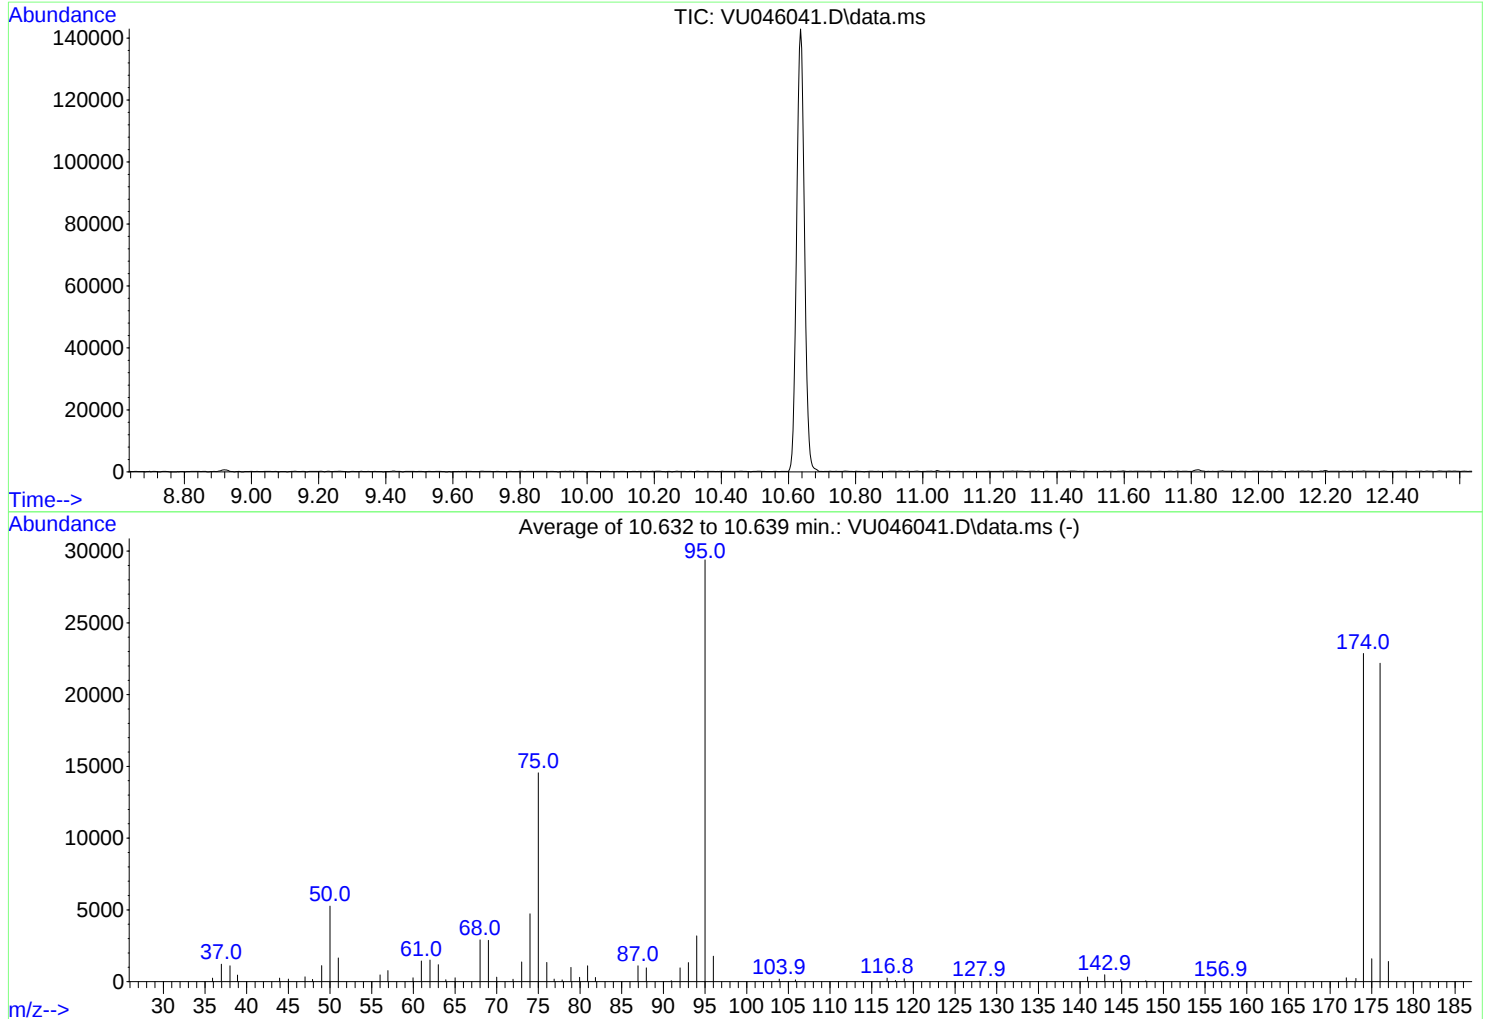

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	5266	PASS
75	95	30	80	49.5	14551	PASS
95	95	100	100	100.0	29392	PASS
96	95	5	9	6.0	1771	PASS
173	174	0.00	2	1.0	226	PASS
174	95	50	120	77.8	22867	PASS
175	174	5	9	7.0	1599	PASS
176	174	95	101	97.0	22184	PASS
177	176	5	9	6.3	1401	PASS

m/z	Abundance
35.90	252.0
37.00	1140.0
38.00	974.0
38.90	477.0
44.00	424.0
45.00	173.0
47.00	367.0
47.90	147.0
49.00	999.0
50.00	5122.0
51.00	1560.0
56.00	468.0
57.00	740.0
59.90	278.0
61.00	1370.0
62.00	1446.0
63.00	1226.0
63.90	137.0
65.00	323.0
68.00	2765.0
69.00	2762.0
70.00	320.0
71.90	161.0
73.00	1405.0
74.00	4423.0
75.00	14314.0
76.00	1299.0
76.90	184.0
77.80	137.0
78.90	912.0
80.00	302.0
80.90	1118.0
81.90	301.0
87.00	1179.0
88.00	964.0
91.00	109.0
92.00	909.0
93.00	1402.0
94.00	3095.0
95.00	28664.0
96.00	1760.0
103.90	201.0
105.80	134.0
116.80	245.0
118.90	209.0
127.90	106.0
140.90	310.0
142.90	444.0
144.90	143.0
147.90	108.0
172.00	276.0
173.10	223.0
174.00	22880.0
175.00	1559.0
176.00	22384.0
177.00	1354.0

Instrument :
MSVOA_U
ClientSampleId :
BFB021

m/z	Abundance
43.90	155.0

Instrument :
MSVOA_U
ClientSampleId :
BFB021

m/z	Abundance
35.90	227.0
36.90	1250.0
38.00	1190.0
38.90	431.0
44.00	360.0
45.00	175.0
47.00	294.0
47.90	159.0
49.00	1215.0
50.00	5247.0
51.00	1716.0
56.00	446.0
56.90	780.0
60.00	246.0
60.90	1468.0
62.00	1527.0
63.00	1084.0
63.90	123.0
65.00	212.0
68.00	2910.0
69.00	2914.0
70.00	281.0
72.00	160.0
73.00	1267.0
74.00	4889.0
75.00	14365.0
76.00	1357.0
76.90	173.0
77.80	104.0
78.90	1064.0
79.90	294.0
80.90	1048.0
81.80	280.0
86.90	1014.0
87.90	946.0
92.00	957.0
93.00	1212.0
94.00	3206.0
95.00	29152.0
96.00	1747.0
103.90	143.0
105.90	112.0
116.90	244.0
117.90	136.0
118.90	185.0
140.90	328.0
143.00	485.0
144.90	132.0
156.90	102.0
171.90	271.0
173.10	215.0
174.00	22248.0
175.00	1570.0
176.00	21264.0
177.00	1401.0

Instrument :
MSVOA_U
ClientSampleId :
BFB021

m/z	Abundance
35.90	260.0
37.00	1268.0
38.00	1149.0
38.90	480.0
44.00	412.0
45.00	177.0
47.00	342.0
47.90	162.0
49.00	1131.0
50.00	5430.0
51.00	1680.0
56.00	493.0
57.00	790.0
59.90	278.0
61.00	1491.0
62.00	1549.0
63.00	1225.0
63.90	138.0
65.00	265.0
68.00	3047.0
69.00	2949.0
70.00	320.0
71.90	169.0
73.00	1434.0
74.00	4879.0
75.00	14974.0
76.00	1360.0
76.90	174.0
77.90	128.0
78.90	1008.0
79.90	307.0
80.90	1142.0
81.90	296.0
87.00	1132.0
88.00	978.0
90.90	101.0
92.00	998.0
93.00	1374.0
94.00	3281.0
95.00	30360.0
96.00	1807.0
103.90	191.0
105.90	116.0
116.80	253.0
117.80	106.0
118.90	198.0
140.90	330.0
143.00	510.0
144.90	153.0
147.90	104.0
172.00	264.0
173.10	240.0
174.00	23472.0
175.00	1668.0
176.00	22904.0
177.00	1448.0

Instrument :
MSVOA_U
ClientSampleId :
BFB021