

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120222\
 Data File : VU052170.D
 Acq On : 02 Dec 2022 10:42
 Operator : JC/MD
 Sample : VU1202WBL04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK008

Quant Time: Dec 02 21:39:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Dec 02 00:27:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.206	114	16598	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.361	117	14723	0.500	ug/L	0.01
11) 1,4-Dichlorobenzene-d4	11.742	152	6431	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.598	65	10644	0.544	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery = 108.000%			
4) 1,2-Dichloroethane-d4	5.661	65	7901	0.426	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 86.000%			
7) 1,2-Dichloropropane-d6	6.639	67	9324	0.527	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery = 106.000%			
8) Toluene-d8	7.845	98	12024	0.451	ug/L	0.01
Spiked Amount 0.500	Range 70 - 130		Recovery = 90.000%			
10) 1,1,2,2-Tetrachloroeth...	10.679	84	9239	0.488	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery = 98.000%			
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.924	75	25	0.012	ug/L	Qvalue # 82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120222\
Data File : VU052170.D
Acq On : 02 Dec 2022 10:42
Operator : JC/MD
Sample : VU1202WBL04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK008


Quant Time: Dec 02 21:39:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 02 00:27:38 2022
Response via : Initial Calibration

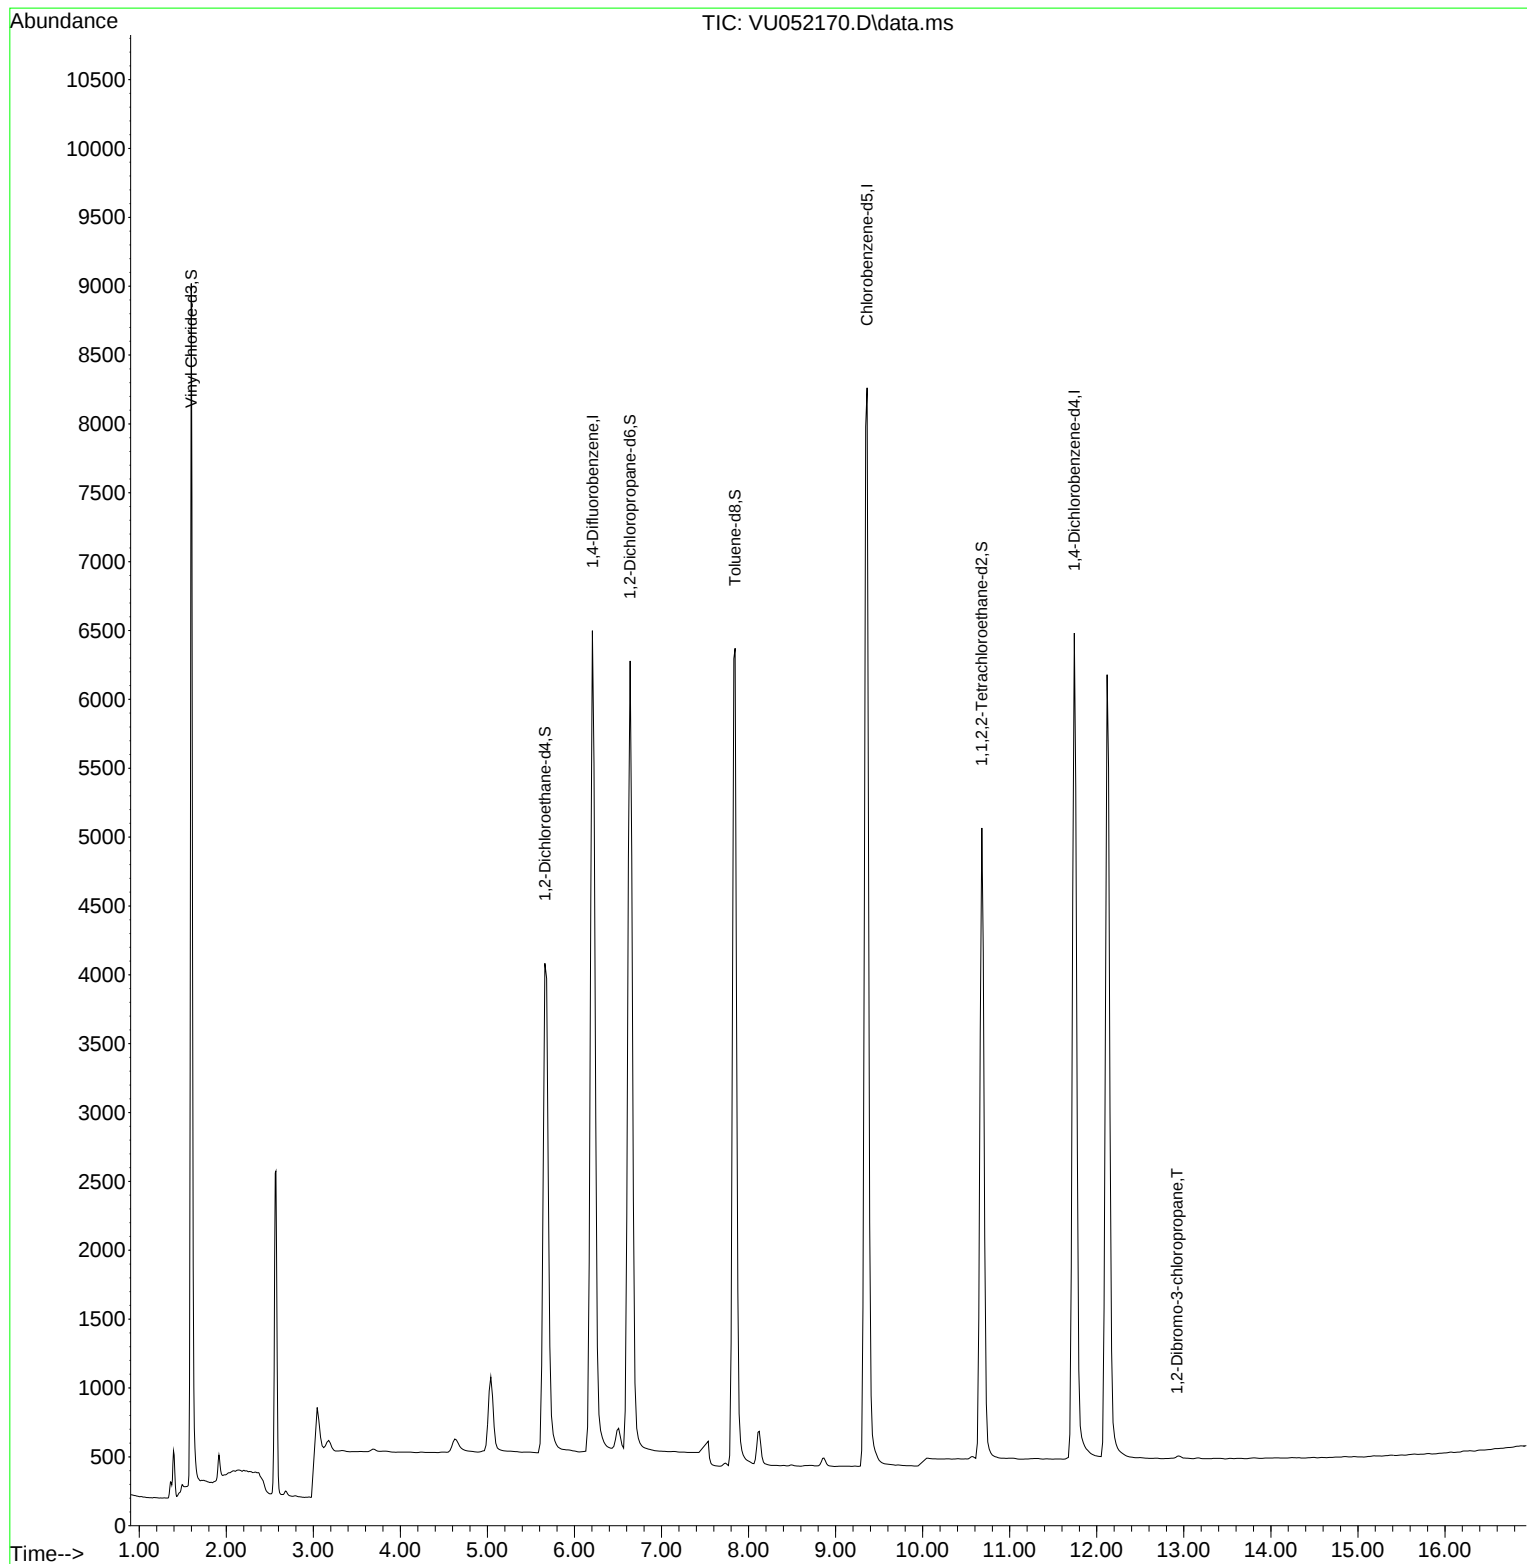

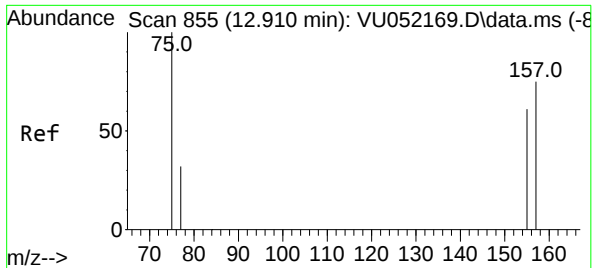

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.012 ug/L
 RT: 12.924 min Scan# 856
 Delta R.T. 0.014 min
 Lab File: VU052170.D
 Acq: 02 Dec 2022 10:42

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK008

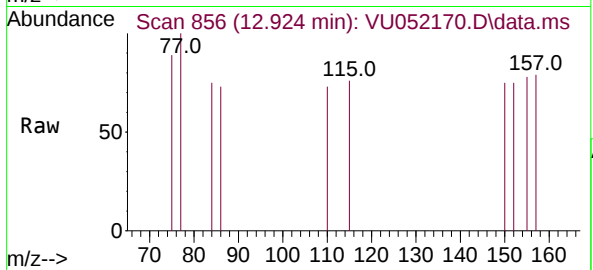

Tgt Ion: 75	Resp: 25
Ion Ratio	Lower Upper
75 100	
157 89.3	62.8 94.2
155 87.5	54.4 81.6#

