


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120222\
 Data File : VU052168.D
 Acq On : 02 Dec 2022 09:08
 Operator : JC/MD
 Sample : BFB008
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB008

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Dec 02 00:27:38 2022

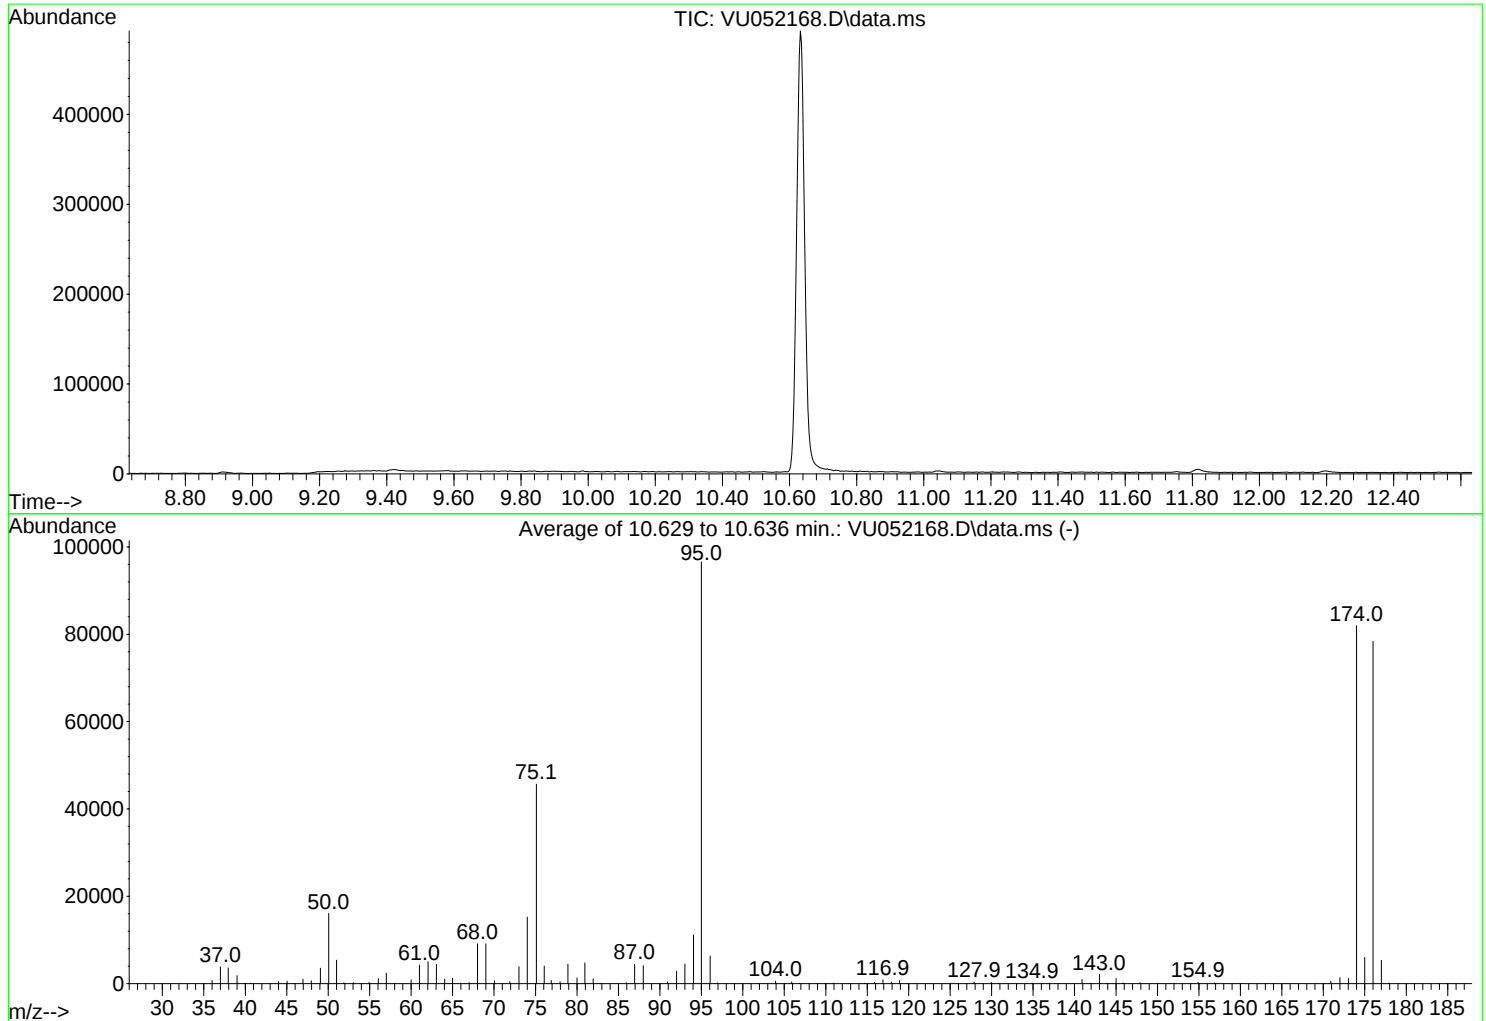

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	16080	PASS
75	95	30	80	47.3	45656	PASS
95	95	100	100	100.0	96587	PASS
96	95	5	9	6.6	6345	PASS
173	174	0.00	2	1.4	1175	PASS
174	95	50	120	84.8	81952	PASS
175	174	5	9	7.3	6013	PASS
176	174	95	101	95.7	78397	PASS
177	176	5	9	6.8	5348	PASS

m/z	Abundance
36.00	1239.0
37.00	106.0
37.90	320.0
39.90	269.0
44.00	483.0

Instrument :
MSVOA_U
ClientSampleId :
BFB008

m/z	Abundance
36.00	1941.0
37.00	3886.0
38.00	3830.0
39.00	1769.0
39.90	276.0
40.60	184.0
44.00	1008.0
45.10	579.0
45.90	143.0
47.00	1136.0
47.90	677.0
49.10	3369.0
50.10	15976.0
51.00	5356.0
51.90	237.0
53.00	208.0
54.90	321.0
56.10	1156.0
57.00	2296.0
58.10	116.0
60.00	954.0
61.00	4097.0
62.00	5052.0
63.10	4386.0
64.00	1134.0
65.00	1210.0
65.90	110.0
67.00	259.0
68.00	8961.0
69.00	8712.0
70.10	618.0
71.90	356.0
73.00	3852.0
74.00	14822.0
75.10	45080.0
76.10	3917.0
76.90	739.0
78.00	389.0
78.90	4378.0
80.00	1209.0
81.00	4714.0
82.00	1055.0
82.80	105.0
85.90	212.0
86.90	4285.0
88.00	3936.0
90.90	364.0
92.00	2584.0
93.00	4444.0
94.10	11039.0
95.00	94592.0
96.10	6524.0
96.90	183.0
104.00	501.0
105.90	464.0
106.90	112.0
108.00	112.0
109.90	107.0
110.90	131.0
112.70	103.0
114.70	116.0
115.80	262.0
116.90	894.0
117.90	337.0
118.90	729.0
127.90	349.0
130.00	254.0
130.80	104.0
134.90	158.0
136.90	115.0
140.90	829.0
141.90	114.0
143.00	2109.0
143.90	128.0
145.00	1140.0
145.80	141.0
147.90	223.0
150.00	112.0
154.90	277.0
156.90	152.0
170.90	494.0
172.00	1426.0
173.00	1073.0
174.00	77888.0
175.00	5771.0
176.00	74736.0
177.00	5030.0
177.90	121.0

Instrument :
MSVOA_U
ClientSampleId :
BFB008

m/z	Abundance
36.00	2041.0
37.00	4076.0
38.00	4022.0
39.00	1901.0
40.00	360.0
40.60	157.0
44.00	933.0
45.10	625.0
45.90	117.0
47.00	1084.0
48.00	705.0
49.00	3689.0
50.00	16592.0
51.00	5550.0
51.90	243.0
53.10	250.0
55.00	331.0
56.00	1140.0
57.00	2460.0
58.00	101.0
60.00	895.0
61.00	4348.0
62.10	5170.0
63.00	4538.0
64.10	1026.0
65.00	1295.0
66.00	151.0
67.00	244.0
68.00	9453.0
69.00	9373.0
70.10	685.0
71.90	465.0
73.00	4028.0
74.00	15693.0
75.10	47048.0
76.10	4194.0
76.90	794.0
78.00	459.0
78.90	4578.0
80.00	1335.0
80.90	4876.0
81.90	1146.0
82.80	110.0
85.90	235.0
86.90	4548.0
88.00	4159.0
90.90	382.0
92.00	2931.0
93.00	4629.0
94.00	11461.0
95.00	99120.0
96.10	6529.0
97.00	198.0
103.90	576.0
105.90	421.0
106.80	101.0
110.90	157.0
114.70	122.0
115.80	293.0
116.90	921.0
117.90	387.0
118.90	768.0
127.90	386.0
129.90	313.0
130.80	114.0
134.90	137.0
137.00	128.0
140.90	947.0
141.90	130.0
143.00	2177.0
143.90	112.0
145.00	1250.0
145.80	173.0
147.90	248.0
154.90	314.0
156.90	182.0
170.90	540.0
172.00	1367.0
173.10	1187.0
174.00	84368.0
175.00	6154.0
176.00	80736.0
177.00	5427.0
177.90	157.0

Instrument :
MSVOA_U
ClientSampleId :
BFB008

m/z	Abundance
36.00	1905.0
37.00	3876.0
38.00	3867.0
39.00	1864.0
40.00	391.0
44.00	804.0
45.00	610.0
46.90	918.0
48.00	635.0
49.00	3613.0
50.00	15673.0
51.00	5262.0
51.90	208.0
53.10	251.0
55.00	285.0
56.00	1089.0
57.00	2381.0
60.00	762.0
61.00	4162.0
62.10	4877.0
63.00	4311.0
64.10	926.0
65.00	1256.0
66.00	152.0
67.00	208.0
68.00	8942.0
69.00	9309.0
70.00	692.0
71.90	494.0
73.00	3765.0
74.00	15234.0
75.10	44840.0
76.00	4017.0
76.90	711.0
77.90	502.0
78.90	4425.0
80.00	1401.0
80.90	4702.0
81.90	1141.0
86.00	250.0
87.00	4380.0
88.00	4273.0
90.90	359.0
92.00	3115.0
93.00	4451.0
94.10	10882.0
95.00	96048.0
96.00	5983.0
97.00	197.0
103.90	566.0
105.90	327.0
108.00	105.0
110.90	128.0
114.70	112.0
115.90	281.0
116.90	840.0
117.90	415.0
118.90	751.0
127.90	392.0
129.90	347.0
134.90	103.0
136.90	128.0
140.90	974.0
141.90	138.0
143.00	2060.0
145.00	1176.0
145.90	190.0
147.90	229.0
150.00	100.0
154.90	317.0
156.90	198.0
170.90	577.0
172.00	1331.0
173.10	1266.0
174.00	83600.0
175.00	6114.0
176.00	79720.0
177.00	5586.0
177.90	157.0

Instrument :
MSVOA_U
ClientSampleId :
BFB008