


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU120318\
Data File : VU028427.D
Acq On : 03 Dec 2018 08:55
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U112818W.M
Title : SW846 8260
Last Update : Thu Nov 29 01:04:49 2018

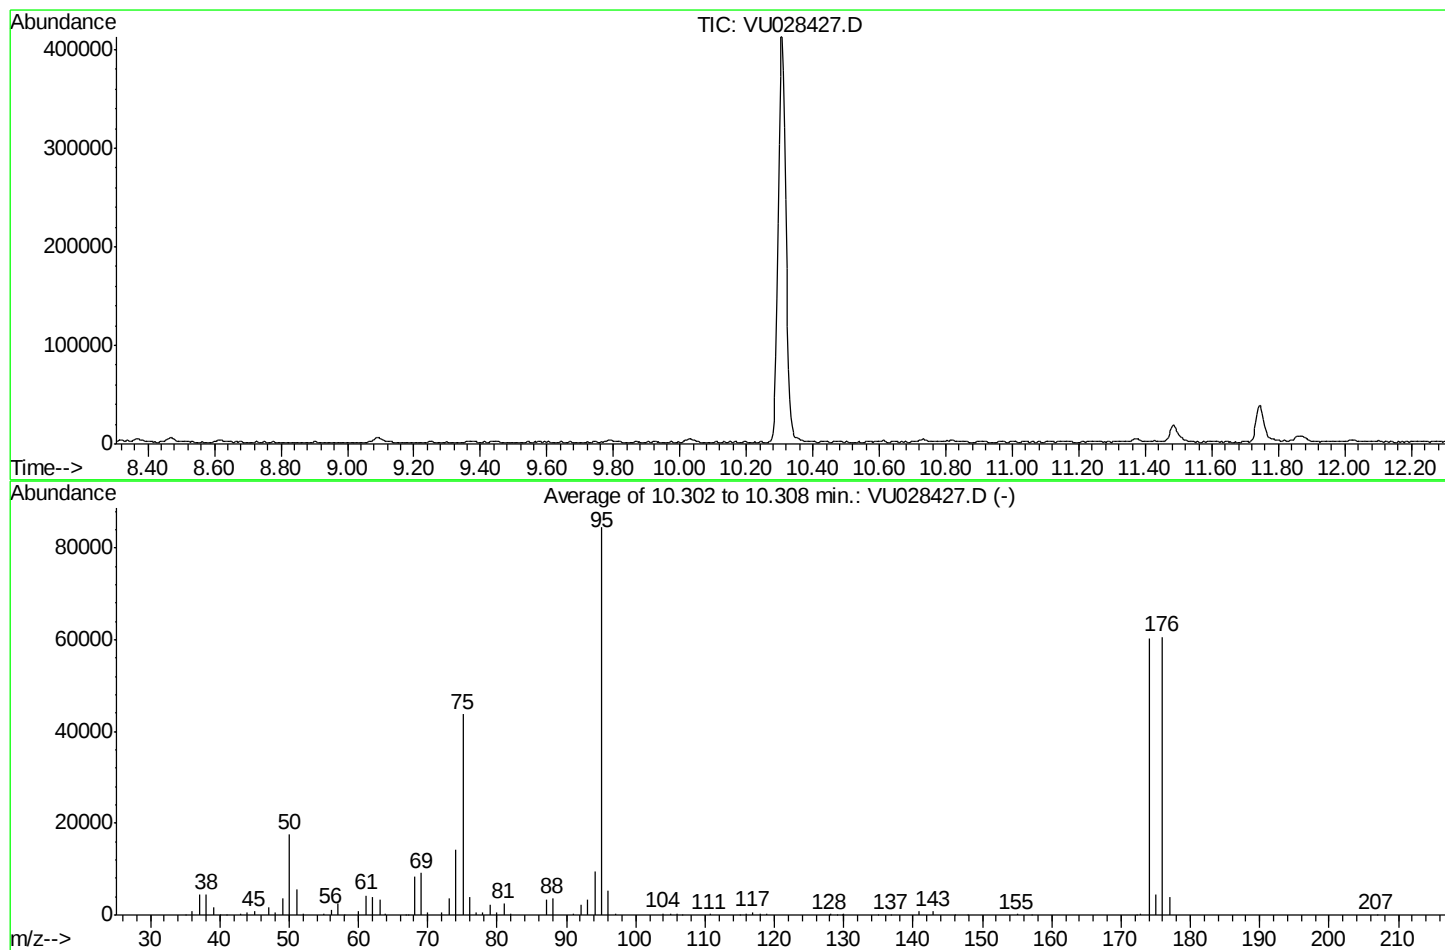

AutoFind: Scans 2839, 2840, 2841; Background Corrected with Scan 2826

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	17460	PASS
75	95	30	60	51.7	43698	PASS
95	95	100	100	100.0	84525	PASS
96	95	5	9	6.3	5311	PASS
173	174	0.00	2	0.5	293	PASS
174	95	50	100	71.2	60173	PASS
175	174	5	9	7.6	4567	PASS
176	174	95	101	100.8	60666	PASS
177	176	5	9	6.5	3947	PASS