


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU120319\
 Data File : VU035938.D
 Acq On : 03 Dec 2019 09:24
 Operator : JC/SP
 Sample : BFB10
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB10

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR120319WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Dec 04 03:35:54 2019

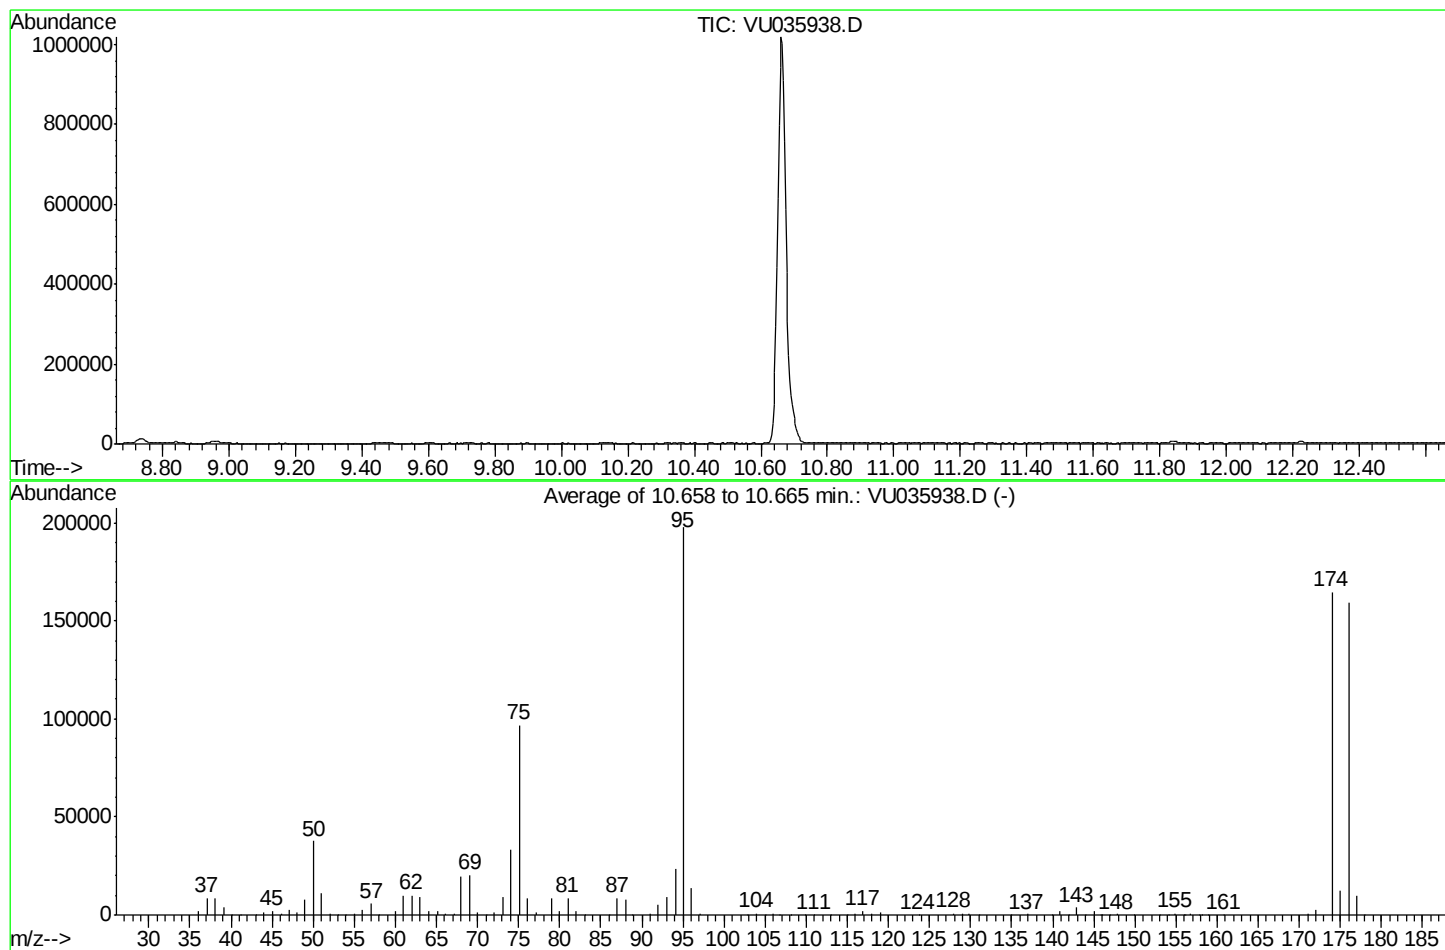

AutoFind: Scans 2898, 2899, 2900; Background Corrected with Scan 2883

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	37589	PASS
75	95	30	80	49.0	96898	PASS
95	95	100	100	100.0	197674	PASS
96	95	5	9	7.0	13772	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	83.3	164650	PASS
175	174	5	9	7.6	12445	PASS
176	174	95	101	96.8	159360	PASS
177	176	5	9	6.3	9982	PASS

m/z	Abundance
36.10	1647.0
37.10	8541.0
38.00	8111.0
39.10	3444.0
40.10	642.0
41.10	163.0
42.90	102.0
44.00	2425.0
45.00	1951.0
46.10	430.0
47.10	2540.0
48.00	1245.0
49.00	7658.0
50.10	36280.0
51.00	10921.0
52.10	487.0
53.10	291.0
54.00	186.0
54.90	633.0
56.00	2775.0
57.00	5633.0
57.90	151.0
60.00	2128.0
61.00	9037.0
62.00	9652.0
63.00	8745.0
64.00	1942.0
65.10	1640.0
66.10	393.0
67.10	438.0
68.00	18368.0
69.00	19720.0
70.10	1464.0
71.10	110.0
72.00	1177.0
73.00	8680.0
74.00	31648.0
75.10	92952.0
76.10	7697.0
77.10	1294.0
79.00	8309.0
79.90	2245.0
81.00	8675.0
81.90	1731.0
83.00	188.0
86.00	265.0
87.00	8595.0
88.00	7961.0
88.80	196.0
91.00	955.0
92.00	5086.0
93.10	9377.0
94.10	22408.0
95.00	187520.0
96.00	13298.0
97.00	534.0
102.70	114.0
104.00	817.0
105.00	239.0
106.00	699.0
106.80	176.0
108.20	162.0
110.90	132.0
113.00	186.0
115.00	155.0
116.00	824.0
116.90	2078.0
117.90	840.0
119.00	1510.0
123.70	119.0
128.00	759.0
129.00	373.0
129.80	536.0
131.00	281.0
134.90	355.0
137.00	297.0
139.90	106.0
140.90	1602.0
142.00	361.0
142.90	3749.0
144.00	219.0
145.00	1937.0
145.80	272.0
147.00	186.0
147.80	447.0
149.90	140.0
153.00	153.0
154.10	191.0
154.90	690.0
155.90	181.0
156.80	404.0
157.80	106.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10

158.10	112.0
158.90	230.0
160.90	282.0
171.00	823.0
172.00	2397.0
174.00	154944.0
175.00	12027.0
176.00	150848.0
176.90	9251.0
177.90	265.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10

m/z	Abundance
36.10	1782.0
37.10	8831.0
38.00	8663.0
39.10	3890.0
40.20	654.0
41.10	201.0
44.00	2486.0
45.00	2068.0
46.10	482.0
47.10	2989.0
48.00	1485.0
49.00	8395.0
50.10	38576.0
51.00	11844.0
52.10	457.0
53.10	329.0
54.00	181.0
54.90	622.0
56.00	2943.0
57.00	6055.0
58.00	169.0
60.00	2254.0
61.00	9754.0
62.00	10236.0
63.00	9817.0
64.00	1816.0
65.10	1763.0
66.10	366.0
67.10	432.0
68.00	20008.0
69.00	20816.0
70.00	1622.0
71.00	135.0
72.00	1197.0
73.00	9273.0
74.00	34024.0
75.00	99472.0
76.10	8608.0
77.10	1284.0
79.00	8765.0
79.90	2362.0
81.00	8778.0
81.90	1732.0
83.10	207.0
85.90	277.0
87.00	9038.0
88.00	8442.0
88.90	152.0
91.00	974.0
92.00	5392.0
93.10	9784.0
94.10	23960.0
95.00	203648.0
96.10	14221.0
97.00	511.0
102.80	122.0
104.00	963.0
105.00	239.0
106.00	833.0
106.80	323.0
108.10	133.0
111.00	160.0
113.00	201.0
115.00	163.0
116.00	862.0
116.90	2083.0
117.90	862.0
119.00	1584.0
128.00	761.0
129.10	395.0
129.80	681.0
131.00	339.0
135.00	318.0
136.90	400.0
139.90	153.0
140.90	1672.0
142.00	329.0
142.90	3816.0
144.00	307.0
145.00	1981.0
145.80	280.0
147.00	185.0
147.90	497.0
149.80	179.0
153.00	206.0
154.10	107.0
154.90	722.0
156.10	168.0
156.80	522.0
157.80	135.0
158.90	314.0
160.80	288.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10

171.00	777.0
172.00	2809.0
174.00	169984.0
175.00	12568.0
176.00	164864.0
177.00	10286.0
177.90	322.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10

m/z	Abundance
36.00	1617.0
37.10	8325.0
38.00	8172.0
39.10	4038.0
40.20	633.0
41.10	191.0
43.00	110.0
44.00	2289.0
45.00	1976.0
46.10	437.0
47.10	2994.0
48.00	1506.0
49.00	8268.0
50.10	37912.0
51.00	11309.0
52.00	468.0
53.00	359.0
54.00	123.0
55.00	642.0
56.00	2933.0
57.10	5849.0
58.00	183.0
60.00	2145.0
61.00	9836.0
62.00	10148.0
63.00	9800.0
64.00	1670.0
65.10	1858.0
66.00	344.0
67.10	455.0
68.00	19816.0
69.10	20224.0
70.00	1676.0
71.00	104.0
72.10	1114.0
73.10	9686.0
74.10	33664.0
75.00	98272.0
76.10	8442.0
77.10	1114.0
79.00	8353.0
79.90	2284.0
81.00	8385.0
82.00	1599.0
83.10	240.0
85.90	290.0
87.00	8562.0
88.00	8110.0
88.90	106.0
91.00	861.0
92.00	5418.0
93.00	9173.0
94.10	23328.0
95.00	201856.0
96.10	13798.0
97.10	417.0
102.90	147.0
104.00	936.0
104.90	231.0
106.00	850.0
106.80	347.0
108.00	106.0
109.90	110.0
110.90	221.0
113.00	202.0
115.00	151.0
115.90	833.0
116.90	1788.0
117.90	841.0
119.00	1492.0
127.90	691.0
129.10	351.0
129.80	716.0
131.00	344.0
135.00	285.0
136.80	439.0
139.90	161.0
140.90	1739.0
142.00	251.0
142.90	3512.0
144.00	342.0
145.00	1875.0
146.00	271.0
146.90	142.0
147.90	491.0
149.80	220.0
152.90	278.0
154.90	681.0
156.80	500.0
157.80	155.0
158.90	300.0
160.80	240.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10

171.00	800.0
172.00	2994.0
174.00	169024.0
175.00	12742.0
176.00	162368.0
176.90	10411.0
177.90	339.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10

Scan 2883 (10.610 min): VU035938.D
BFB10

m/z	Abundance
40.00	548.0
44.00	1387.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10