


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU120320\
Data File : VU041448.D
Acq On : 03 Dec 2020 09:54
Operator : SY/MD
Sample : BFB18
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB18

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR120320WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Dec 04 03:11:16 2020

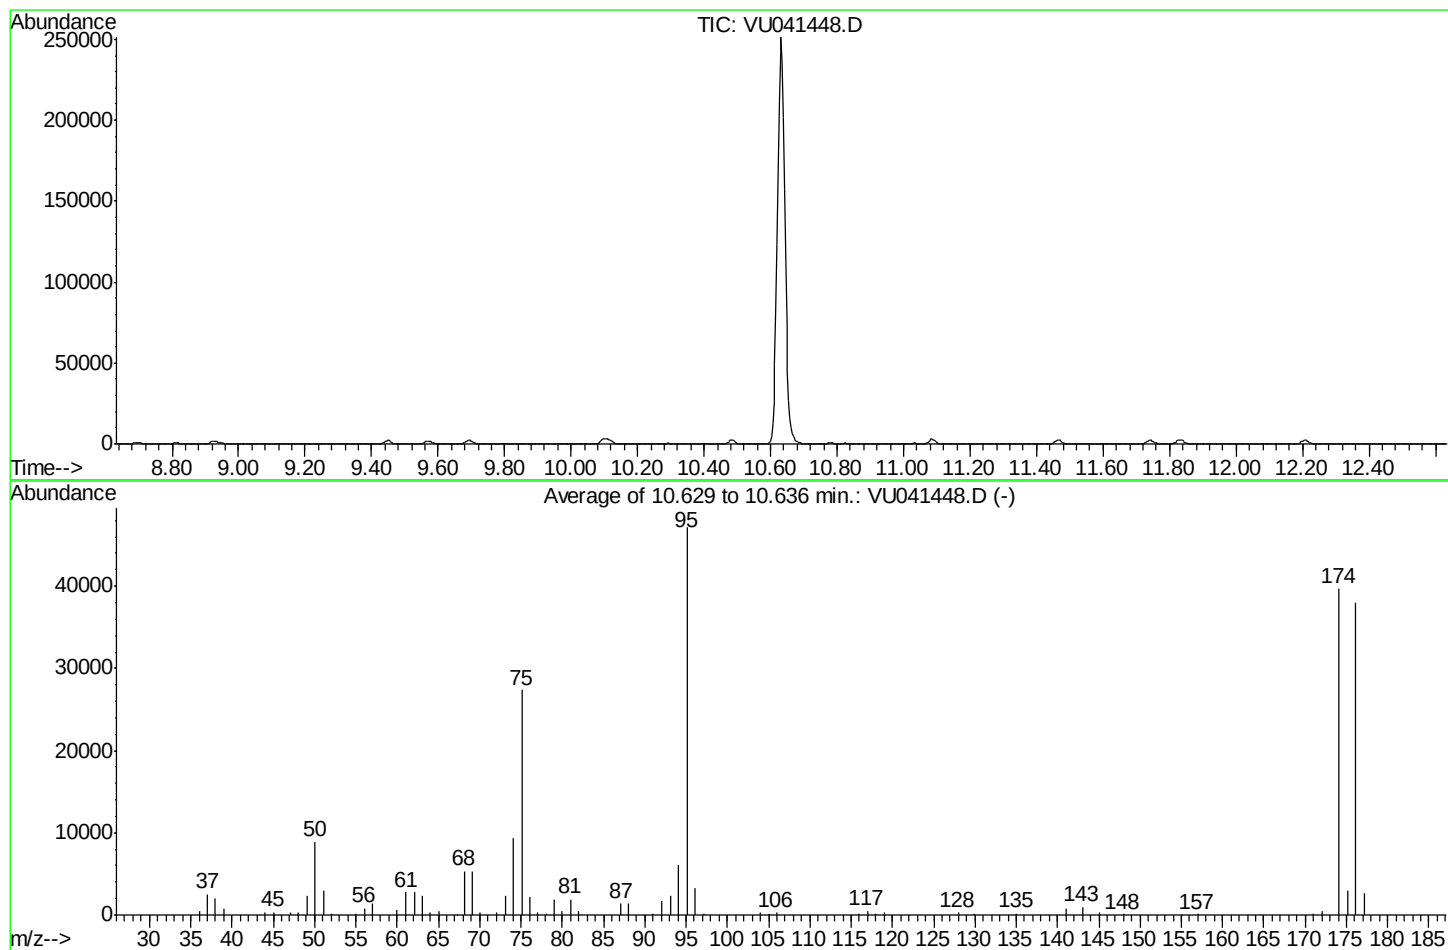

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	8916	PASS
75	95	30	80	58.0	27346	PASS
95	95	100	100	100.0	47157	PASS
96	95	5	9	7.0	3304	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.0	39634	PASS
175	174	5	9	7.4	2952	PASS
176	174	95	101	95.7	37938	PASS
177	176	5	9	6.8	2574	PASS