

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
 Data File : VU046068.D
 Acq On : 03 Dec 2021 12:16
 Operator : SY/MD
 Sample : VU1203MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK045

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046068.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	92	rVB	102011	108831	12.48%	1.535%
2	1.919	171	180	194	rVB	79549	102683	11.78%	1.448%
3	2.195	263	266	268	rBV	270	194	0.02%	0.003%
4	2.504	359	362	369	rBV2	284	299	0.03%	0.004%
5	2.572	371	383	414	rBV	170902	288857	33.13%	4.074%
6	2.758	437	441	445	rBV	155	137	0.02%	0.002%
7	2.800	445	454	464	rVV	992	1406	0.16%	0.020%
8	3.051	524	532	545	rVB2	1310	2257	0.26%	0.032%
9	3.356	623	627	628	rBV2	232	181	0.02%	0.003%
10	3.404	637	642	647	rBV	194	309	0.04%	0.004%
11	3.475	655	664	666	rBV	187	318	0.04%	0.004%
12	3.520	672	678	680	rBV	160	180	0.02%	0.003%
13	3.678	724	727	732	rBB	138	158	0.02%	0.002%
14	3.797	761	764	768	rVB	171	152	0.02%	0.002%
15	3.832	773	775	781	rBB	141	165	0.02%	0.002%
16	3.867	782	786	788	rBV	162	152	0.02%	0.002%
17	3.903	793	797	800	rBV	149	166	0.02%	0.002%
18	4.009	827	830	833	rVB	214	161	0.02%	0.002%
19	4.189	882	886	888	rBB	145	124	0.01%	0.002%
20	4.260	906	908	912	rVB	187	150	0.02%	0.002%
21	4.285	912	916	918	rBV	156	153	0.02%	0.002%
22	4.330	926	930	934	rBB	178	186	0.02%	0.003%
23	4.382	942	946	948	rBV	139	143	0.02%	0.002%
24	4.481	971	977	979	rBV	140	196	0.02%	0.003%
25	4.642	1009	1027	1064	rBV	78189	250782	28.77%	3.537%
26	4.957	1121	1125	1127	rBV	156	156	0.02%	0.002%
27	5.006	1136	1140	1143	rBV2	395	286	0.03%	0.004%
28	5.067	1143	1159	1180	rVV	157740	348145	39.93%	4.910%
29	5.295	1226	1230	1234	rBV2	489	424	0.05%	0.006%
30	5.436	1270	1274	1279	rBV	159	208	0.02%	0.003%
31	5.497	1290	1293	1296	rBV	166	149	0.02%	0.002%
32	5.575	1311	1317	1320	rBV	157	228	0.03%	0.003%
33	5.613	1326	1329	1333	rBB	134	142	0.02%	0.002%
34	5.729	1343	1365	1387	rBV2	323276	871787	100.00%	12.295%
35	5.989	1444	1446	1450	rBV	194	180	0.02%	0.003%
36	6.038	1458	1461	1464	rBV	193	183	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
 Data File : VU046068.D
 Acq On : 03 Dec 2021 12:16
 Operator : SY/MD
 Sample : VU1203MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK045

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	6.118	1483	1486	1489	rVV2	226	191	0.02%	0.003%
38	6.253	1513	1528	1548	rBV	297465	559346	64.16%	7.889%
39	6.401	1570	1574	1579	rVB2	377	314	0.04%	0.004%
40	6.533	1603	1615	1628	rBV5	5720	12546	1.44%	0.177%
41	6.694	1650	1665	1683	rBV	201007	391300	44.88%	5.519%
42	6.948	1742	1744	1748	rBV	129	134	0.02%	0.002%
43	7.034	1769	1771	1774	rVV	183	161	0.02%	0.002%
44	7.054	1775	1777	1780	rVB2	357	188	0.02%	0.003%
45	7.185	1808	1818	1828	rVV3	2202	3628	0.42%	0.051%
46	7.240	1832	1835	1839	rVB	156	155	0.02%	0.002%
47	7.349	1866	1869	1872	rBV	140	135	0.02%	0.002%
48	7.404	1883	1886	1892	rVB2	153	125	0.01%	0.002%
49	7.568	1923	1937	1954	rVV	113001	196722	22.57%	2.774%
50	7.687	1968	1974	1983	rVB2	1580	2224	0.26%	0.031%
51	7.899	2027	2040	2056	rBV	395284	697348	79.99%	9.835%
52	8.182	2116	2128	2148	rBV	78032	128647	14.76%	1.814%
53	8.256	2148	2151	2153	rVV3	283	146	0.02%	0.002%
54	8.439	2204	2208	2210	rBV	196	126	0.01%	0.002%
55	8.636	2257	2269	2301	rBV	273471	503376	57.74%	7.099%
56	8.928	2357	2360	2362	rBV	268	147	0.02%	0.002%
57	9.160	2428	2432	2434	rBV2	191	172	0.02%	0.002%
58	9.420	2499	2513	2535	rBV	412581	699410	80.23%	9.864%
59	9.574	2553	2561	2571	rBV2	853	1191	0.14%	0.017%
60	9.636	2576	2580	2585	rBV2	442	482	0.06%	0.007%
61	9.700	2592	2600	2606	rBV	1340	1846	0.21%	0.026%
62	10.115	2718	2729	2737	rVB5	1359	2344	0.27%	0.033%
63	10.343	2794	2800	2803	rBV	124	127	0.01%	0.002%
64	10.417	2817	2823	2826	rBV	225	312	0.04%	0.004%
65	10.488	2838	2845	2853	rBV2	903	1055	0.12%	0.015%
66	10.671	2893	2902	2910	rVB3	1429	2031	0.23%	0.029%
67	10.758	2917	2929	2945	rBV	297010	480074	55.07%	6.771%
68	10.825	2948	2950	2953	rVB2	402	201	0.02%	0.003%
69	10.867	2958	2963	2969	rVV2	416	435	0.05%	0.006%
70	10.902	2971	2974	2978	rVV	219	225	0.03%	0.003%
71	11.092	3026	3033	3041	rBV	758	1201	0.14%	0.017%
72	11.285	3089	3093	3096	rBV	159	127	0.01%	0.002%
73	11.468	3140	3150	3161	rVB5	2105	3256	0.37%	0.046%
74	11.703	3220	3223	3230	rVB	445	359	0.04%	0.005%
75	11.751	3230	3238	3244	rBV3	1759	2139	0.25%	0.030%
76	11.816	3244	3258	3277	rBV	445297	708761	81.30%	9.996%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
 Data File : VU046068.D
 Acq On : 03 Dec 2021 12:16
 Operator : SY/MD
 Sample : VU1203MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK045

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.941	3292	3297	3301	rBV2	371	437	0.05%	0.006%
78	11.973	3303	3307	3315	rVB3	1049	1142	0.13%	0.016%
79	12.195	3363	3376	3393	rBV	418602	676130	77.56%	9.536%
80	12.996	3622	3625	3631	rVV2	447	307	0.04%	0.004%
81	13.115	3659	3662	3664	rBV	168	129	0.01%	0.002%
82	13.221	3687	3695	3704	rBV2	2470	3242	0.37%	0.046%
83	13.378	3742	3744	3750	rVB	223	130	0.01%	0.002%
84	13.481	3773	3776	3779	rBV2	191	127	0.01%	0.002%
85	13.497	3779	3781	3786	rVB	228	137	0.02%	0.002%
86	13.658	3829	3831	3836	rVB	265	149	0.02%	0.002%
87	13.844	3882	3889	3897	rBV3	4078	5539	0.64%	0.078%
88	14.089	3955	3965	3976	rBV	7236	11284	1.29%	0.159%
89	14.330	4031	4040	4050	rBV4	4284	6286	0.72%	0.089%
90	14.574	4112	4116	4120	rBV2	312	356	0.04%	0.005%
91	14.764	4173	4175	4178	rVB	337	132	0.02%	0.002%
92	14.889	4211	4214	4220	rVB	232	183	0.02%	0.003%
93	14.931	4224	4227	4229	rBV2	210	173	0.02%	0.002%
94	15.053	4261	4265	4269	rBV2	207	164	0.02%	0.002%
95	15.130	4286	4289	4292	rVB2	220	130	0.01%	0.002%
96	15.156	4292	4297	4300	rBV	282	304	0.03%	0.004%
97	15.301	4340	4342	4347	rVB2	485	324	0.04%	0.005%
98	15.327	4347	4350	4352	rBV2	303	237	0.03%	0.003%
99	15.651	4448	4451	4454	rBV3	294	193	0.02%	0.003%
100	15.806	4495	4499	4504	rBV2	252	287	0.03%	0.004%




Sum of corrected areas: 7090457

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
Data File : VU046068.D
Acq On : 03 Dec 2021 12:16
Operator : SY/MD
Sample : VU1203MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK045

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

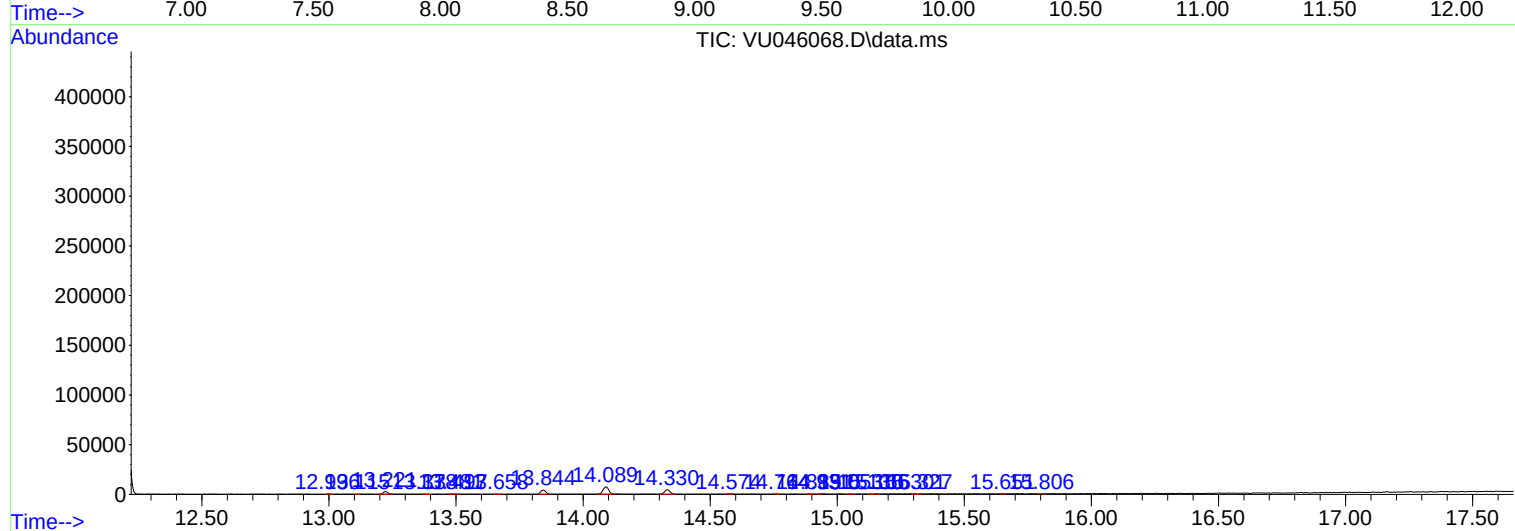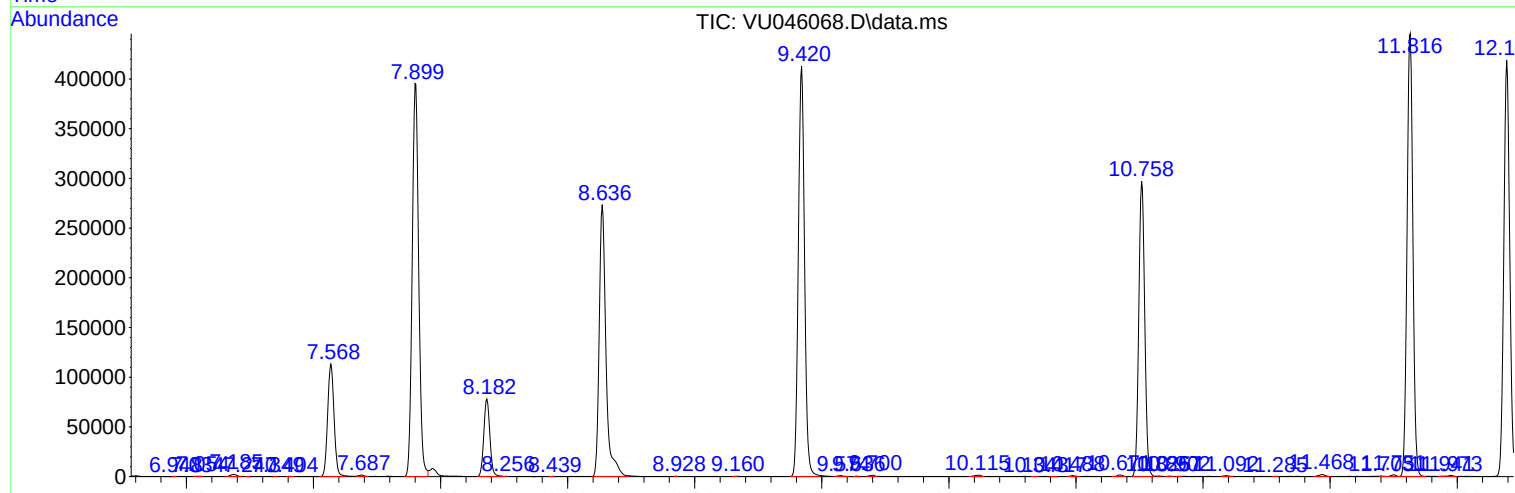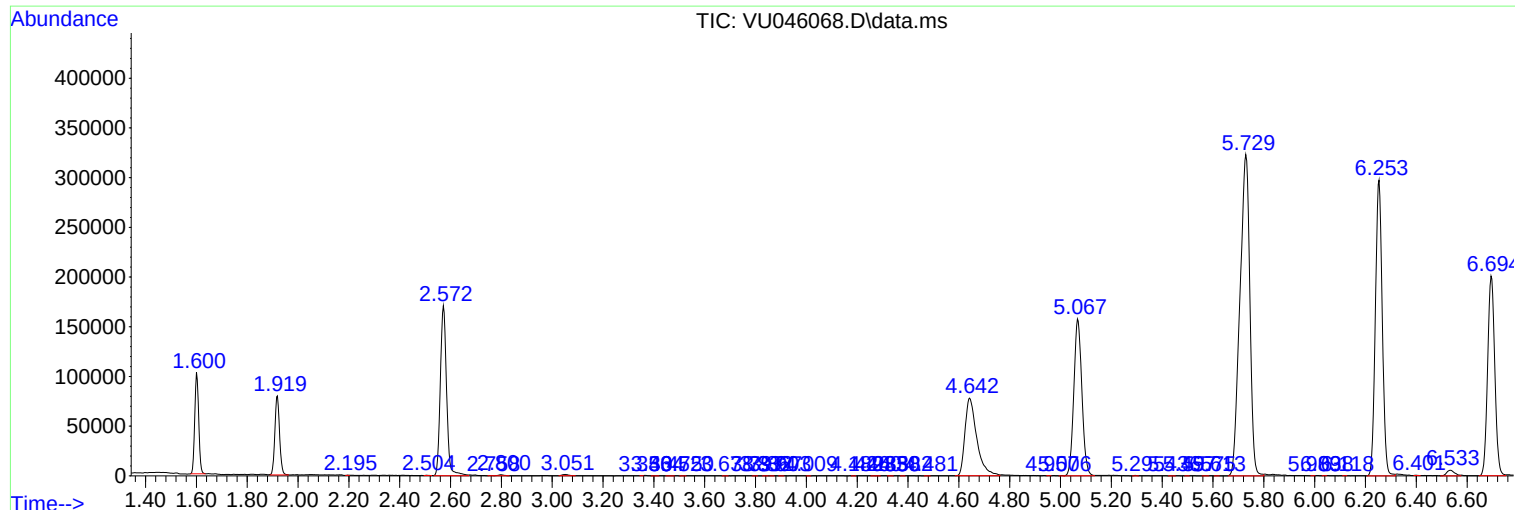

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
Data File : VU046068.D
Acq On : 03 Dec 2021 12:16
Operator : SY/MD
Sample : VU1203MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK045

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
Data File : VU046068.D
Acq On : 03 Dec 2021 12:16
Operator : SY/MD
Sample : VU1203MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK045

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc