

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
 Data File : VU046070.D
 Acq On : 03 Dec 2021 13:42
 Operator : SY/MD
 Sample : PB141130TB
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VLEB130

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046070.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	95	rBV	92406	101425	12.48%	1.576%
2	1.919	170	180	193	rBV	74439	95292	11.73%	1.481%
3	2.202	266	268	273	rVB	257	108	0.01%	0.002%
4	2.572	370	383	417	rBV	160243	269655	33.18%	4.191%
5	2.800	446	454	460	rVV	394	623	0.08%	0.010%
6	2.954	499	502	509	rVB	258	309	0.04%	0.005%
7	3.051	523	532	543	rBV3	3774	6830	0.84%	0.106%
8	3.125	551	555	557	rBV	155	155	0.02%	0.002%
9	3.189	563	575	589	rVB2	2118	4891	0.60%	0.076%
10	3.723	736	741	744	rBV	135	190	0.02%	0.003%
11	3.874	785	788	790	rBV	155	137	0.02%	0.002%
12	3.922	797	803	805	rBV	146	194	0.02%	0.003%
13	4.044	838	841	845	rBB	173	165	0.02%	0.003%
14	4.086	846	854	858	rBB	137	233	0.03%	0.004%
15	4.121	859	865	868	rBV	142	209	0.03%	0.003%
16	4.141	869	871	874	rVB	170	118	0.01%	0.002%
17	4.639	1009	1026	1064	rBV	78155	234363	28.84%	3.642%
18	4.903	1105	1108	1110	rBV	155	111	0.01%	0.002%
19	4.999	1134	1138	1139	rBB	218	110	0.01%	0.002%
20	5.067	1142	1159	1187	rBV	143572	325449	40.05%	5.058%
21	5.166	1187	1190	1193	rVV2	200	151	0.02%	0.002%
22	5.186	1193	1196	1199	rVB2	203	139	0.02%	0.002%
23	5.279	1223	1225	1229	rVV2	164	120	0.01%	0.002%
24	5.324	1236	1239	1246	rVB	113	120	0.01%	0.002%
25	5.404	1262	1264	1266	rBV	164	114	0.01%	0.002%
26	5.629	1330	1334	1337	rBV	187	207	0.03%	0.003%
27	5.729	1343	1365	1385	rBV2	299877	812665	100.00%	12.630%
28	5.854	1402	1404	1406	rBV2	319	159	0.02%	0.002%
29	5.973	1439	1441	1444	rBV2	181	139	0.02%	0.002%
30	6.034	1457	1460	1462	rBV	252	130	0.02%	0.002%
31	6.070	1468	1471	1472	rBV	144	104	0.01%	0.002%
32	6.105	1479	1482	1485	rVB2	226	104	0.01%	0.002%
33	6.121	1485	1487	1490	rVB	226	126	0.02%	0.002%
34	6.195	1508	1510	1512	rBV	230	118	0.01%	0.002%
35	6.253	1512	1528	1548	rBV	254998	479361	58.99%	7.450%
36	6.440	1583	1586	1593	rBV2	192	311	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
 Data File : VU046070.D
 Acq On : 03 Dec 2021 13:42
 Operator : SY/MD
 Sample : PB141130TB
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VLEB130

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	6.488	1599	1601	1604	rVB	420	206	0.03%	0.003%
38	6.533	1605	1615	1629	rBV3	7238	14530	1.79%	0.226%
39	6.694	1651	1665	1683	rBV	190853	368410	45.33%	5.726%
40	6.803	1697	1699	1704	rVB3	554	423	0.05%	0.007%
41	6.825	1704	1706	1710	rVB2	277	166	0.02%	0.003%
42	6.999	1755	1760	1761	rBV	163	170	0.02%	0.003%
43	7.044	1769	1774	1775	rBV	328	247	0.03%	0.004%
44	7.182	1810	1817	1831	rBV5	2321	3397	0.42%	0.053%
45	7.362	1869	1873	1874	rBV	156	133	0.02%	0.002%
46	7.568	1923	1937	1960	rBV	104993	181448	22.33%	2.820%
47	7.687	1967	1974	1984	rBV3	1323	2186	0.27%	0.034%
48	7.803	2007	2010	2015	rVB2	272	231	0.03%	0.004%
49	7.832	2016	2019	2025	rBV	160	246	0.03%	0.004%
50	7.899	2025	2040	2058	rBV	364216	651939	80.22%	10.132%
51	8.182	2116	2128	2144	rBV	71856	117241	14.43%	1.822%
52	8.269	2153	2155	2159	rVB	306	144	0.02%	0.002%
53	8.292	2159	2162	2165	rBV	211	153	0.02%	0.002%
54	8.340	2174	2177	2179	rBV	249	175	0.02%	0.003%
55	8.394	2191	2194	2200	rVB2	217	151	0.02%	0.002%
56	8.636	2256	2269	2302	rBV	251194	453484	55.80%	7.048%
57	9.038	2390	2394	2396	rBV	152	151	0.02%	0.002%
58	9.070	2400	2404	2407	rVV	176	152	0.02%	0.002%
59	9.160	2430	2432	2437	rVB2	171	132	0.02%	0.002%
60	9.420	2500	2513	2539	rBV	361393	600689	73.92%	9.335%
61	9.575	2556	2561	2564	rBV2	356	291	0.04%	0.005%
62	9.697	2593	2599	2606	rVB2	608	889	0.11%	0.014%
63	9.854	2641	2648	2651	rBV	105	143	0.02%	0.002%
64	9.973	2681	2685	2688	rBV	125	100	0.01%	0.002%
65	10.118	2728	2730	2733	rVB2	197	124	0.02%	0.002%
66	10.337	2796	2798	2801	rVB	242	110	0.01%	0.002%
67	10.362	2801	2806	2809	rBV	110	126	0.02%	0.002%
68	10.674	2895	2903	2912	rBV2	1556	2158	0.27%	0.034%
69	10.758	2916	2929	2947	rVB	276849	444264	54.67%	6.904%
70	10.864	2955	2962	2964	rBV2	329	282	0.03%	0.004%
71	10.899	2969	2973	2976	rBV	246	190	0.02%	0.003%
72	10.922	2978	2980	2984	rVB2	199	121	0.01%	0.002%
73	10.999	3002	3004	3009	rVB2	160	100	0.01%	0.002%
74	11.092	3030	3033	3036	rBV2	178	125	0.02%	0.002%
75	11.465	3141	3149	3151	rBV2	953	1262	0.16%	0.020%
76	11.697	3215	3221	3226	rVB2	724	803	0.10%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
 Data File : VU046070.D
 Acq On : 03 Dec 2021 13:42
 Operator : SY/MD
 Sample : PB141130TB
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VLEB130

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.726	3226	3230	3234	rBV	152	143	0.02%	0.002%
78	11.748	3234	3237	3241	rVV	201	146	0.02%	0.002%
79	11.812	3245	3257	3275	rVB	390642	610859	75.17%	9.494%
80	11.922	3289	3291	3293	rBV	180	100	0.01%	0.002%
81	11.976	3301	3308	3314	rVB4	1180	1380	0.17%	0.021%
82	12.195	3363	3376	3392	rVB	396124	634596	78.09%	9.862%
83	12.407	3440	3442	3448	rVB	235	128	0.02%	0.002%
84	12.854	3579	3581	3585	rVB2	216	130	0.02%	0.002%
85	13.102	3655	3658	3664	rVB	165	127	0.02%	0.002%
86	13.217	3692	3694	3697	rBV	220	132	0.02%	0.002%
87	13.404	3750	3752	3757	rVB2	239	187	0.02%	0.003%
88	13.774	3864	3867	3872	rBV2	201	181	0.02%	0.003%
89	13.848	3884	3890	3895	rVB3	599	731	0.09%	0.011%
90	13.999	3929	3937	3940	rBV	244	351	0.04%	0.005%
91	14.092	3960	3966	3973	rBV	809	1129	0.14%	0.018%
92	14.330	4039	4040	4046	rVB	439	355	0.04%	0.006%
93	14.700	4153	4155	4162	rVB2	299	191	0.02%	0.003%
94	14.938	4224	4229	4233	rBV2	189	192	0.02%	0.003%
95	15.143	4290	4293	4296	rBV2	342	217	0.03%	0.003%
96	15.256	4325	4328	4330	rBV	202	116	0.01%	0.002%
97	15.307	4339	4344	4346	rBV	351	300	0.04%	0.005%
98	15.713	4468	4470	4471	rBV	227	107	0.01%	0.002%
99	16.147	4602	4605	4607	rBV	302	154	0.02%	0.002%
100	16.970	4858	4861	4866	rBV4	598	612	0.08%	0.010%




Sum of corrected areas: 6434491

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
Data File : VU046070.D
Acq On : 03 Dec 2021 13:42
Operator : SY/MD
Sample : PB141130TB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VLEB130

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

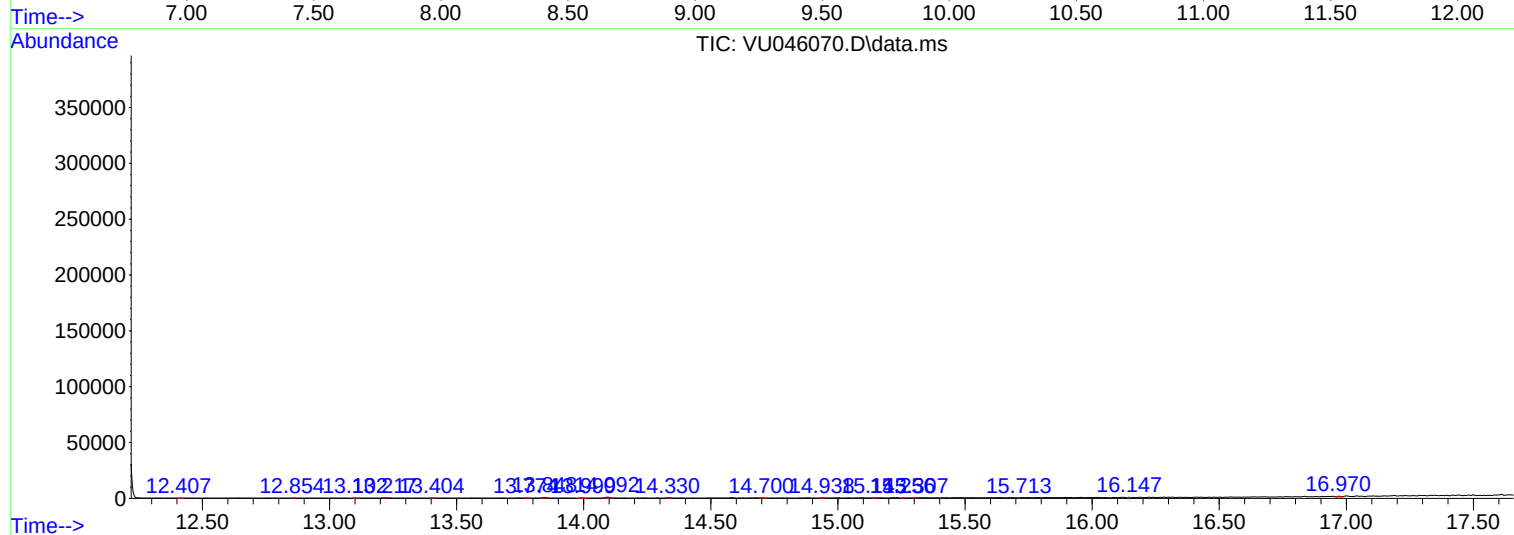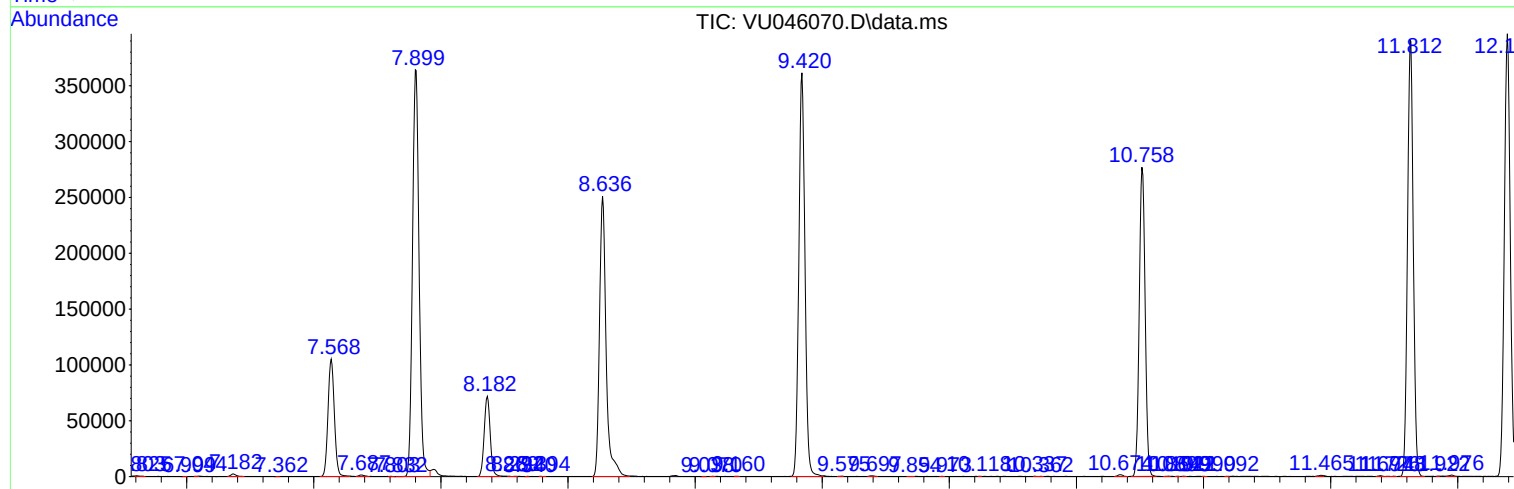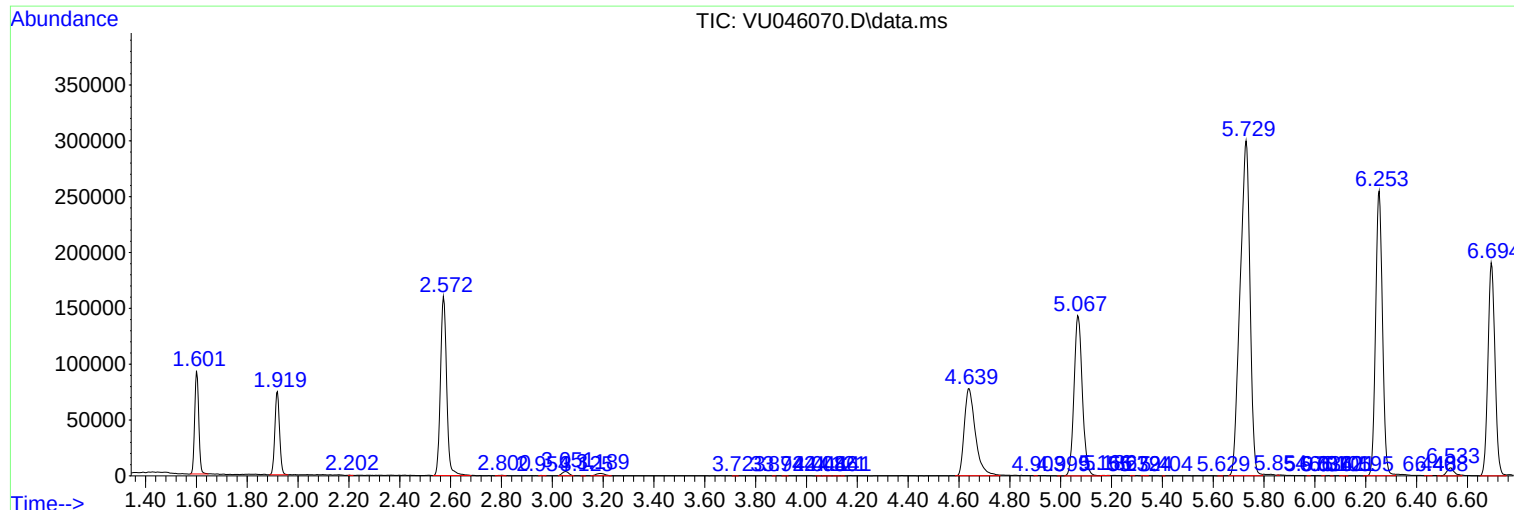

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
Data File : VU046070.D
Acq On : 03 Dec 2021 13:42
Operator : SY/MD
Sample : PB141130TB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VLEB130

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
Data File : VU046070.D
Acq On : 03 Dec 2021 13:42
Operator : SY/MD
Sample : PB141130TB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VLEB130

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc