

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
 Data File : VU046072.D
 Acq On : 03 Dec 2021 14:38
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK006

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046072.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	93	rVB	93281	102586	11.77%	1.430%
2	1.916	170	179	192	rBV	76122	98650	11.31%	1.376%
3	2.514	361	365	367	rBV	325	223	0.03%	0.003%
4	2.572	371	383	410	rBV	166417	280436	32.16%	3.910%
5	2.800	449	454	459	rBV	264	351	0.04%	0.005%
6	2.961	499	504	509	rBV	270	295	0.03%	0.004%
7	3.051	522	532	542	rVB	3967	6871	0.79%	0.096%
8	3.115	549	552	560	rBV2	191	174	0.02%	0.002%
9	3.186	563	574	588	rVV	3153	6339	0.73%	0.088%
10	3.411	639	644	646	rBV	272	234	0.03%	0.003%
11	3.482	662	666	670	rBV	160	225	0.03%	0.003%
12	3.629	709	712	715	rBV	184	180	0.02%	0.003%
13	3.793	759	763	770	rBB	149	246	0.03%	0.003%
14	4.350	929	936	941	rBB	154	263	0.03%	0.004%
15	4.395	947	950	953	rBV	199	192	0.02%	0.003%
16	4.636	1006	1025	1059	rBV2	92474	269167	30.87%	3.753%
17	5.067	1143	1159	1183	rVV	154525	347825	39.89%	4.850%
18	5.295	1226	1230	1233	rVB2	411	382	0.04%	0.005%
19	5.498	1290	1293	1297	rVV2	292	256	0.03%	0.004%
20	5.729	1342	1365	1388	rBV2	319203	871917	100.00%	12.158%
21	5.890	1412	1415	1422	rBV2	234	247	0.03%	0.003%
22	5.999	1447	1449	1451	rVB2	432	218	0.03%	0.003%
23	6.047	1459	1464	1467	rVB2	310	350	0.04%	0.005%
24	6.144	1490	1494	1496	rBV	266	199	0.02%	0.003%
25	6.253	1513	1528	1552	rBV	272375	520060	59.65%	7.252%
26	6.533	1605	1615	1638	rVB3	6538	13552	1.55%	0.189%
27	6.694	1651	1665	1683	rBV	209645	398680	45.72%	5.559%
28	6.806	1698	1700	1704	rVB2	735	488	0.06%	0.007%
29	6.935	1733	1740	1742	rBB	271	245	0.03%	0.003%
30	6.977	1751	1753	1758	rVB	189	170	0.02%	0.002%
31	7.047	1769	1775	1781	rVB2	323	396	0.05%	0.006%
32	7.124	1794	1799	1805	rBB	159	233	0.03%	0.003%
33	7.186	1808	1818	1830	rVB3	2243	4204	0.48%	0.059%
34	7.288	1844	1850	1855	rBV	186	297	0.03%	0.004%
35	7.433	1888	1895	1897	rBV	251	262	0.03%	0.004%
36	7.568	1924	1937	1950	rBV	116686	198619	22.78%	2.770%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
 Data File : VU046072.D
 Acq On : 03 Dec 2021 14:38
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK006

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.687	1967	1974	1984	rVB2	1598	2693	0.31%	0.038%
38	7.803	2005	2010	2013	rBV	295	257	0.03%	0.004%
39	7.899	2026	2040	2057	rBV	399329	700085	80.29%	9.762%
40	8.083	2095	2097	2100	rVB2	316	211	0.02%	0.003%
41	8.179	2116	2127	2147	rBV	79692	132245	15.17%	1.844%
42	8.250	2147	2149	2155	rVB3	382	346	0.04%	0.005%
43	8.430	2202	2205	2207	rBV	244	167	0.02%	0.002%
44	8.636	2255	2269	2300	rBV	290625	523906	60.09%	7.305%
45	8.819	2322	2326	2331	rVB	240	186	0.02%	0.003%
46	8.912	2349	2355	2364	rVV3	1150	1949	0.22%	0.027%
47	9.420	2499	2513	2537	rBV	393900	657476	75.41%	9.168%
48	9.575	2554	2561	2567	rVB2	649	887	0.10%	0.012%
49	9.694	2591	2598	2608	rVB2	1467	2354	0.27%	0.033%
50	10.112	2720	2728	2730	rBV3	571	759	0.09%	0.011%
51	10.671	2893	2902	2909	rBV3	1671	2311	0.27%	0.032%
52	10.758	2917	2929	2950	rBV	305155	495151	56.79%	6.904%
53	10.870	2957	2964	2966	rBV	247	305	0.03%	0.004%
54	10.999	2999	3004	3008	rBV2	367	441	0.05%	0.006%
55	11.118	3033	3041	3048	rVB6	2409	3499	0.40%	0.049%
56	11.237	3075	3078	3080	rBV2	239	167	0.02%	0.002%
57	11.295	3092	3096	3098	rBV	278	179	0.02%	0.002%
58	11.372	3117	3120	3124	rBV	219	180	0.02%	0.003%
59	11.414	3129	3133	3134	rBV2	439	274	0.03%	0.004%
60	11.459	3139	3147	3148	rBV3	1627	1409	0.16%	0.020%
61	11.697	3215	3221	3228	rVB4	1051	1368	0.16%	0.019%
62	11.812	3243	3257	3272	rBV	444638	689192	79.04%	9.610%
63	11.915	3282	3289	3291	rBV4	645	581	0.07%	0.008%
64	11.973	3303	3307	3314	rVB3	977	1160	0.13%	0.016%
65	12.060	3324	3334	3347	rBV4	3672	7213	0.83%	0.101%
66	12.121	3351	3353	3357	rVV2	658	434	0.05%	0.006%
67	12.150	3359	3362	3363	rVV	451	279	0.03%	0.004%
68	12.195	3363	3376	3394	rVV	448264	707756	81.17%	9.869%
69	12.327	3409	3417	3427	rVB4	4347	6202	0.71%	0.086%
70	12.401	3436	3440	3443	rBV3	462	328	0.04%	0.005%
71	12.523	3474	3478	3481	rVV3	309	286	0.03%	0.004%
72	12.545	3481	3485	3488	rVV3	597	518	0.06%	0.007%
73	12.562	3488	3490	3496	rVB	267	202	0.02%	0.003%
74	12.899	3592	3595	3600	rBV	211	169	0.02%	0.002%
75	13.385	3742	3746	3750	rBV2	196	163	0.02%	0.002%
76	13.436	3754	3762	3767	rBV2	1290	1535	0.18%	0.021%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
 Data File : VU046072.D
 Acq On : 03 Dec 2021 14:38
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK006

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	13.652	3820	3829	3843	rVB4	2394	4056	0.47%	0.057%
78	13.835	3884	3886	3895	rVV3	383	504	0.06%	0.007%
79	13.986	3929	3933	3935	rVV	384	230	0.03%	0.003%
80	14.089	3955	3965	3979	rVB	20682	31903	3.66%	0.445%
81	14.201	3997	4000	4002	rBV2	390	259	0.03%	0.004%
82	14.282	4023	4025	4029	rBV	309	165	0.02%	0.002%
83	14.333	4035	4041	4044	rVB3	300	349	0.04%	0.005%
84	14.423	4064	4069	4073	rBV	573	658	0.08%	0.009%
85	14.571	4110	4115	4117	rBV	282	281	0.03%	0.004%
86	14.619	4128	4130	4134	rVB	292	169	0.02%	0.002%
87	14.697	4151	4154	4157	rVB	397	271	0.03%	0.004%
88	14.816	4188	4191	4195	rVB2	434	325	0.04%	0.005%
89	14.864	4202	4206	4211	rVB2	430	412	0.05%	0.006%
90	14.889	4211	4214	4216	rBV	361	249	0.03%	0.003%
91	14.986	4241	4244	4247	rBV2	277	212	0.02%	0.003%
92	15.060	4261	4267	4269	rBV2	374	363	0.04%	0.005%
93	15.137	4288	4291	4294	rVB2	310	195	0.02%	0.003%
94	15.169	4296	4301	4305	rBV2	425	418	0.05%	0.006%
95	15.224	4307	4318	4331	rVB	21657	32534	3.73%	0.454%
96	15.410	4367	4376	4390	rBV	9829	15053	1.73%	0.210%
97	15.954	4538	4545	4554	rVB2	4743	6866	0.79%	0.096%
98	16.140	4598	4603	4613	rVB5	1349	1829	0.21%	0.026%
99	16.262	4635	4641	4648	rVB7	1795	2269	0.26%	0.032%
100	16.407	4682	4686	4693	rBV5	1917	2115	0.24%	0.029%




Sum of corrected areas: 7171540

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
Data File : VU046072.D
Acq On : 03 Dec 2021 14:38
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK006

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

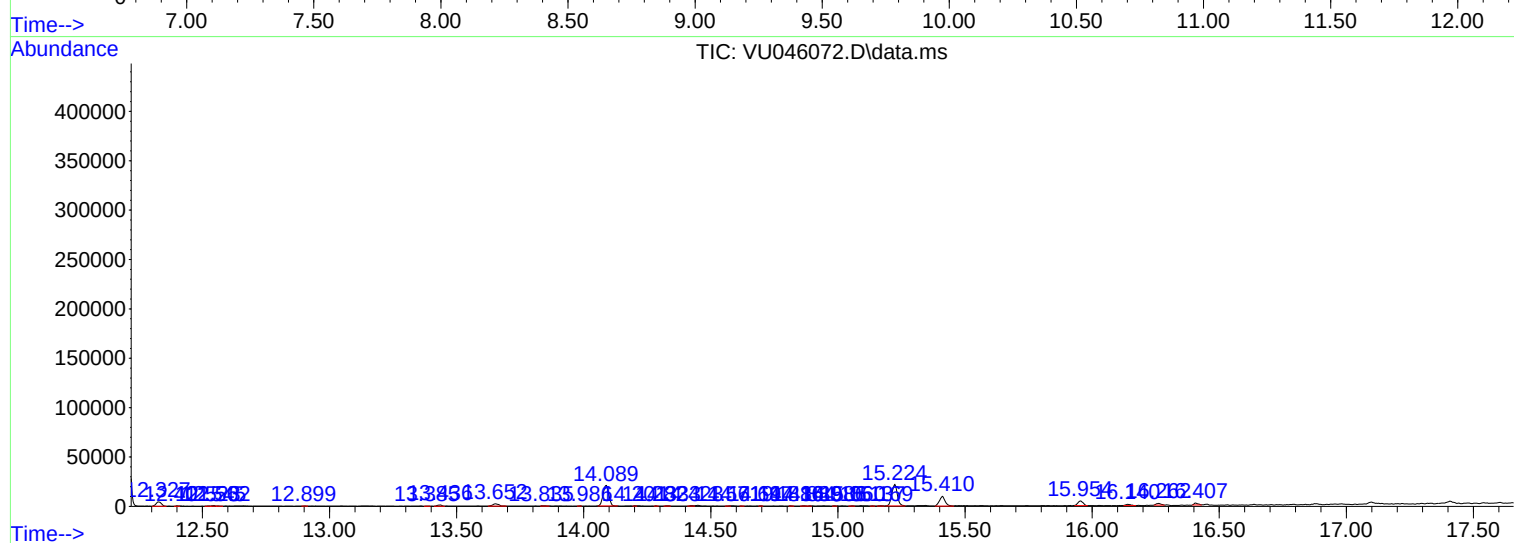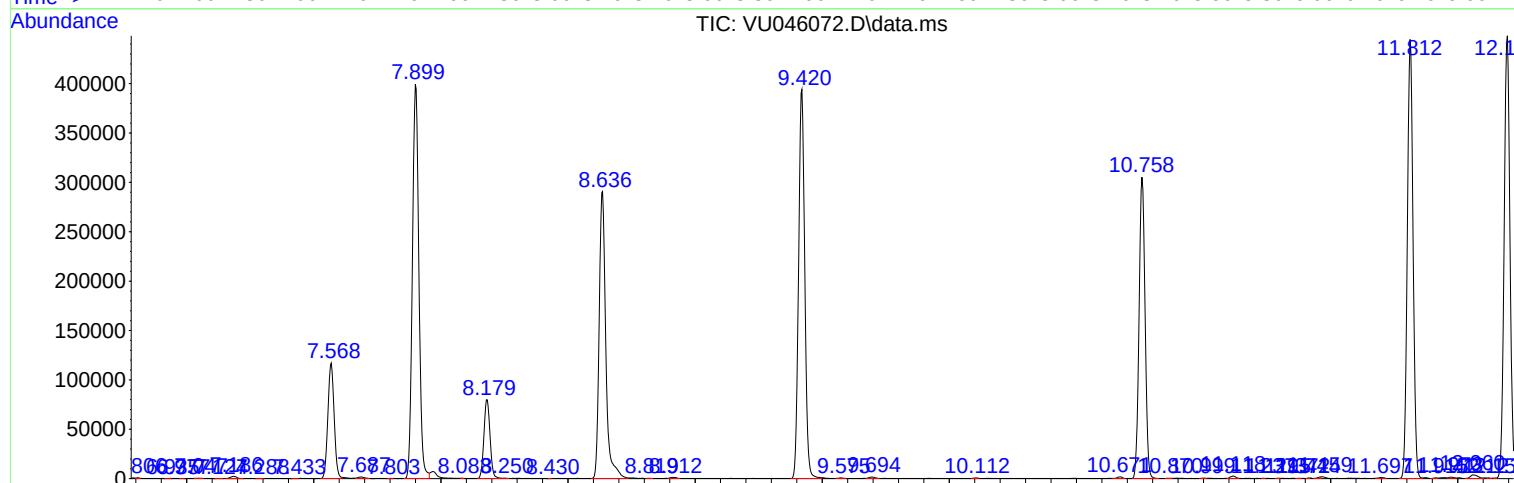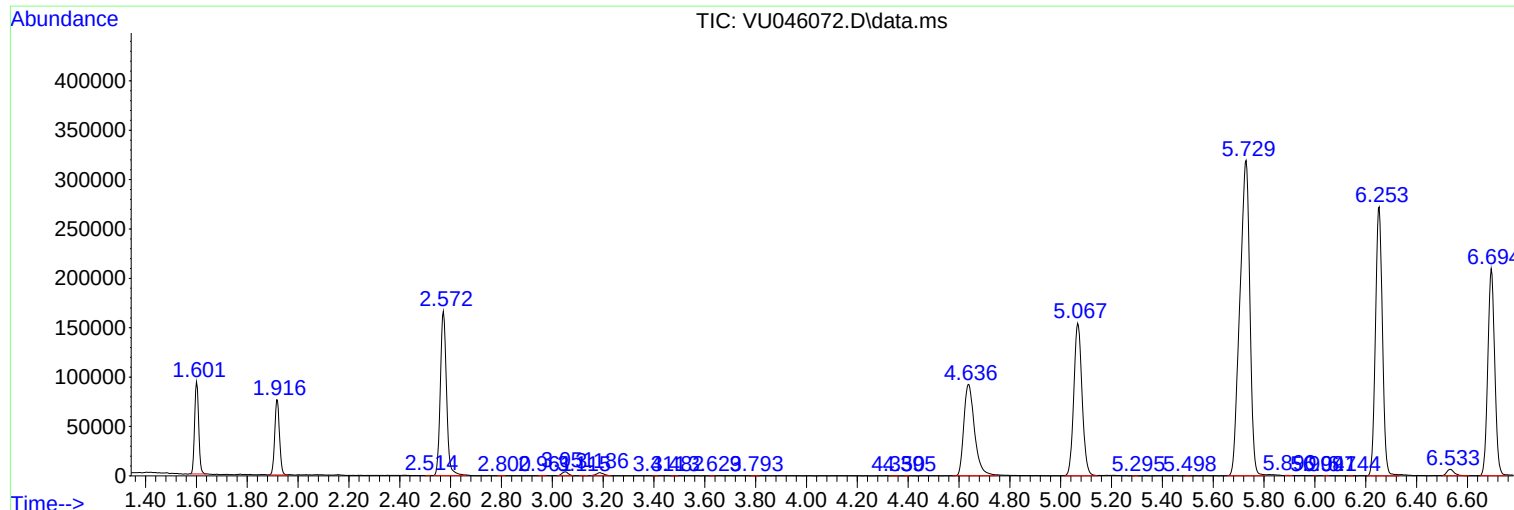

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
Data File : VU046072.D
Acq On : 03 Dec 2021 14:38
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK006

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
Data File : VU046072.D
Acq On : 03 Dec 2021 14:38
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK006

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------