

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
 Data File : VU046074.D
 Acq On : 03 Dec 2021 15:25
 Operator : SY/MD
 Sample : M4869-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESQN3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046074.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.359	3	6	10	rBV2	3966	3313	0.39%	0.048%
2	1.392	10	16	25	rVB2	22614	23999	2.80%	0.345%
3	1.601	72	81	92	rVB	101349	114480	13.35%	1.645%
4	1.916	170	179	192	rBV	76753	97686	11.39%	1.404%
5	2.083	227	231	241	rVB	3099	3596	0.42%	0.052%
6	2.379	317	323	331	rBV3	2753	3859	0.45%	0.055%
7	2.411	331	333	339	rVB	361	225	0.03%	0.003%
8	2.514	363	365	370	rVB	273	148	0.02%	0.002%
9	2.572	370	383	403	rBV	163663	274032	31.95%	3.938%
10	2.800	448	454	461	rVV2	375	581	0.07%	0.008%
11	2.912	486	489	493	rVB	243	140	0.02%	0.002%
12	2.957	500	503	507	rBV2	211	201	0.02%	0.003%
13	3.044	526	530	531	rBV	288	197	0.02%	0.003%
14	3.192	568	576	579	rBV	564	855	0.10%	0.012%
15	3.639	709	715	718	rBV	185	275	0.03%	0.004%
16	3.877	779	789	802	rVB3	1321	2776	0.32%	0.040%
17	4.006	826	829	831	rBV	180	135	0.02%	0.002%
18	4.154	871	875	879	rBV	215	263	0.03%	0.004%
19	4.211	891	893	896	rBV	191	149	0.02%	0.002%
20	4.269	908	911	914	rBV	169	158	0.02%	0.002%
21	4.392	944	949	955	rBV	168	299	0.03%	0.004%
22	4.578	1004	1007	1010	rBV	181	186	0.02%	0.003%
23	4.636	1010	1025	1053	rBV2	84525	248199	28.94%	3.567%
24	4.851	1089	1092	1095	rVB2	204	144	0.02%	0.002%
25	4.896	1103	1106	1108	rBV	283	230	0.03%	0.003%
26	5.067	1140	1159	1178	rBV	156631	344488	40.17%	4.951%
27	5.289	1222	1228	1230	rBV	464	423	0.05%	0.006%
28	5.301	1230	1232	1236	rVV2	521	320	0.04%	0.005%
29	5.353	1243	1248	1253	rBV	204	287	0.03%	0.004%
30	5.543	1302	1307	1311	rBV	181	217	0.03%	0.003%
31	5.581	1316	1319	1325	rVB	155	215	0.03%	0.003%
32	5.623	1326	1332	1334	rBV2	275	271	0.03%	0.004%
33	5.729	1342	1365	1385	rBV2	317104	857593	100.00%	12.324%
34	5.819	1390	1393	1397	rBV4	586	506	0.06%	0.007%
35	5.867	1406	1408	1412	rVB	532	377	0.04%	0.005%
36	6.012	1449	1453	1455	rBV2	283	239	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
 Data File : VU046074.D
 Acq On : 03 Dec 2021 15:25
 Operator : SY/MD
 Sample : M4869-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESQN3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	6.063	1467	1469	1473	rVB	192	151	0.02%	0.002%
38	6.092	1473	1478	1479	rBV	186	191	0.02%	0.003%
39	6.250	1512	1527	1545	rBV	283002	534742	62.35%	7.685%
40	6.530	1605	1614	1629	rBV5	2575	5345	0.62%	0.077%
41	6.584	1629	1631	1635	rVB	371	244	0.03%	0.004%
42	6.620	1639	1642	1646	rVB	161	157	0.02%	0.002%
43	6.645	1646	1650	1651	rBV	207	158	0.02%	0.002%
44	6.694	1651	1665	1684	rBV	199486	385936	45.00%	5.546%
45	6.800	1695	1698	1699	rBV	204	122	0.01%	0.002%
46	6.809	1699	1701	1709	rVB3	767	795	0.09%	0.011%
47	7.044	1766	1774	1779	rVB2	341	624	0.07%	0.009%
48	7.137	1800	1803	1808	rVV	142	167	0.02%	0.002%
49	7.182	1808	1817	1828	rVV3	2256	3673	0.43%	0.053%
50	7.359	1867	1872	1878	rVB	183	304	0.04%	0.004%
51	7.395	1881	1883	1887	rBV	276	204	0.02%	0.003%
52	7.449	1897	1900	1905	rBV	160	208	0.02%	0.003%
53	7.568	1922	1937	1951	rBV	112151	192499	22.45%	2.766%
54	7.684	1966	1973	1981	rVB4	1648	2539	0.30%	0.036%
55	7.784	2001	2004	2009	rVB	195	132	0.02%	0.002%
56	7.899	2025	2040	2057	rBV	393152	678975	79.17%	9.757%
57	8.083	2093	2097	2100	rVB2	176	164	0.02%	0.002%
58	8.179	2113	2127	2142	rBV	74926	125077	14.58%	1.797%
59	8.295	2160	2163	2167	rVB3	244	187	0.02%	0.003%
60	8.469	2212	2217	2219	rBV2	349	325	0.04%	0.005%
61	8.581	2245	2252	2255	rBV	192	309	0.04%	0.004%
62	8.636	2255	2269	2302	rVV	286095	515178	60.07%	7.404%
63	9.269	2460	2466	2469	rBV	196	269	0.03%	0.004%
64	9.417	2500	2512	2540	rBV	399022	670218	78.15%	9.632%
65	9.571	2556	2560	2564	rVV	235	231	0.03%	0.003%
66	9.694	2590	2598	2605	rBV3	825	1259	0.15%	0.018%
67	9.751	2614	2616	2622	rVB	281	213	0.02%	0.003%
68	10.099	2722	2724	2728	rVB	273	160	0.02%	0.002%
69	10.671	2894	2902	2913	rVB3	1272	1800	0.21%	0.026%
70	10.758	2915	2929	2948	rVB	311127	487422	56.84%	7.005%
71	10.864	2957	2962	2965	rBV2	277	295	0.03%	0.004%
72	10.890	2967	2970	2976	rVB	405	386	0.05%	0.006%
73	11.407	3128	3131	3135	rVB2	225	167	0.02%	0.002%
74	11.462	3138	3148	3159	rBV6	1091	2141	0.25%	0.031%
75	11.697	3214	3221	3222	rBV2	470	439	0.05%	0.006%
76	11.812	3245	3257	3273	rBV	428040	681176	79.43%	9.789%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
 Data File : VU046074.D
 Acq On : 03 Dec 2021 15:25
 Operator : SY/MD
 Sample : M4869-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESQN3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.944	3292	3298	3302	rVV	581	592	0.07%	0.009%
78	11.973	3302	3307	3315	rVB5	799	1093	0.13%	0.016%
79	12.057	3330	3333	3334	rBV	447	267	0.03%	0.004%
80	12.102	3345	3347	3351	rVB	242	123	0.01%	0.002%
81	12.195	3362	3376	3391	rBV	411657	669140	78.03%	9.616%
82	12.330	3411	3418	3423	rBV2	917	1088	0.13%	0.016%
83	12.610	3502	3505	3508	rBV	211	140	0.02%	0.002%
84	12.632	3508	3512	3516	rVV2	191	183	0.02%	0.003%
85	13.140	3666	3670	3673	rBV3	254	200	0.02%	0.003%
86	13.433	3757	3761	3762	rVV	245	130	0.02%	0.002%
87	13.610	3813	3816	3820	rVB	242	144	0.02%	0.002%
88	13.841	3885	3888	3892	rVB2	411	334	0.04%	0.005%
89	14.089	3956	3965	3978	rVB	2934	4228	0.49%	0.061%
90	14.526	4098	4101	4103	rBV	182	124	0.01%	0.002%
91	14.581	4111	4118	4120	rBV2	397	520	0.06%	0.007%
92	14.867	4204	4207	4209	rBV2	326	206	0.02%	0.003%
93	15.018	4250	4254	4258	rVB2	303	262	0.03%	0.004%
94	15.057	4264	4266	4268	rBV	251	124	0.01%	0.002%
95	15.172	4297	4302	4305	rBV	300	268	0.03%	0.004%
96	15.227	4311	4319	4326	rBV2	1753	2819	0.33%	0.041%
97	15.401	4370	4373	4374	rBV	539	238	0.03%	0.003%
98	15.475	4393	4396	4398	rBV	248	129	0.02%	0.002%
99	16.272	4642	4644	4647	rBV	398	169	0.02%	0.002%
100	16.713	4778	4781	4783	rBV2	635	390	0.05%	0.006%




Sum of corrected areas: 6958555

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
Data File : VU046074.D
Acq On : 03 Dec 2021 15:25
Operator : SY/MD
Sample : M4869-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESQN3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

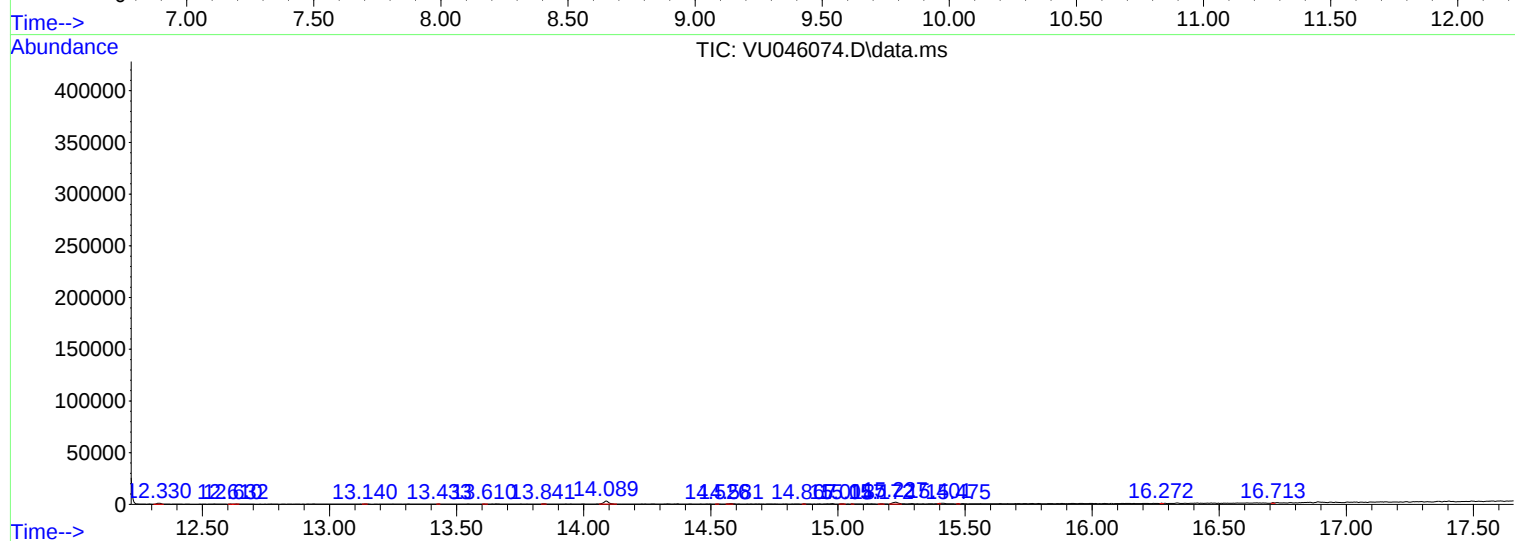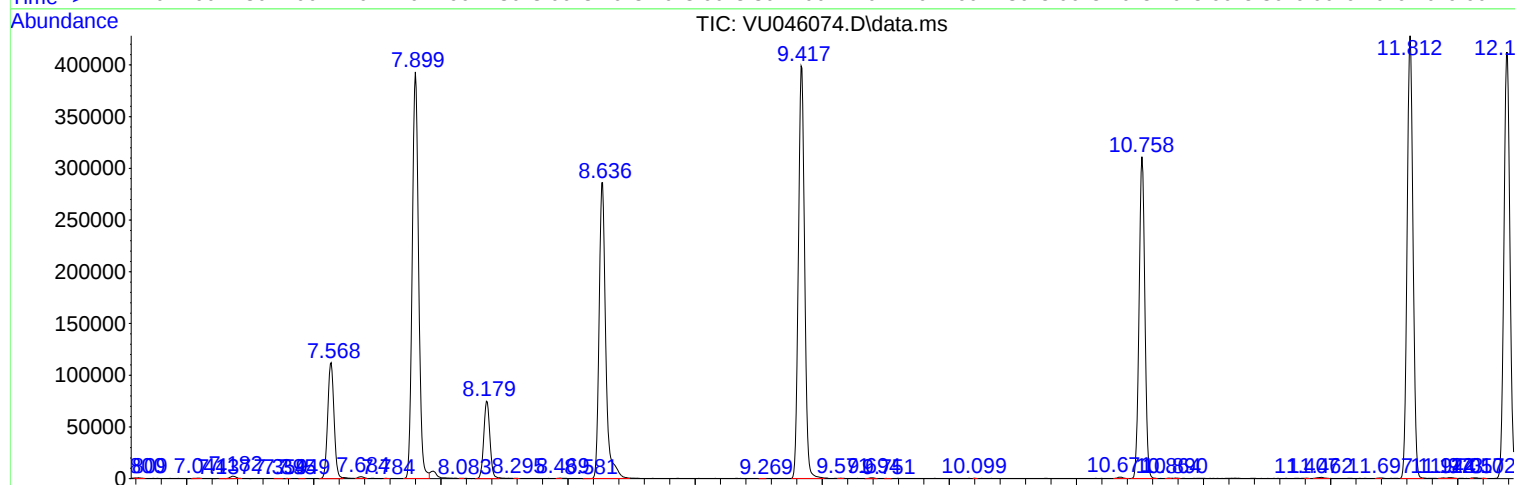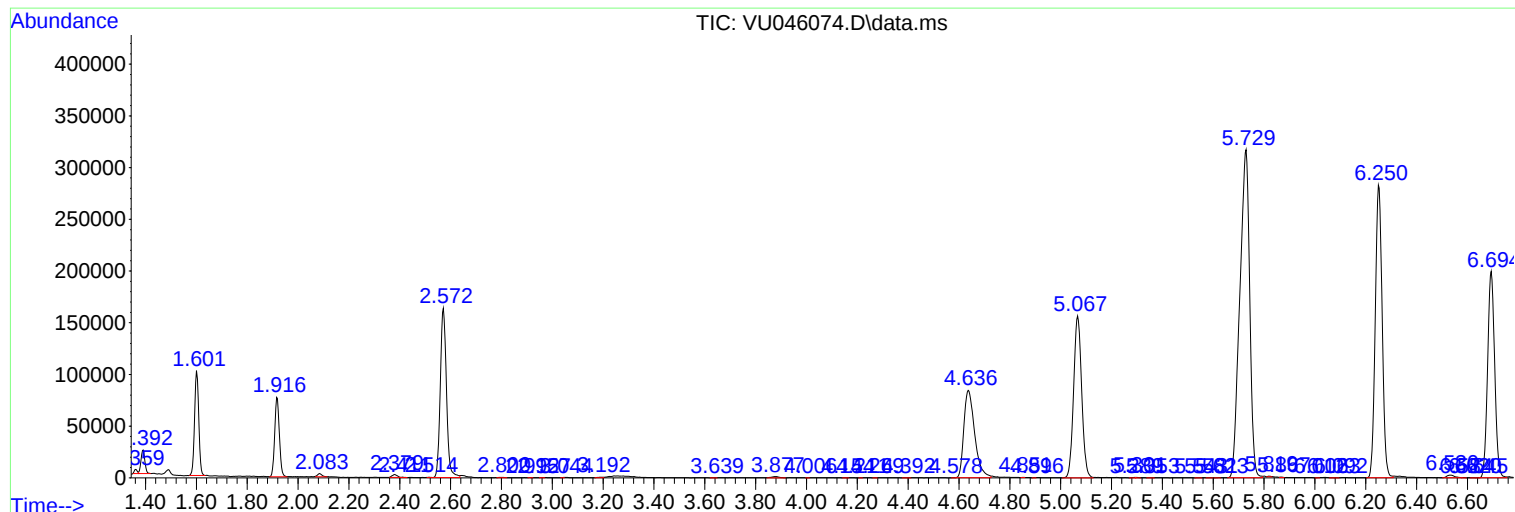

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
Data File : VU046074.D
Acq On : 03 Dec 2021 15:25
Operator : SY/MD
Sample : M4869-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESQN3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
Data File : VU046074.D
Acq On : 03 Dec 2021 15:25
Operator : SY/MD
Sample : M4869-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESQN3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc