

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
 Data File : VU046078.D
 Acq On : 03 Dec 2021 16:55
 Operator : SY/MD
 Sample : M4870-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046078.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	93	rVB	102721	111093	14.51%	1.780%
2	1.919	171	180	194	rVB	72138	92845	12.13%	1.488%
3	2.360	314	317	320	rVB2	359	233	0.03%	0.004%
4	2.405	326	331	334	rBV	292	352	0.05%	0.006%
5	2.572	370	383	404	rBV	168330	276153	36.07%	4.426%
6	2.700	420	423	428	rVB	155	156	0.02%	0.003%
7	2.768	441	444	445	rVV2	188	129	0.02%	0.002%
8	2.797	446	453	466	rVB	1823	3085	0.40%	0.049%
9	2.958	501	503	507	rBV	158	146	0.02%	0.002%
10	3.051	524	532	544	rVB2	2782	4430	0.58%	0.071%
11	3.183	564	573	575	rBV2	1980	2472	0.32%	0.040%
12	3.356	621	627	629	rBV3	663	693	0.09%	0.011%
13	3.453	654	657	660	rBV	196	184	0.02%	0.003%
14	3.675	721	726	727	rBV	155	158	0.02%	0.003%
15	3.768	750	755	757	rBV	149	180	0.02%	0.003%
16	3.842	774	778	780	rBV	149	151	0.02%	0.002%
17	3.954	809	813	816	rBB	153	151	0.02%	0.002%
18	3.974	816	819	822	rBB	150	124	0.02%	0.002%
19	4.003	825	828	831	rBV	146	142	0.02%	0.002%
20	4.035	835	838	841	rBV	168	151	0.02%	0.002%
21	4.083	848	853	856	rBV	146	196	0.03%	0.003%
22	4.379	939	945	949	rBV	185	284	0.04%	0.005%
23	4.414	954	956	959	rBV	149	125	0.02%	0.002%
24	4.575	1004	1006	1009	rBV	130	120	0.02%	0.002%
25	4.636	1009	1025	1056	rBV	65711	189168	24.71%	3.032%
26	5.067	1142	1159	1180	rBV	131147	292657	38.22%	4.690%
27	5.189	1189	1197	1202	rBV3	352	642	0.08%	0.010%
28	5.289	1223	1228	1230	rBV	441	306	0.04%	0.005%
29	5.395	1259	1261	1264	rBV	281	156	0.02%	0.003%
30	5.729	1341	1365	1387	rBV2	281383	765644	100.00%	12.271%
31	5.887	1412	1414	1418	rVB2	334	185	0.02%	0.003%
32	5.906	1418	1420	1424	rVB2	262	161	0.02%	0.003%
33	5.925	1424	1426	1431	rBV	146	144	0.02%	0.002%
34	6.044	1459	1463	1466	rBV2	208	157	0.02%	0.003%
35	6.179	1502	1505	1507	rBV	179	150	0.02%	0.002%
36	6.250	1512	1527	1547	rBV	263572	499966	65.30%	8.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
 Data File : VU046078.D
 Acq On : 03 Dec 2021 16:55
 Operator : SY/MD
 Sample : M4870-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	6.449	1587	1589	1592	rVB2	244	147	0.02%	0.002%
38	6.475	1592	1597	1602	rVB2	331	456	0.06%	0.007%
39	6.539	1605	1617	1627	rBV8	2883	5807	0.76%	0.093%
40	6.642	1644	1649	1651	rBV	300	224	0.03%	0.004%
41	6.694	1651	1665	1684	rBV	173284	335875	43.87%	5.383%
42	6.803	1696	1699	1701	rBV3	310	216	0.03%	0.003%
43	6.993	1754	1758	1762	rBV	136	189	0.02%	0.003%
44	7.041	1771	1773	1775	rBV	209	150	0.02%	0.002%
45	7.182	1814	1817	1821	rBV	147	179	0.02%	0.003%
46	7.568	1924	1937	1956	rVV	99180	174659	22.81%	2.799%
47	7.681	1970	1972	1976	rVB2	151	124	0.02%	0.002%
48	7.710	1976	1981	1985	rVB	194	252	0.03%	0.004%
49	7.736	1985	1989	1993	rBV	164	208	0.03%	0.003%
50	7.793	2001	2007	2015	rBV2	715	924	0.12%	0.015%
51	7.899	2027	2040	2057	rBV	361425	631286	82.45%	10.117%
52	8.179	2116	2127	2144	rVV	68514	114155	14.91%	1.830%
53	8.240	2144	2146	2153	rVB3	684	544	0.07%	0.009%
54	8.366	2182	2185	2188	rBV	149	155	0.02%	0.002%
55	8.552	2240	2243	2246	rBV2	717	564	0.07%	0.009%
56	8.633	2256	2268	2302	rBV	215054	385843	50.39%	6.184%
57	8.809	2319	2323	2325	rVB2	252	156	0.02%	0.003%
58	8.919	2348	2357	2364	rBV4	1775	2730	0.36%	0.044%
59	8.989	2375	2379	2381	rBV2	181	129	0.02%	0.002%
60	9.166	2432	2434	2436	rVB	390	182	0.02%	0.003%
61	9.227	2450	2453	2457	rVB	285	238	0.03%	0.004%
62	9.253	2457	2461	2466	rBV	194	288	0.04%	0.005%
63	9.417	2499	2512	2549	rBV	378514	637930	83.32%	10.224%
64	9.575	2552	2561	2574	rVB	1505	2140	0.28%	0.034%
65	9.642	2577	2582	2585	rBV2	277	281	0.04%	0.005%
66	9.694	2591	2598	2607	rVB	1861	2724	0.36%	0.044%
67	10.105	2717	2726	2738	rVB5	2310	4229	0.55%	0.068%
68	10.288	2780	2783	2786	rBV	197	166	0.02%	0.003%
69	10.488	2838	2845	2854	rBV4	1765	2356	0.31%	0.038%
70	10.674	2893	2903	2910	rVB3	2047	2960	0.39%	0.047%
71	10.758	2916	2929	2946	rBV	241558	389744	50.90%	6.246%
72	10.825	2946	2950	2957	rVB2	797	907	0.12%	0.015%
73	10.864	2957	2962	2963	rBV	286	203	0.03%	0.003%
74	10.922	2978	2980	2985	rVB	186	127	0.02%	0.002%
75	11.092	3024	3033	3040	rBV2	1456	2171	0.28%	0.035%
76	11.121	3040	3042	3049	rVB3	328	247	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
 Data File : VU046078.D
 Acq On : 03 Dec 2021 16:55
 Operator : SY/MD
 Sample : M4870-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.462	3138	3148	3159	rVB3	3208	5310	0.69%	0.085%
78	11.578	3179	3184	3188	rVB2	249	283	0.04%	0.005%
79	11.700	3217	3222	3229	rVB2	845	905	0.12%	0.015%
80	11.745	3229	3236	3245	rBV4	2906	4300	0.56%	0.069%
81	11.813	3245	3257	3281	rVV	413147	654865	85.53%	10.495%
82	11.938	3293	3296	3301	rBV3	604	655	0.09%	0.010%
83	11.973	3303	3307	3315	rVB2	1503	1820	0.24%	0.029%
84	12.195	3361	3376	3391	rBV	358576	578511	75.56%	9.272%
85	12.327	3413	3417	3422	rVB3	630	554	0.07%	0.009%
86	12.375	3428	3432	3434	rBV	146	126	0.02%	0.002%
87	12.388	3434	3436	3439	rVV	226	141	0.02%	0.002%
88	12.996	3622	3625	3628	rBV4	567	528	0.07%	0.008%
89	13.221	3686	3695	3705	rBV3	4561	6374	0.83%	0.102%
90	13.841	3880	3888	3899	rBV2	6566	9224	1.20%	0.148%
91	14.089	3955	3965	3976	rVV2	12009	18635	2.43%	0.299%
92	14.288	4023	4027	4029	rBV	184	156	0.02%	0.003%
93	14.330	4032	4040	4049	rVV2	7855	10705	1.40%	0.172%
94	14.693	4150	4153	4158	rBV	251	265	0.03%	0.004%
95	14.967	4233	4238	4239	rBV	194	170	0.02%	0.003%
96	15.028	4253	4257	4259	rVV	244	168	0.02%	0.003%
97	15.047	4259	4263	4265	rVB2	278	165	0.02%	0.003%
98	15.208	4309	4313	4314	rBV	225	160	0.02%	0.003%
99	15.378	4359	4366	4367	rBV	296	307	0.04%	0.005%
100	16.687	4771	4773	4779	rBV2	406	297	0.04%	0.005%




Sum of corrected areas: 6239578

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
Data File : VU046078.D
Acq On : 03 Dec 2021 16:55
Operator : SY/MD
Sample : M4870-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

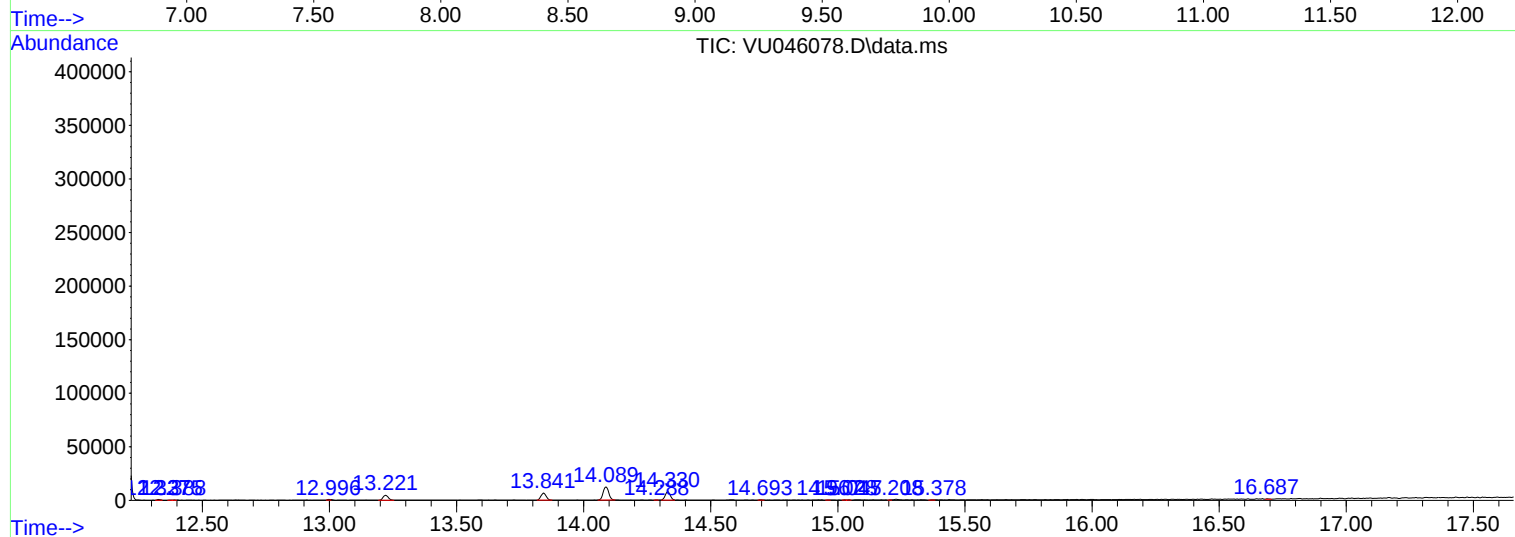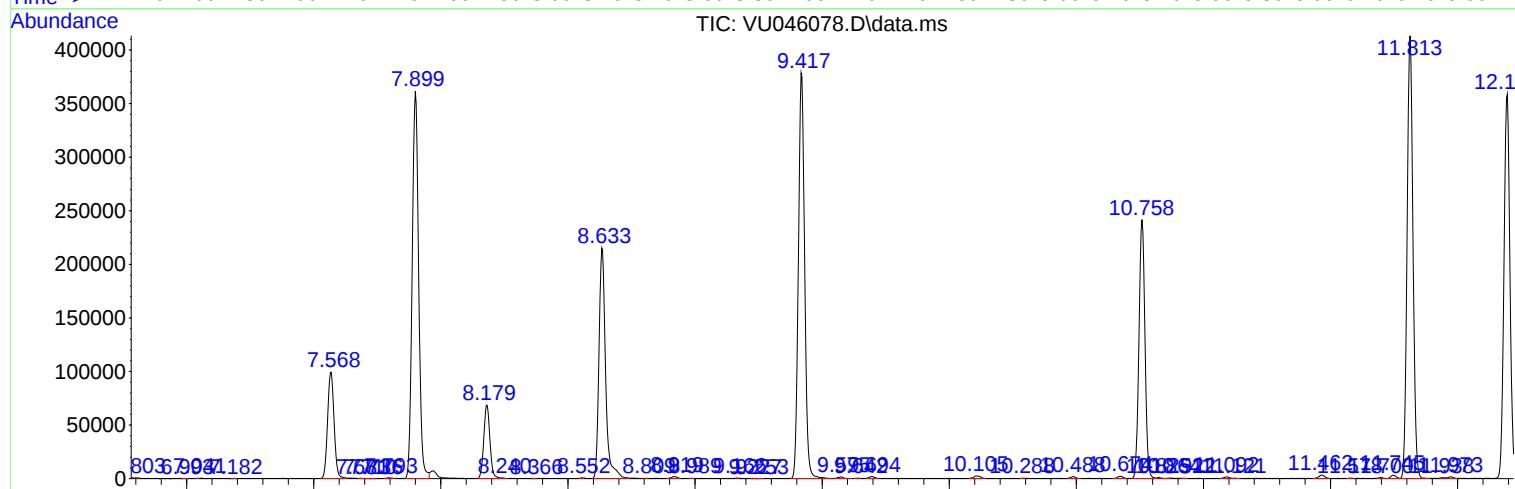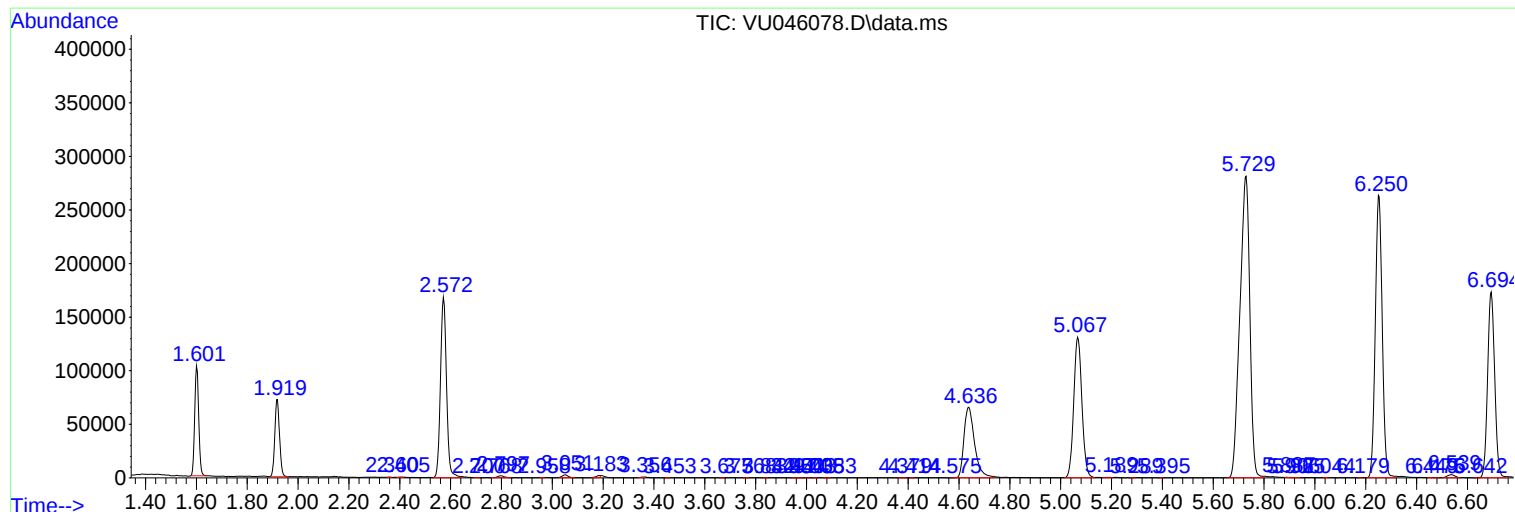

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
Data File : VU046078.D
Acq On : 03 Dec 2021 16:55
Operator : SY/MD
Sample : M4870-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
Data File : VU046078.D
Acq On : 03 Dec 2021 16:55
Operator : SY/MD
Sample : M4870-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------