

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
 Data File : VU046079.D
 Acq On : 03 Dec 2021 17:17
 Operator : SY/MD
 Sample : M4869-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESQN4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046079.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.392	12	16	26	rVB2	3738	3722	0.48%	0.058%
2	1.601	73	81	91	rBV	84603	93735	12.11%	1.460%
3	1.919	171	180	193	rVB	67839	87693	11.33%	1.366%
4	2.202	265	268	271	rVB	239	145	0.02%	0.002%
5	2.382	316	324	331	rBV2	2972	4355	0.56%	0.068%
6	2.572	370	383	401	rBV	148289	246441	31.84%	3.838%
7	2.703	422	424	429	rVB2	286	159	0.02%	0.002%
8	2.803	446	455	462	rBV2	1046	1577	0.20%	0.025%
9	2.951	497	501	503	rBV2	161	142	0.02%	0.002%
10	3.044	525	530	531	rBV	413	352	0.05%	0.005%
11	3.195	571	577	581	rBV2	667	862	0.11%	0.013%
12	3.453	655	657	661	rVB	192	154	0.02%	0.002%
13	3.636	711	714	717	rBV	139	143	0.02%	0.002%
14	3.806	764	767	770	rBV	162	150	0.02%	0.002%
15	3.854	779	782	785	rBV	150	151	0.02%	0.002%
16	4.028	833	836	837	rBV	186	135	0.02%	0.002%
17	4.301	917	921	923	rBB	235	151	0.02%	0.002%
18	4.330	926	930	935	rBV	173	238	0.03%	0.004%
19	4.382	943	946	952	rBB	172	196	0.03%	0.003%
20	4.526	987	991	993	rBV	145	145	0.02%	0.002%
21	4.636	1009	1025	1052	rBV	85211	228390	29.51%	3.557%
22	4.954	1122	1124	1126	rVB	266	131	0.02%	0.002%
23	4.970	1126	1129	1131	rBV	189	157	0.02%	0.002%
24	4.986	1132	1134	1140	rVB2	173	131	0.02%	0.002%
25	5.067	1143	1159	1182	rBV	139624	312502	40.37%	4.867%
26	5.163	1186	1189	1191	rBV4	244	146	0.02%	0.002%
27	5.247	1213	1215	1221	rVB2	270	251	0.03%	0.004%
28	5.430	1266	1272	1276	rBB	173	242	0.03%	0.004%
29	5.510	1291	1297	1299	rBV	156	210	0.03%	0.003%
30	5.629	1329	1334	1338	rBV	172	207	0.03%	0.003%
31	5.729	1342	1365	1384	rBV2	283299	774011	100.00%	12.054%
32	6.009	1447	1452	1453	rBV	243	203	0.03%	0.003%
33	6.018	1453	1455	1457	rVV2	324	226	0.03%	0.004%
34	6.038	1459	1461	1467	rVV3	409	493	0.06%	0.008%
35	6.086	1474	1476	1480	rVV	289	217	0.03%	0.003%
36	6.115	1483	1485	1489	rVB	311	263	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
 Data File : VU046079.D
 Acq On : 03 Dec 2021 17:17
 Operator : SY/MD
 Sample : M4869-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESQN4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	6.250	1511	1527	1545	rBV	274770	513944	66.40%	8.004%
38	6.530	1605	1614	1628	rVB3	4659	9048	1.17%	0.141%
39	6.623	1639	1643	1646	rBB	195	179	0.02%	0.003%
40	6.694	1651	1665	1683	rBV	184333	355189	45.89%	5.531%
41	7.041	1768	1773	1775	rBV2	303	344	0.04%	0.005%
42	7.186	1808	1818	1826	rBV3	2117	3614	0.47%	0.056%
43	7.218	1826	1828	1837	rVB	208	317	0.04%	0.005%
44	7.359	1870	1872	1877	rVB	274	192	0.02%	0.003%
45	7.391	1878	1882	1885	rBB	187	172	0.02%	0.003%
46	7.420	1886	1891	1892	rBV	163	173	0.02%	0.003%
47	7.501	1912	1916	1919	rBB	177	175	0.02%	0.003%
48	7.568	1923	1937	1953	rBV	101739	175567	22.68%	2.734%
49	7.681	1965	1972	1985	rVB4	1649	2994	0.39%	0.047%
50	7.742	1985	1991	1993	rBV2	283	296	0.04%	0.005%
51	7.793	2002	2007	2009	rBV2	249	254	0.03%	0.004%
52	7.806	2009	2011	2014	rVB	288	155	0.02%	0.002%
53	7.845	2020	2023	2025	rBV	200	157	0.02%	0.002%
54	7.899	2025	2040	2056	rBV	351719	607360	78.47%	9.459%
55	8.063	2089	2091	2095	rVB2	412	315	0.04%	0.005%
56	8.179	2116	2127	2144	rBV	68165	112889	14.58%	1.758%
57	8.295	2160	2163	2166	rVB	222	133	0.02%	0.002%
58	8.632	2255	2268	2299	rBV	270496	477930	61.75%	7.443%
59	8.880	2337	2345	2347	rBV	116	163	0.02%	0.003%
60	9.166	2429	2434	2435	rBV	216	201	0.03%	0.003%
61	9.417	2499	2512	2547	rVB	387332	647847	83.70%	10.089%
62	9.571	2552	2560	2565	rBV	718	888	0.11%	0.014%
63	9.697	2591	2599	2607	rVB	1216	1609	0.21%	0.025%
64	10.111	2719	2728	2739	rVB4	821	1358	0.18%	0.021%
65	10.488	2839	2845	2850	rVB2	455	553	0.07%	0.009%
66	10.668	2896	2901	2910	rVB5	1212	1517	0.20%	0.024%
67	10.758	2916	2929	2946	rVV	281528	450677	58.23%	7.018%
68	10.819	2946	2948	2953	rVB2	230	211	0.03%	0.003%
69	10.867	2960	2963	2966	rBV	292	152	0.02%	0.002%
70	10.890	2967	2970	2973	rVV3	320	264	0.03%	0.004%
71	11.086	3026	3031	3034	rBV3	600	681	0.09%	0.011%
72	11.465	3140	3149	3158	rVB4	1433	2339	0.30%	0.036%
73	11.697	3216	3221	3227	rBV3	519	481	0.06%	0.007%
74	11.748	3231	3237	3245	rVB3	1099	1464	0.19%	0.023%
75	11.812	3245	3257	3275	rBV	422235	657759	84.98%	10.243%
76	11.902	3281	3285	3290	rVB2	331	237	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
 Data File : VU046079.D
 Acq On : 03 Dec 2021 17:17
 Operator : SY/MD
 Sample : M4869-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESQN4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.944	3292	3298	3301	rBV	500	500	0.06%	0.008%
78	11.976	3301	3308	3316	rVV4	855	1188	0.15%	0.019%
79	12.063	3332	3335	3338	rBB2	234	167	0.02%	0.003%
80	12.082	3338	3341	3344	rBV	235	175	0.02%	0.003%
81	12.195	3362	3376	3391	rBV	376256	613920	79.32%	9.561%
82	12.587	3496	3498	3505	rVB	307	234	0.03%	0.004%
83	12.639	3510	3514	3517	rBV2	185	150	0.02%	0.002%
84	12.761	3549	3552	3556	rVB2	216	150	0.02%	0.002%
85	13.063	3642	3646	3649	rBV	227	134	0.02%	0.002%
86	13.108	3656	3660	3666	rBV	173	228	0.03%	0.004%
87	13.224	3689	3696	3704	rVB3	2066	2359	0.30%	0.037%
88	13.574	3802	3805	3809	rVB2	213	161	0.02%	0.003%
89	13.841	3881	3888	3896	rVV2	2592	3369	0.44%	0.052%
90	13.944	3917	3920	3925	rBV	217	135	0.02%	0.002%
91	14.089	3956	3965	3976	rBV2	4145	5779	0.75%	0.090%
92	14.150	3981	3984	3986	rBV	246	139	0.02%	0.002%
93	14.330	4034	4040	4048	rVB3	2042	2514	0.32%	0.039%
94	14.465	4079	4082	4086	rVB2	189	132	0.02%	0.002%
95	14.581	4116	4118	4122	rVB	396	243	0.03%	0.004%
96	14.918	4221	4223	4229	rBV2	231	167	0.02%	0.003%
97	14.957	4233	4235	4241	rVB2	257	212	0.03%	0.003%
98	15.012	4248	4252	4255	rBV	274	259	0.03%	0.004%
99	15.227	4314	4319	4323	rBV3	431	458	0.06%	0.007%
100	15.619	4438	4441	4446	rBV2	288	293	0.04%	0.005%




Sum of corrected areas: 6421290

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
Data File : VU046079.D
Acq On : 03 Dec 2021 17:17
Operator : SY/MD
Sample : M4869-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESQN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

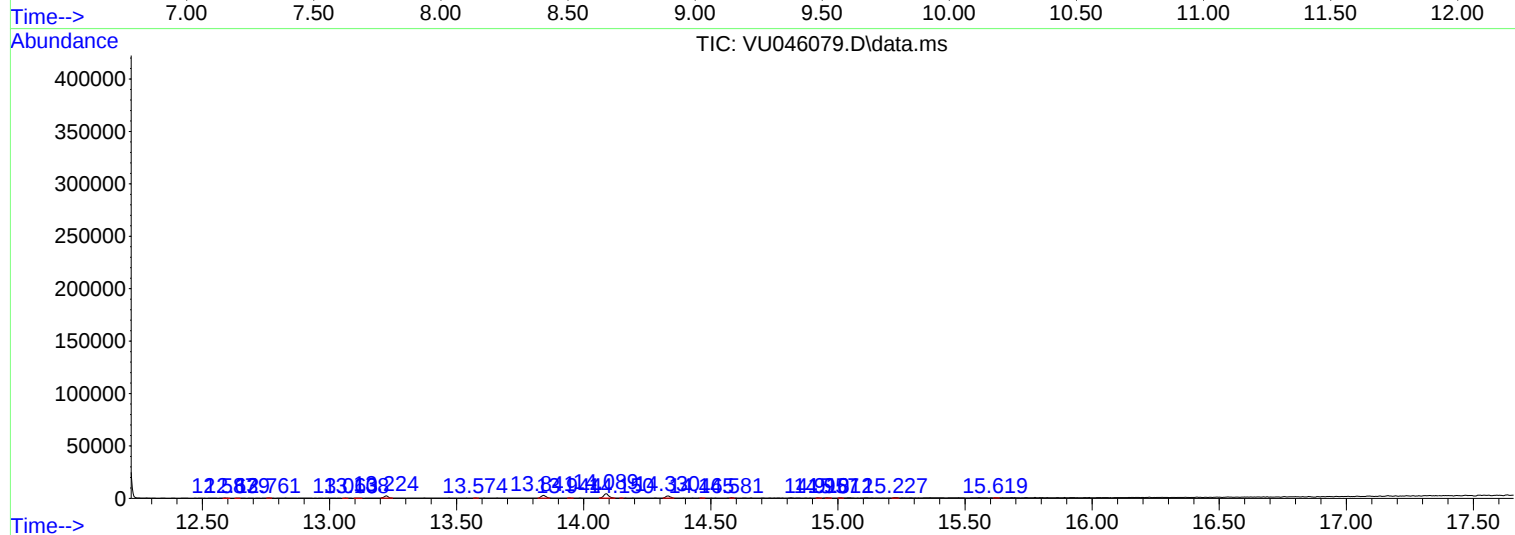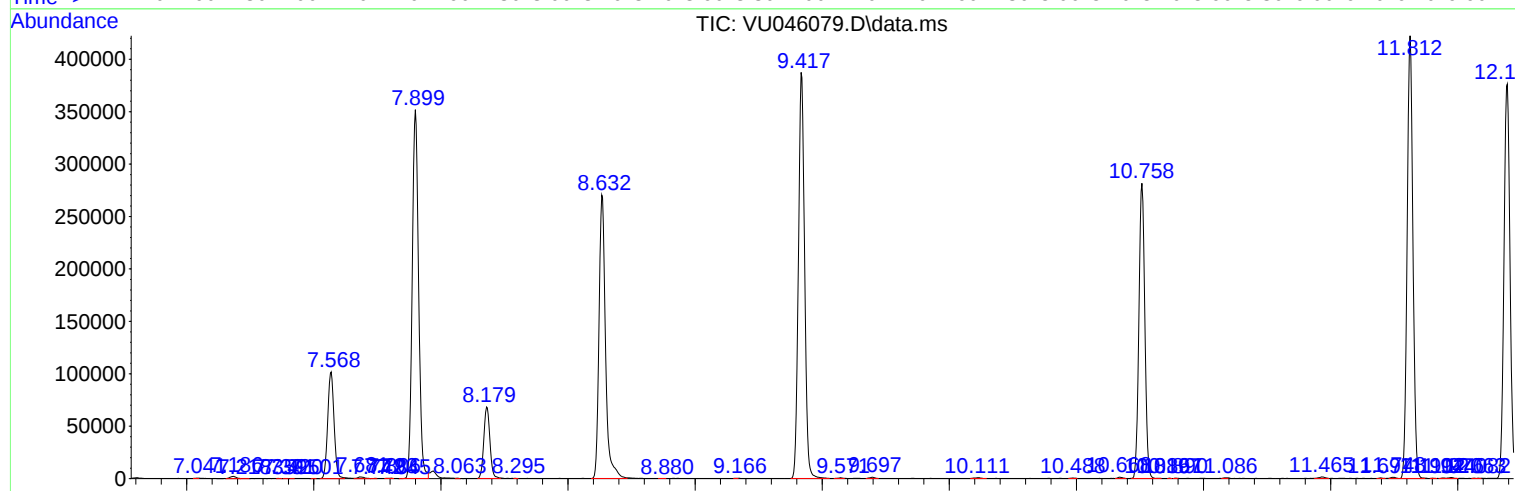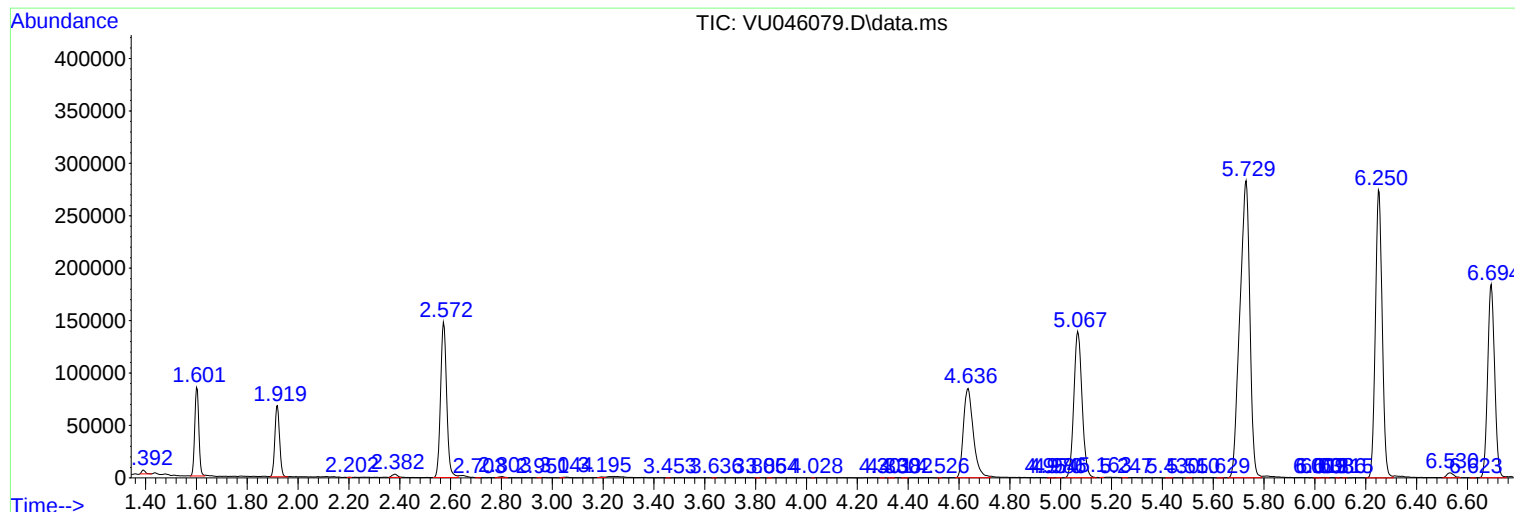

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
Data File : VU046079.D
Acq On : 03 Dec 2021 17:17
Operator : SY/MD
Sample : M4869-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESQN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
Data File : VU046079.D
Acq On : 03 Dec 2021 17:17
Operator : SY/MD
Sample : M4869-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESQN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc