

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
 Data File : VU046080.D
 Acq On : 03 Dec 2021 17:39
 Operator : SY/MD
 Sample : M4869-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESQN5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046080.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.362	3	7	9	rBV2	5879	5231	0.65%	0.078%
2	1.391	10	16	26	rVB3	27543	35339	4.36%	0.528%
3	1.491	43	47	54	rVB	8432	8001	0.99%	0.120%
4	1.600	73	81	88	rBV	93984	110984	13.70%	1.660%
5	1.919	174	180	191	rVB	76161	96772	11.95%	1.447%
6	2.510	361	364	369	rVB3	369	309	0.04%	0.005%
7	2.571	370	383	405	rBV	154061	259130	31.99%	3.875%
8	2.706	423	425	428	rBV	209	115	0.01%	0.002%
9	2.726	428	431	436	rVB3	262	214	0.03%	0.003%
10	2.806	445	456	462	rBV3	1161	2298	0.28%	0.034%
11	3.189	566	575	581	rBV4	1271	2613	0.32%	0.039%
12	3.414	641	645	648	rBV	258	185	0.02%	0.003%
13	3.825	770	773	775	rBV	184	153	0.02%	0.002%
14	4.099	855	858	862	rBV	173	185	0.02%	0.003%
15	4.121	862	865	870	rVB	123	136	0.02%	0.002%
16	4.394	947	950	952	rBV	135	121	0.01%	0.002%
17	4.452	965	968	971	rBV	134	146	0.02%	0.002%
18	4.533	990	993	995	rBV	162	134	0.02%	0.002%
19	4.636	1008	1025	1060	rBV	83767	247844	30.60%	3.706%
20	4.800	1074	1076	1079	rVB2	295	156	0.02%	0.002%
21	4.980	1126	1132	1136	rVB	308	394	0.05%	0.006%
22	5.005	1137	1140	1142	rBV	135	123	0.02%	0.002%
23	5.066	1142	1159	1178	rBV	152632	332210	41.01%	4.968%
24	5.176	1187	1193	1195	rBV2	371	455	0.06%	0.007%
25	5.211	1199	1204	1211	rVV2	391	633	0.08%	0.009%
26	5.240	1211	1213	1216	rVB	266	132	0.02%	0.002%
27	5.288	1222	1228	1234	rVB3	421	462	0.06%	0.007%
28	5.340	1242	1244	1247	rBV	134	118	0.01%	0.002%
29	5.481	1284	1288	1291	rBB	154	151	0.02%	0.002%
30	5.526	1297	1302	1309	rBV	173	329	0.04%	0.005%
31	5.729	1342	1365	1384	rBV2	297106	809997	100.00%	12.112%
32	5.922	1423	1425	1430	rVB2	185	128	0.02%	0.002%
33	5.951	1430	1434	1435	rBV2	244	142	0.02%	0.002%
34	5.992	1442	1447	1449	rBV	170	190	0.02%	0.003%
35	6.047	1461	1464	1466	rVV2	263	214	0.03%	0.003%
36	6.121	1483	1487	1491	rVV2	166	177	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
 Data File : VU046080.D
 Acq On : 03 Dec 2021 17:39
 Operator : SY/MD
 Sample : M4869-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESQN5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	6.163	1498	1500	1504	rBV	225	162	0.02%	0.002%
38	6.250	1513	1527	1546	rBV	265890	500923	61.84%	7.490%
39	6.372	1563	1565	1571	rVB2	335	205	0.03%	0.003%
40	6.533	1608	1615	1623	rVB4	1349	2264	0.28%	0.034%
41	6.571	1623	1627	1631	rVB2	152	126	0.02%	0.002%
42	6.610	1635	1639	1642	rBV	160	190	0.02%	0.003%
43	6.693	1650	1665	1684	rBV	194281	373283	46.08%	5.582%
44	6.915	1728	1734	1738	rBB	156	177	0.02%	0.003%
45	6.938	1739	1741	1743	rBV	230	133	0.02%	0.002%
46	7.041	1768	1773	1781	rVV2	283	516	0.06%	0.008%
47	7.182	1808	1817	1827	rVB2	2328	3500	0.43%	0.052%
48	7.230	1830	1832	1836	rVB	170	141	0.02%	0.002%
49	7.256	1836	1840	1842	rBV	170	172	0.02%	0.003%
50	7.301	1852	1854	1856	rBV	224	132	0.02%	0.002%
51	7.568	1924	1937	1952	rBV	104801	181586	22.42%	2.715%
52	7.642	1958	1960	1963	rVB	371	206	0.03%	0.003%
53	7.661	1963	1966	1967	rVV2	318	191	0.02%	0.003%
54	7.687	1967	1974	1983	rVB3	1696	2478	0.31%	0.037%
55	7.796	2004	2008	2009	rBV	193	148	0.02%	0.002%
56	7.899	2026	2040	2057	rBV	368542	640747	79.10%	9.581%
57	8.073	2091	2094	2097	rBV2	249	234	0.03%	0.003%
58	8.102	2100	2103	2106	rVB	178	124	0.02%	0.002%
59	8.179	2115	2127	2147	rBV	70730	118737	14.66%	1.775%
60	8.301	2162	2165	2168	rVB	227	152	0.02%	0.002%
61	8.635	2255	2269	2300	rBV	289725	516816	63.80%	7.728%
62	8.877	2338	2344	2348	rBV	203	318	0.04%	0.005%
63	9.092	2407	2411	2415	rBV	235	295	0.04%	0.004%
64	9.156	2428	2431	2434	rBV3	334	232	0.03%	0.003%
65	9.417	2499	2512	2538	rBV	378913	632589	78.10%	9.459%
66	9.568	2554	2559	2561	rBV	394	360	0.04%	0.005%
67	9.693	2592	2598	2607	rBV4	1106	1628	0.20%	0.024%
68	9.764	2615	2620	2623	rBV2	276	243	0.03%	0.004%
69	10.098	2721	2724	2726	rBV	254	199	0.02%	0.003%
70	10.487	2841	2845	2850	rBV	216	242	0.03%	0.004%
71	10.671	2895	2902	2912	rVB3	1341	1763	0.22%	0.026%
72	10.758	2916	2929	2947	rVB	305538	488030	60.25%	7.297%
73	10.864	2960	2962	2964	rBV	190	129	0.02%	0.002%
74	10.893	2968	2971	2974	rVB3	285	232	0.03%	0.003%
75	11.092	3030	3033	3036	rVB2	496	351	0.04%	0.005%
76	11.346	3110	3112	3116	rVB	232	122	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
 Data File : VU046080.D
 Acq On : 03 Dec 2021 17:39
 Operator : SY/MD
 Sample : M4869-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESQN5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.465	3139	3149	3157	rBV3	1008	1780	0.22%	0.027%
78	11.584	3182	3186	3190	rVB2	203	164	0.02%	0.002%
79	11.700	3217	3222	3225	rVB2	411	382	0.05%	0.006%
80	11.745	3232	3236	3239	rBV	456	474	0.06%	0.007%
81	11.812	3244	3257	3275	rBV	415059	645319	79.67%	9.649%
82	11.889	3279	3281	3283	rVB	249	127	0.02%	0.002%
83	12.063	3330	3335	3339	rBV3	385	471	0.06%	0.007%
84	12.195	3360	3376	3391	rBV	402869	644237	79.54%	9.633%
85	12.349	3420	3424	3428	rBV2	160	144	0.02%	0.002%
86	12.465	3458	3460	3467	rVB	177	128	0.02%	0.002%
87	12.552	3481	3487	3490	rBV2	182	236	0.03%	0.004%
88	12.645	3513	3516	3518	rBV2	195	133	0.02%	0.002%
89	13.220	3690	3695	3702	rVB2	788	866	0.11%	0.013%
90	13.841	3882	3888	3894	rBV2	1228	1472	0.18%	0.022%
91	14.089	3957	3965	3975	rVB	2029	2987	0.37%	0.045%
92	14.333	4036	4041	4048	rVB3	971	1028	0.13%	0.015%
93	14.577	4114	4117	4120	rBV	294	302	0.04%	0.005%
94	14.741	4164	4168	4178	rBV	187	293	0.04%	0.004%
95	14.899	4213	4217	4220	rVB2	230	156	0.02%	0.002%
96	15.272	4329	4333	4336	rBV2	203	210	0.03%	0.003%
97	15.326	4346	4350	4352	rBV	263	240	0.03%	0.004%
98	15.391	4367	4370	4371	rBV	188	132	0.02%	0.002%
99	15.442	4382	4386	4388	rBV2	323	245	0.03%	0.004%
100	16.211	4623	4625	4627	rBV	291	143	0.02%	0.002%




Sum of corrected areas: 6687666

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
Data File : VU046080.D
Acq On : 03 Dec 2021 17:39
Operator : SY/MD
Sample : M4869-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESQN5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

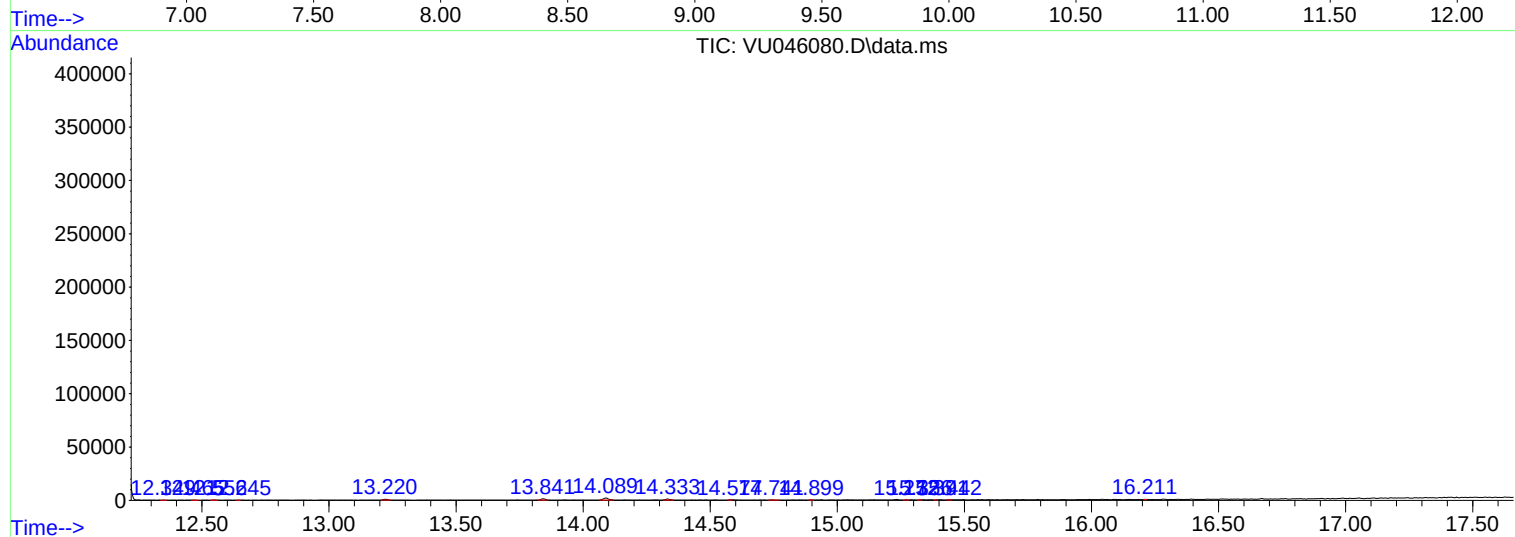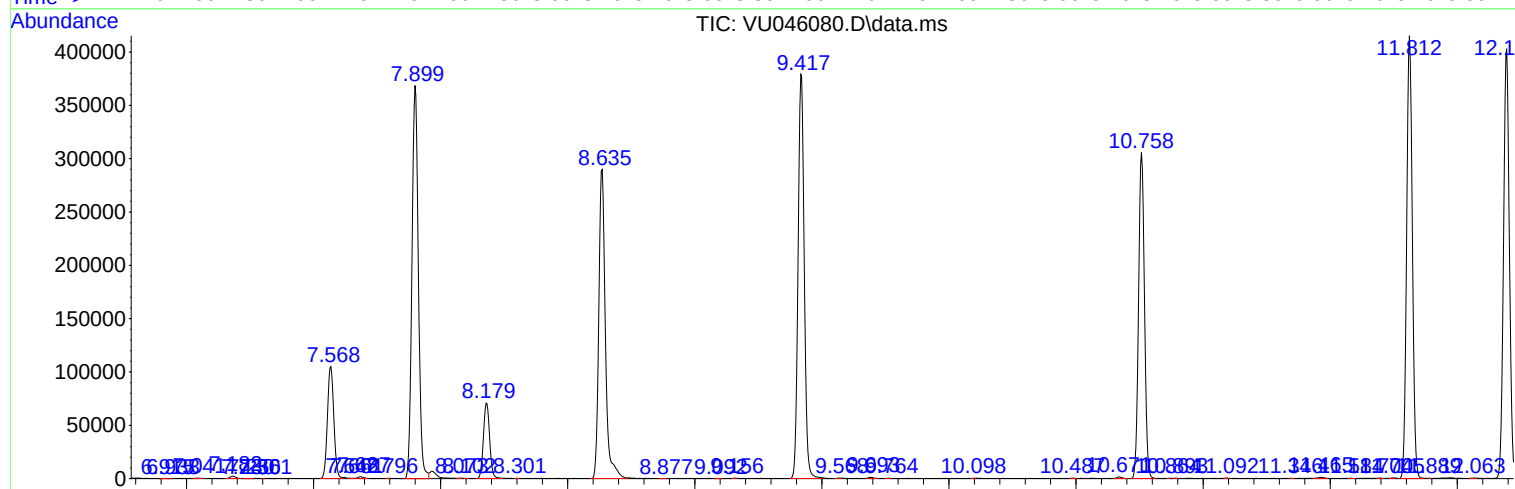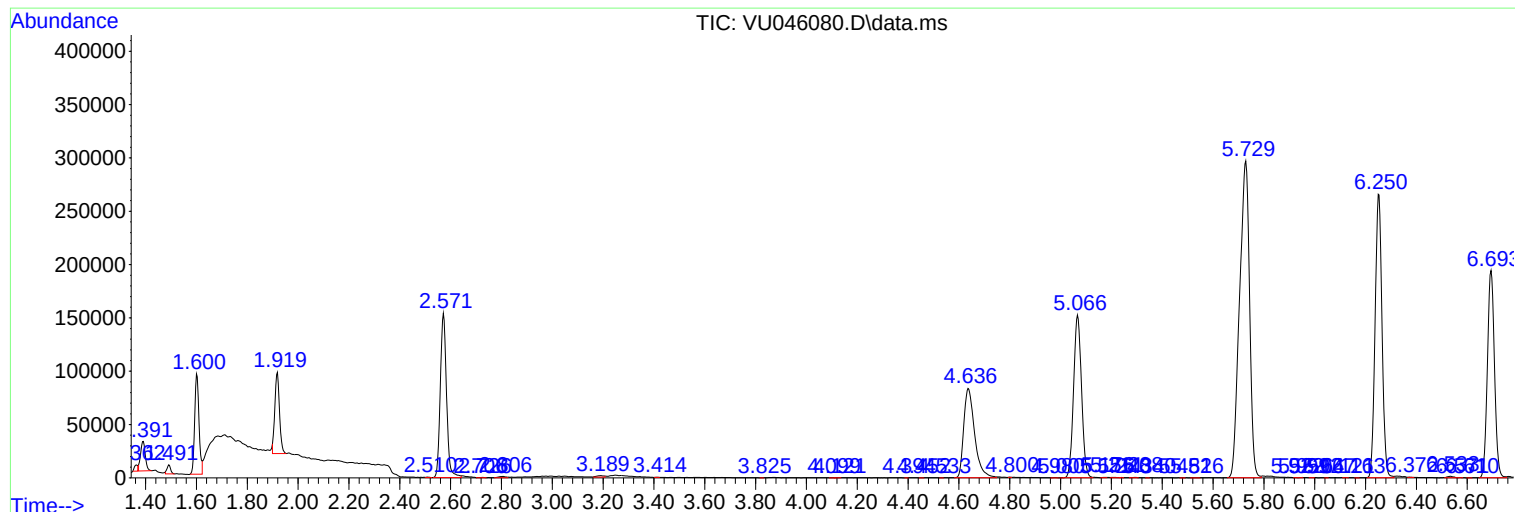

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
Data File : VU046080.D
Acq On : 03 Dec 2021 17:39
Operator : SY/MD
Sample : M4869-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESQN5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
Data File : VU046080.D
Acq On : 03 Dec 2021 17:39
Operator : SY/MD
Sample : M4869-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESQN5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc