

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
 Data File : VU046081.D
 Acq On : 03 Dec 2021 18:02
 Operator : SY/MD
 Sample : M4869-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESQN6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046081.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	96	rVB	84387	92298	11.90%	1.442%
2	1.916	171	179	191	rBV	68121	90852	11.72%	1.420%
3	2.504	360	362	365	rBV2	242	125	0.02%	0.002%
4	2.572	371	383	407	rBV	146655	247130	31.87%	3.861%
5	2.748	434	438	440	rVB	264	149	0.02%	0.002%
6	2.800	447	454	462	rVB2	520	906	0.12%	0.014%
7	2.954	499	502	506	rBV	266	223	0.03%	0.003%
8	3.051	527	532	537	rBV2	468	528	0.07%	0.008%
9	3.189	568	575	583	rBV2	496	837	0.11%	0.013%
10	3.240	587	591	593	rBV2	171	155	0.02%	0.002%
11	3.449	653	656	663	rBV	134	121	0.02%	0.002%
12	3.970	815	818	823	rVB	176	174	0.02%	0.003%
13	4.083	850	853	858	rBV	150	193	0.02%	0.003%
14	4.192	884	887	889	rBV	155	134	0.02%	0.002%
15	4.218	893	895	898	rVV	222	159	0.02%	0.002%
16	4.250	901	905	908	rBB	135	141	0.02%	0.002%
17	4.282	908	915	922	rBV	219	390	0.05%	0.006%
18	4.565	999	1003	1006	rBB	141	145	0.02%	0.002%
19	4.636	1009	1025	1062	rBV2	81324	229153	29.55%	3.580%
20	4.835	1086	1087	1094	rVB2	267	153	0.02%	0.002%
21	4.919	1109	1113	1117	rVB	179	128	0.02%	0.002%
22	5.067	1142	1159	1182	rBV	145815	315698	40.71%	4.933%
23	5.160	1182	1188	1191	rBV3	349	484	0.06%	0.008%
24	5.288	1224	1228	1229	rBV2	180	118	0.02%	0.002%
25	5.398	1259	1262	1265	rVB	153	129	0.02%	0.002%
26	5.729	1342	1365	1383	rBV2	282474	775400	100.00%	12.115%
27	5.909	1416	1421	1422	rBV2	204	172	0.02%	0.003%
28	6.022	1453	1456	1459	rBV	280	185	0.02%	0.003%
29	6.041	1459	1462	1463	rVV	419	225	0.03%	0.004%
30	6.054	1463	1466	1469	rVV2	348	249	0.03%	0.004%
31	6.176	1502	1504	1509	rBV	153	182	0.02%	0.003%
32	6.250	1513	1527	1548	rBV	275317	518834	66.91%	8.107%
33	6.533	1608	1615	1625	rVB4	1809	3124	0.40%	0.049%
34	6.694	1650	1665	1684	rVV	184683	354688	45.74%	5.542%
35	6.764	1684	1687	1694	rVV4	730	830	0.11%	0.013%
36	6.803	1696	1699	1703	rVB	335	234	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
 Data File : VU046081.D
 Acq On : 03 Dec 2021 18:02
 Operator : SY/MD
 Sample : M4869-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESQN6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	6.874	1718	1721	1723	rBV	142	122	0.02%	0.002%
38	6.973	1749	1752	1756	rVB	165	151	0.02%	0.002%
39	7.041	1770	1773	1780	rBV2	282	368	0.05%	0.006%
40	7.179	1810	1816	1827	rVB5	2100	3543	0.46%	0.055%
41	7.247	1832	1837	1841	rBV	193	275	0.04%	0.004%
42	7.369	1869	1875	1877	rBV	172	220	0.03%	0.003%
43	7.414	1884	1889	1891	rBB	158	158	0.02%	0.002%
44	7.439	1894	1897	1901	rBB	173	157	0.02%	0.002%
45	7.465	1901	1905	1907	rBV	289	225	0.03%	0.004%
46	7.520	1919	1922	1924	rBV	168	142	0.02%	0.002%
47	7.568	1924	1937	1956	rVV	99792	172135	22.20%	2.690%
48	7.687	1966	1974	1982	rBV2	1740	2325	0.30%	0.036%
49	7.787	2000	2005	2009	rBB2	258	262	0.03%	0.004%
50	7.819	2012	2015	2018	rBV	164	157	0.02%	0.002%
51	7.899	2025	2040	2056	rBV	349050	605104	78.04%	9.455%
52	8.179	2115	2127	2141	rBV	67340	110066	14.19%	1.720%
53	8.475	2209	2219	2228	rVB3	2154	3226	0.42%	0.050%
54	8.542	2236	2240	2246	rBV	103	132	0.02%	0.002%
55	8.632	2255	2268	2301	rBV	268364	475508	61.32%	7.430%
56	9.073	2399	2405	2407	rBV	175	235	0.03%	0.004%
57	9.156	2428	2431	2436	rVV2	253	250	0.03%	0.004%
58	9.417	2499	2512	2536	rBV	385631	647590	83.52%	10.118%
59	9.571	2554	2560	2565	rVB	295	375	0.05%	0.006%
60	9.632	2575	2579	2581	rVB2	179	131	0.02%	0.002%
61	9.690	2591	2597	2603	rBV2	675	867	0.11%	0.014%
62	10.111	2721	2728	2732	rVV3	287	372	0.05%	0.006%
63	10.565	2865	2869	2878	rBV	175	159	0.02%	0.002%
64	10.668	2896	2901	2910	rBV3	934	1113	0.14%	0.017%
65	10.758	2916	2929	2946	rVB	289015	458201	59.09%	7.159%
66	10.864	2959	2962	2963	rBV	193	121	0.02%	0.002%
67	10.896	2965	2972	2979	rVB4	1795	2660	0.34%	0.042%
68	11.089	3028	3032	3034	rBV	217	177	0.02%	0.003%
69	11.462	3141	3148	3159	rVB2	990	1609	0.21%	0.025%
70	11.697	3218	3221	3225	rVB2	536	369	0.05%	0.006%
71	11.748	3232	3237	3241	rBV	428	390	0.05%	0.006%
72	11.812	3245	3257	3273	rBV	416141	651979	84.08%	10.187%
73	11.938	3294	3296	3299	rBV	221	129	0.02%	0.002%
74	11.980	3303	3309	3313	rVB	569	626	0.08%	0.010%
75	12.063	3332	3335	3338	rBV	193	160	0.02%	0.002%
76	12.195	3362	3376	3390	rBV	381915	613743	79.15%	9.590%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
 Data File : VU046081.D
 Acq On : 03 Dec 2021 18:02
 Operator : SY/MD
 Sample : M4869-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESQN6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	12.774	3549	3556	3562	rVB4	664	899	0.12%	0.014%
78	13.205	3684	3690	3691	rBV	180	171	0.02%	0.003%
79	13.221	3691	3695	3702	rVB	606	637	0.08%	0.010%
80	13.539	3791	3794	3797	rBV	153	122	0.02%	0.002%
81	13.623	3817	3820	3825	rBV	138	141	0.02%	0.002%
82	13.835	3884	3886	3887	rBV	383	170	0.02%	0.003%
83	14.089	3957	3965	3975	rVB3	1435	2305	0.30%	0.036%
84	14.211	3997	4003	4005	rBV	182	220	0.03%	0.003%
85	14.340	4035	4043	4045	rVB3	533	643	0.08%	0.010%
86	14.500	4091	4093	4101	rBV	220	194	0.03%	0.003%
87	14.581	4112	4118	4123	rBV3	542	607	0.08%	0.009%
88	14.725	4160	4163	4166	rVB	253	200	0.03%	0.003%
89	14.857	4201	4204	4209	rVB2	216	164	0.02%	0.003%
90	14.950	4231	4233	4242	rVB	330	192	0.02%	0.003%
91	14.995	4243	4247	4251	rBV	178	160	0.02%	0.002%
92	15.105	4278	4281	4284	rVB	354	230	0.03%	0.004%
93	15.130	4286	4289	4291	rBV2	363	252	0.03%	0.004%
94	15.224	4315	4318	4320	rVB	406	236	0.03%	0.004%
95	15.237	4320	4322	4324	rBV	289	138	0.02%	0.002%
96	15.860	4510	4516	4527	rBV2	361	836	0.11%	0.013%
97	16.108	4590	4593	4596	rVB	434	280	0.04%	0.004%
98	16.220	4626	4628	4634	rBV3	355	299	0.04%	0.005%
99	16.709	4778	4780	4783	rBV2	485	359	0.05%	0.006%
100	16.921	4843	4846	4848	rBV3	644	457	0.06%	0.007%




Sum of corrected areas: 6400090

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
Data File : VU046081.D
Acq On : 03 Dec 2021 18:02
Operator : SY/MD
Sample : M4869-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESQN6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

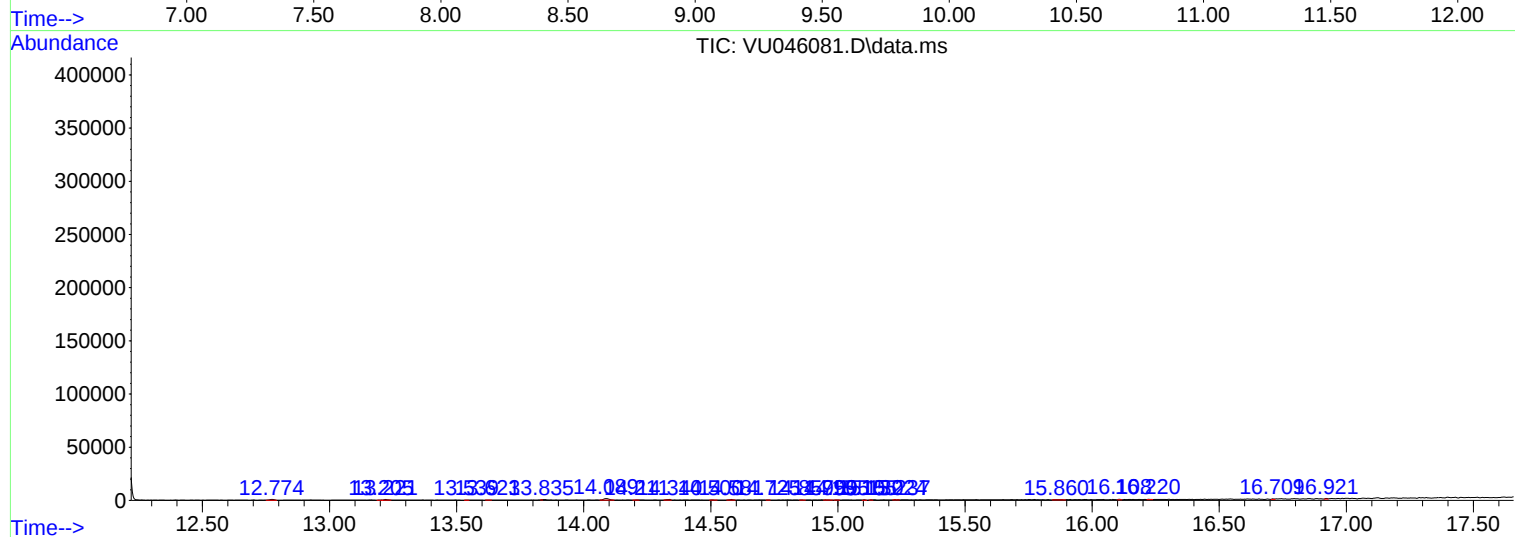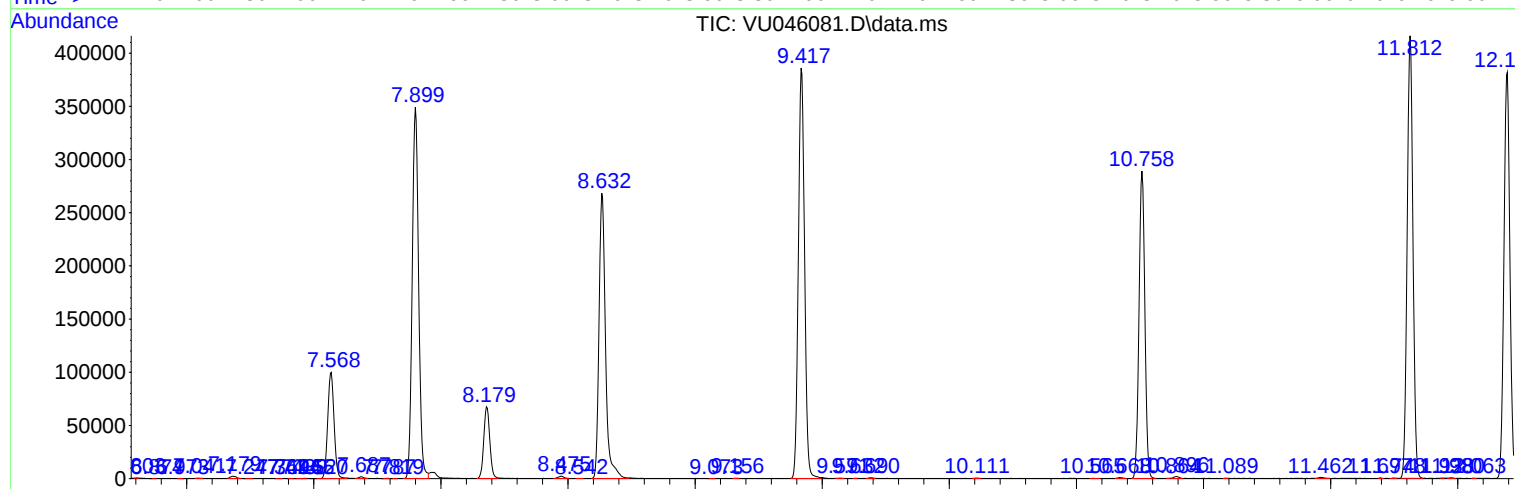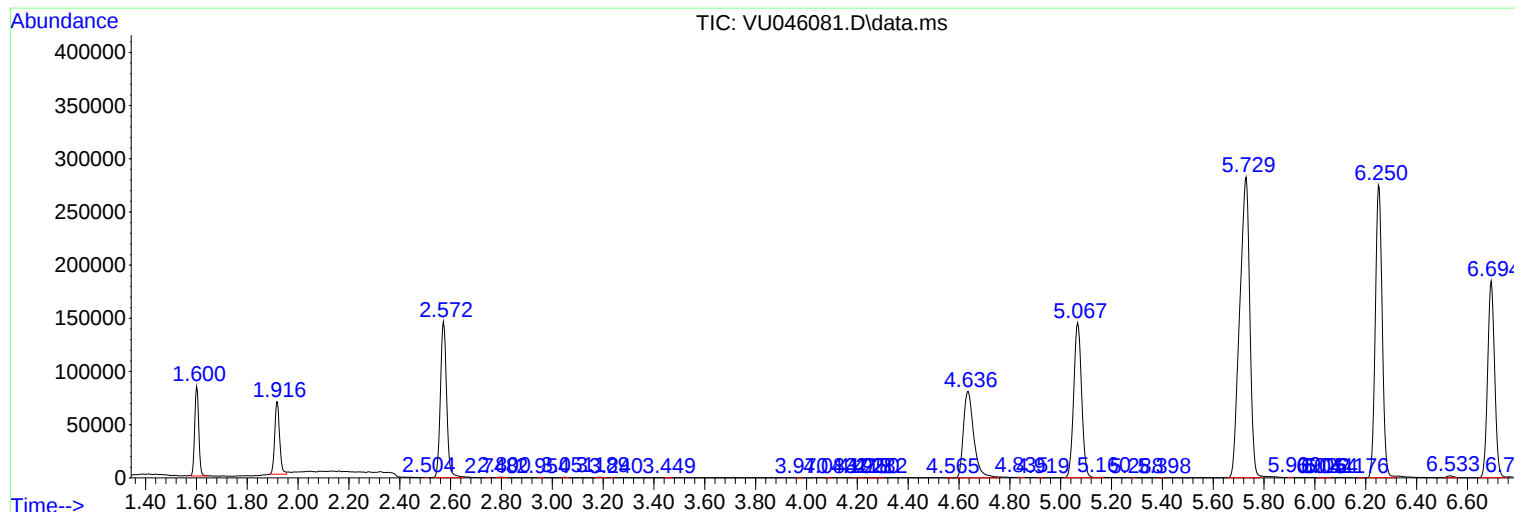

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
Data File : VU046081.D
Acq On : 03 Dec 2021 18:02
Operator : SY/MD
Sample : M4869-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESQN6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
Data File : VU046081.D
Acq On : 03 Dec 2021 18:02
Operator : SY/MD
Sample : M4869-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESQN6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc