

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
 Data File : VU046085.D
 Acq On : 03 Dec 2021 19:31
 Operator : SY/MD
 Sample : M4869-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESQP0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046085.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.514	40	54	75	rBV	64668	304074	40.50%	4.644%
2	1.600	76	81	101	rVB	89102	128524	17.12%	1.963%
3	1.919	173	180	192	rVB	68561	90372	12.04%	1.380%
4	2.501	359	361	368	rVB2	199	154	0.02%	0.002%
5	2.571	370	383	413	rVV	141111	235391	31.35%	3.595%
6	2.784	447	449	451	rVV	338	213	0.03%	0.003%
7	2.803	451	455	459	rVV2	479	513	0.07%	0.008%
8	2.835	463	465	468	rVV	168	110	0.01%	0.002%
9	2.854	468	471	474	rVB2	179	139	0.02%	0.002%
10	2.893	480	483	487	rVB	188	120	0.02%	0.002%
11	2.957	497	503	509	rBV2	244	414	0.06%	0.006%
12	3.054	528	533	541	rVB3	750	1007	0.13%	0.015%
13	3.211	566	582	584	rBV2	1270	2625	0.35%	0.040%
14	3.481	657	666	669	rBV	190	354	0.05%	0.005%
15	3.539	679	684	688	rBV	133	132	0.02%	0.002%
16	3.729	740	743	746	rVB	200	153	0.02%	0.002%
17	3.745	746	748	751	rBV	154	127	0.02%	0.002%
18	3.806	763	767	769	rBV	157	152	0.02%	0.002%
19	3.870	784	787	790	rBB	180	143	0.02%	0.002%
20	3.912	796	800	802	rBV	136	139	0.02%	0.002%
21	4.057	842	845	847	rBV	157	126	0.02%	0.002%
22	4.102	854	859	861	rBV	150	153	0.02%	0.002%
23	4.221	893	896	899	rBB	154	121	0.02%	0.002%
24	4.256	902	907	909	rBV	141	173	0.02%	0.003%
25	4.314	920	925	930	rBV	170	252	0.03%	0.004%
26	4.443	962	965	967	rVV	169	140	0.02%	0.002%
27	4.584	1005	1009	1010	rBV	142	126	0.02%	0.002%
28	4.639	1010	1026	1054	rBV	75586	215812	28.74%	3.296%
29	5.067	1143	1159	1180	rBV	141703	305156	40.64%	4.660%
30	5.195	1196	1199	1201	rBV2	338	231	0.03%	0.004%
31	5.227	1205	1209	1213	rVB2	480	391	0.05%	0.006%
32	5.282	1224	1226	1228	rBV	253	184	0.02%	0.003%
33	5.298	1228	1231	1233	rVB2	248	186	0.02%	0.003%
34	5.494	1288	1292	1295	rBV	154	183	0.02%	0.003%
35	5.510	1295	1297	1301	rVB	169	137	0.02%	0.002%
36	5.600	1321	1325	1329	rBB	158	157	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
 Data File : VU046085.D
 Acq On : 03 Dec 2021 19:31
 Operator : SY/MD
 Sample : M4869-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESQP0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	5.729	1343	1365	1384	rBV3	273678	750858	100.00%	11.467%
38	5.832	1395	1397	1408	rVB2	703	1012	0.13%	0.015%
39	5.970	1437	1440	1443	rBV2	188	177	0.02%	0.003%
40	5.986	1443	1445	1448	rVB2	283	154	0.02%	0.002%
41	6.005	1448	1451	1454	rVB	218	117	0.02%	0.002%
42	6.060	1465	1468	1472	rBV	139	161	0.02%	0.002%
43	6.092	1475	1478	1480	rBV	154	133	0.02%	0.002%
44	6.157	1494	1498	1501	rBB	187	177	0.02%	0.003%
45	6.250	1512	1527	1545	rBV	262983	502230	66.89%	7.670%
46	6.404	1573	1575	1586	rVB2	385	488	0.06%	0.007%
47	6.533	1607	1615	1623	rBV3	1209	1669	0.22%	0.025%
48	6.694	1648	1665	1682	rBV	179316	347031	46.22%	5.300%
49	6.812	1701	1702	1708	rVB	647	396	0.05%	0.006%
50	6.851	1708	1714	1718	rBV2	324	391	0.05%	0.006%
51	6.928	1734	1738	1741	rBV	150	181	0.02%	0.003%
52	7.041	1767	1773	1783	rVB2	400	743	0.10%	0.011%
53	7.179	1809	1816	1827	rBV5	1927	3469	0.46%	0.053%
54	7.250	1834	1838	1842	rBV	193	252	0.03%	0.004%
55	7.337	1862	1865	1867	rBV	138	123	0.02%	0.002%
56	7.449	1896	1900	1903	rBB	138	139	0.02%	0.002%
57	7.568	1924	1937	1951	rVV	94934	163895	21.83%	2.503%
58	7.684	1966	1973	1984	rVB	1209	2018	0.27%	0.031%
59	7.777	1999	2002	2005	rBV	168	171	0.02%	0.003%
60	7.796	2005	2008	2011	rVV	234	183	0.02%	0.003%
61	7.822	2011	2016	2019	rVV2	186	193	0.03%	0.003%
62	7.899	2026	2040	2057	rBV	335632	581796	77.48%	8.885%
63	8.066	2088	2092	2097	rBV	164	182	0.02%	0.003%
64	8.179	2115	2127	2148	rBV	63973	106059	14.13%	1.620%
65	8.472	2209	2218	2231	rBV2	3291	5697	0.76%	0.087%
66	8.636	2256	2269	2303	rVV	258907	465554	62.00%	7.110%
67	9.420	2499	2513	2551	rVB	378628	630084	83.92%	9.623%
68	9.571	2556	2560	2564	rVB	157	172	0.02%	0.003%
69	9.697	2591	2599	2605	rBV3	528	912	0.12%	0.014%
70	10.063	2709	2713	2716	rBV	238	260	0.03%	0.004%
71	10.099	2722	2724	2727	rBV	193	138	0.02%	0.002%
72	10.407	2816	2820	2825	rBV	127	135	0.02%	0.002%
73	10.658	2895	2898	2899	rBV	314	156	0.02%	0.002%
74	10.674	2899	2903	2906	rVB3	676	539	0.07%	0.008%
75	10.758	2917	2929	2947	rBV	285250	452809	60.31%	6.915%
76	10.893	2962	2971	2988	rVB3	2970	4732	0.63%	0.072%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
 Data File : VU046085.D
 Acq On : 03 Dec 2021 19:31
 Operator : SY/MD
 Sample : M4869-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESQP0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.008	3001	3007	3009	rBV	104	122	0.02%	0.002%
78	11.089	3028	3032	3037	rVB2	273	247	0.03%	0.004%
79	11.465	3142	3149	3159	rVB4	734	1211	0.16%	0.018%
80	11.697	3216	3221	3225	rBV	168	193	0.03%	0.003%
81	11.812	3244	3257	3277	rVB	406652	634297	84.48%	9.687%
82	11.928	3290	3293	3294	rBV	281	125	0.02%	0.002%
83	12.195	3363	3376	3390	rBV	366826	592809	78.95%	9.053%
84	12.487	3465	3467	3472	rVB2	213	175	0.02%	0.003%
85	12.770	3548	3555	3563	rVB	1107	1561	0.21%	0.024%
86	12.848	3577	3579	3582	rVB	235	114	0.02%	0.002%
87	13.304	3717	3721	3724	rBV	179	185	0.02%	0.003%
88	13.446	3762	3765	3770	rVB	246	165	0.02%	0.003%
89	13.796	3872	3874	3879	rVB	226	119	0.02%	0.002%
90	13.844	3886	3889	3891	rBV	357	240	0.03%	0.004%
91	14.089	3960	3965	3971	rBV2	454	660	0.09%	0.010%
92	14.574	4111	4116	4123	rVB	393	518	0.07%	0.008%
93	14.658	4139	4142	4144	rBV	225	116	0.02%	0.002%
94	14.745	4166	4169	4171	rBV2	205	118	0.02%	0.002%
95	14.860	4201	4205	4209	rVB2	158	120	0.02%	0.002%
96	14.989	4243	4245	4248	rVV	367	196	0.03%	0.003%
97	15.175	4301	4303	4308	rVB	193	113	0.02%	0.002%
98	15.330	4348	4351	4354	rBV2	235	195	0.03%	0.003%
99	15.362	4358	4361	4365	rBV	238	194	0.03%	0.003%
100	15.912	4530	4532	4536	rVB	289	110	0.01%	0.002%




Sum of corrected areas: 6547873

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
Data File : VU046085.D
Acq On : 03 Dec 2021 19:31
Operator : SY/MD
Sample : M4869-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESQP0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

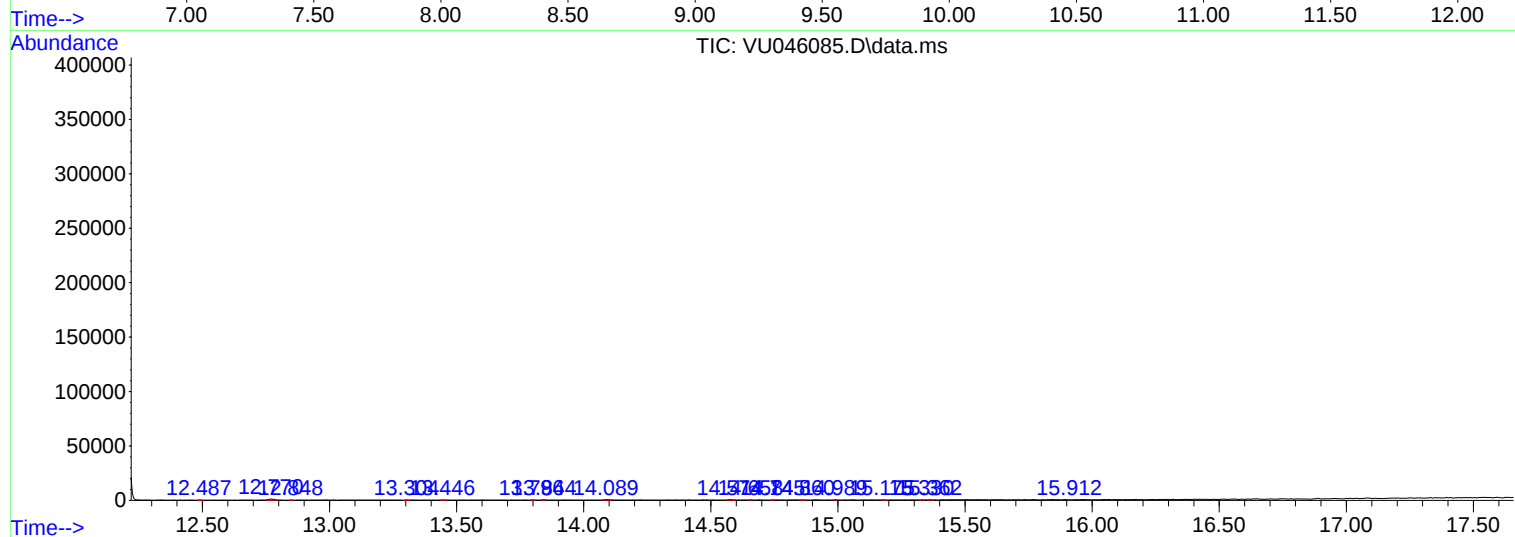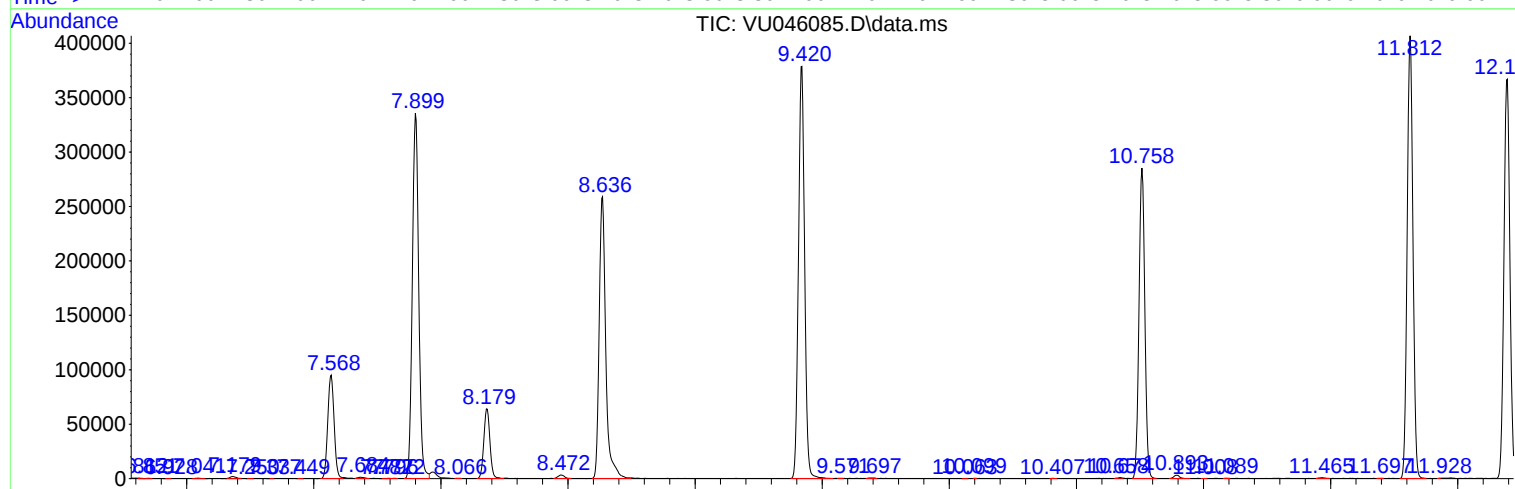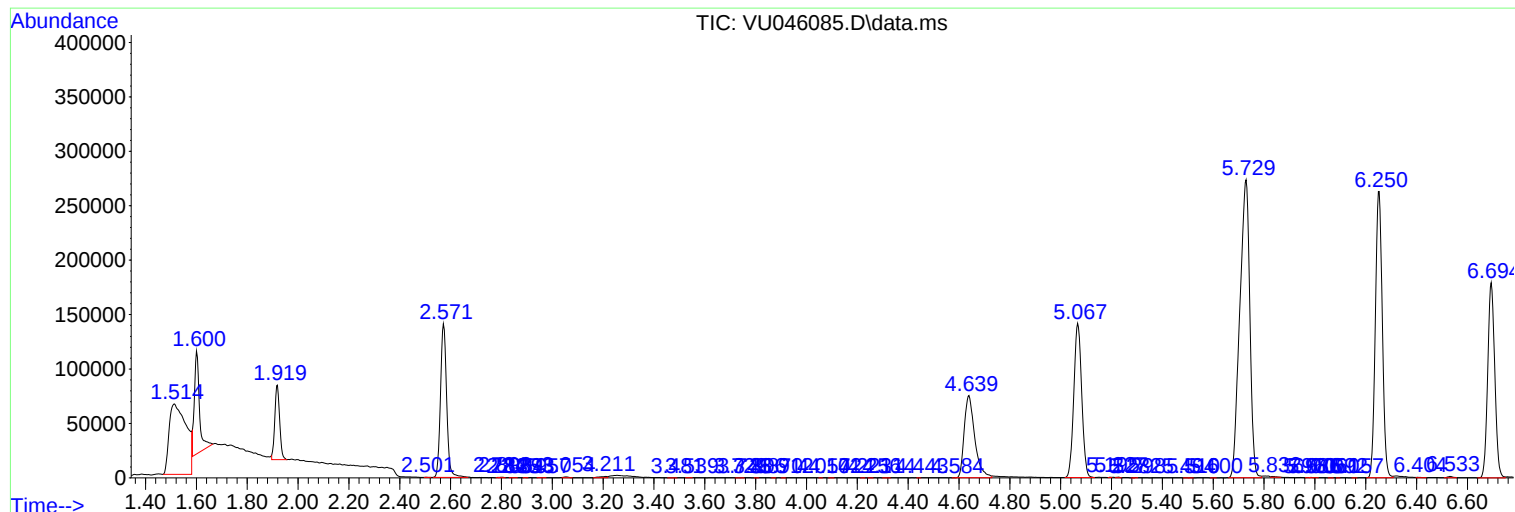

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
Data File : VU046085.D
Acq On : 03 Dec 2021 19:31
Operator : SY/MD
Sample : M4869-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESQP0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
Data File : VU046085.D
Acq On : 03 Dec 2021 19:31
Operator : SY/MD
Sample : M4869-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESQP0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc