


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120321\
Data File : VU046066.D
Acq On : 03 Dec 2021 10:02
Operator : SY/MD
Sample : BFB022
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB022

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Title : VOC Analysis
Last Update : Fri Dec 03 05:08:36 2021

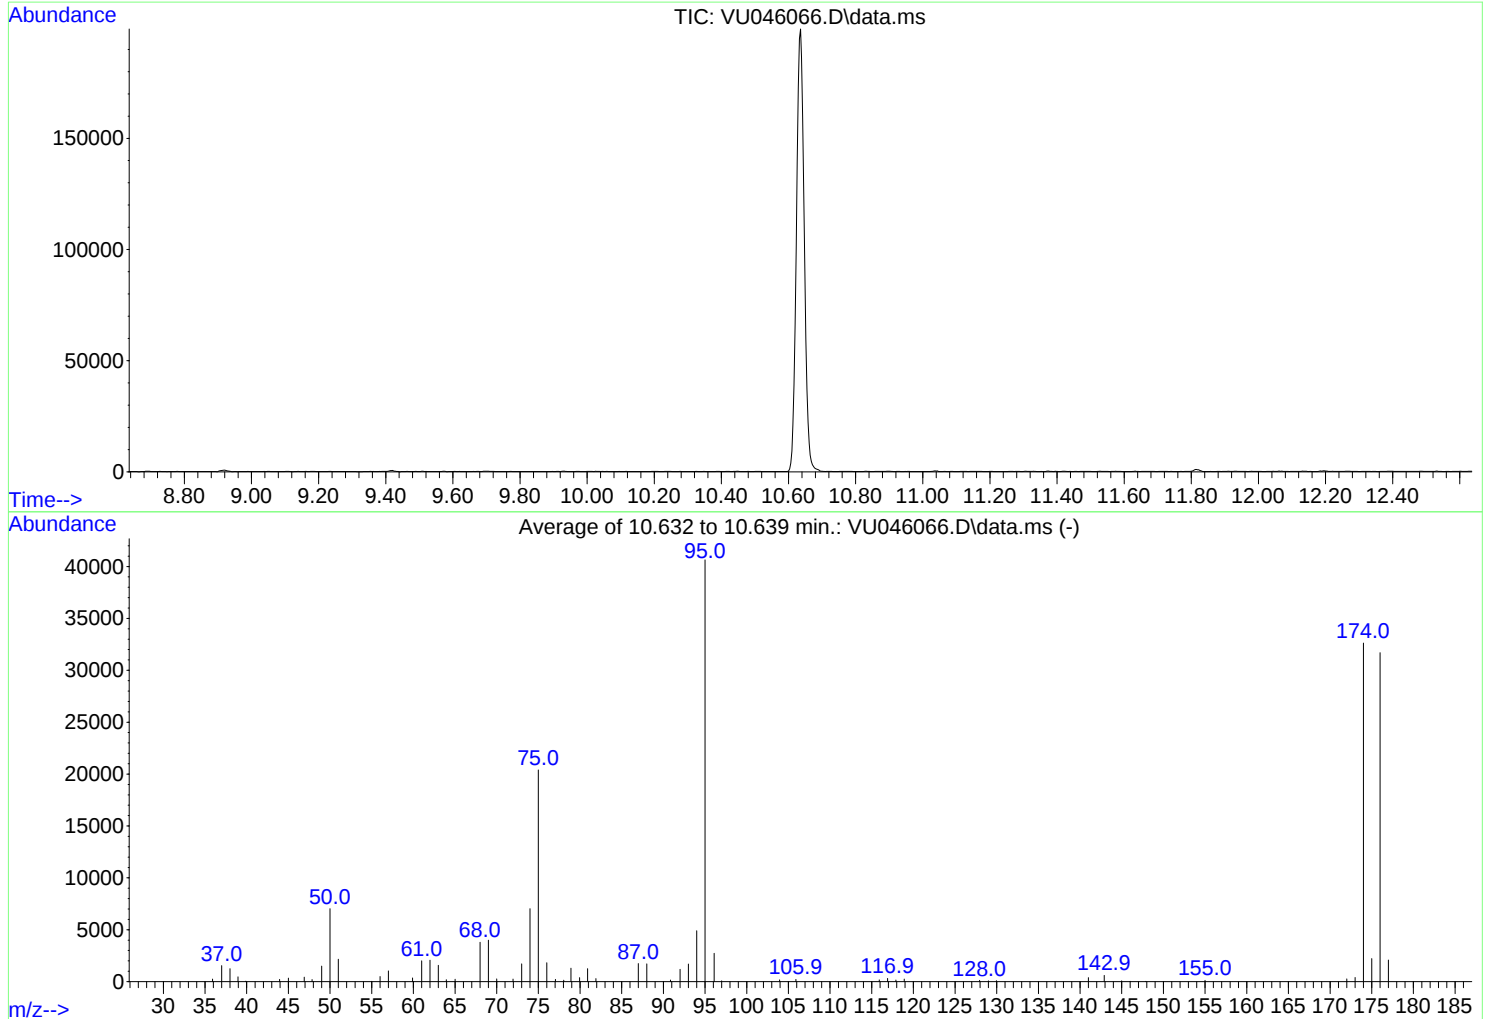

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	7029	PASS
75	95	30	80	50.2	20405	PASS
95	95	100	100	100.0	40645	PASS
96	95	5	9	6.7	2730	PASS
173	174	0.00	2	1.2	396	PASS
174	95	50	120	80.3	32627	PASS
175	174	5	9	6.8	2216	PASS
176	174	95	101	97.2	31701	PASS
177	176	5	9	6.6	2080	PASS

m/z	Abundance
44.00	172.0

Instrument :
MSVOA_U
ClientSampleId :
BFB022

m/z	Abundance
35.90	254.0
37.00	1583.0
38.00	1317.0
38.90	517.0
39.90	129.0
44.00	409.0
45.00	312.0
46.90	423.0
47.80	197.0
49.00	1549.0
50.00	7077.0
51.00	2328.0
56.00	507.0
57.00	1100.0
59.90	370.0
61.00	2065.0
62.00	2133.0
63.00	1715.0
63.90	185.0
65.00	247.0
68.00	3943.0
69.00	4165.0
70.10	294.0
72.00	241.0
73.00	1685.0
74.00	7015.0
75.00	21032.0
76.00	2045.0
77.10	240.0
78.10	115.0
78.90	1334.0
79.90	418.0
80.90	1284.0
81.90	288.0
87.00	1664.0
88.00	1647.0
90.80	154.0
92.00	1268.0
93.00	1759.0
94.00	4952.0
95.00	41016.0
96.10	2854.0
97.00	107.0
103.90	186.0
105.90	232.0
115.90	171.0
116.90	318.0
117.90	160.0
118.90	226.0
127.90	131.0
129.00	101.0
129.90	150.0
141.00	396.0
142.90	570.0
146.00	105.0
147.90	104.0
155.00	127.0
172.00	266.0
173.00	345.0
174.00	31800.0
175.00	2225.0
176.00	31064.0
177.00	2123.0

Instrument :
MSVOA_U
ClientSampleId :
BFB022

m/z	Abundance
35.90	262.0
37.00	1542.0
38.00	1264.0
39.00	469.0
43.90	399.0
45.00	366.0
46.90	441.0
47.80	202.0
49.00	1501.0
50.00	7201.0
51.00	2220.0
55.00	100.0
56.00	510.0
57.00	1049.0
59.90	377.0
61.00	2088.0
62.00	2164.0
63.00	1641.0
63.90	191.0
65.00	232.0
68.00	3907.0
69.00	4144.0
70.00	247.0
71.90	248.0
73.00	1806.0
74.00	7278.0
75.00	20984.0
76.00	1867.0
77.00	215.0
78.00	149.0
78.90	1331.0
80.00	391.0
80.90	1277.0
81.90	308.0
87.00	1804.0
88.00	1756.0
90.90	163.0
92.00	1247.0
93.00	1712.0
94.00	5070.0
95.00	41712.0
96.10	2811.0
97.00	103.0
104.00	184.0
105.90	227.0
115.90	173.0
116.90	334.0
117.90	161.0
118.90	271.0
128.00	116.0
129.00	112.0
130.00	126.0
141.00	397.0
142.90	635.0
145.00	101.0
155.00	132.0
172.00	254.0
173.00	401.0
174.00	33648.0
175.00	2257.0
176.00	32736.0
177.00	2141.0

Instrument :
MSVOA_U
ClientSampleId :
BFB022

m/z	Abundance
35.90	239.0
37.00	1486.0
38.00	1185.0
39.00	425.0
43.90	368.0
45.00	354.0
46.90	435.0
47.90	187.0
49.00	1438.0
50.00	6810.0
51.00	1942.0
56.00	460.0
57.00	957.0
59.90	340.0
61.00	1872.0
62.00	1894.0
63.00	1385.0
64.00	182.0
65.00	221.0
68.00	3511.0
69.00	3674.0
69.90	239.0
71.90	253.0
73.00	1651.0
74.00	6781.0
75.00	19200.0
76.00	1553.0
77.00	196.0
78.00	178.0
78.90	1229.0
80.00	355.0
80.90	1183.0
81.90	295.0
87.00	1762.0
88.00	1724.0
90.90	145.0
92.00	1067.0
93.00	1602.0
94.00	4686.0
95.00	39208.0
96.10	2525.0
103.90	159.0
105.90	207.0
115.90	152.0
116.90	287.0
117.90	143.0
118.90	253.0
128.00	107.0
141.00	369.0
142.90	619.0
145.00	108.0
155.00	135.0
172.00	259.0
173.00	443.0
174.00	32432.0
175.00	2166.0
176.00	31304.0
177.00	1976.0

Instrument :
MSVOA_U
ClientSampleId :
BFB022