
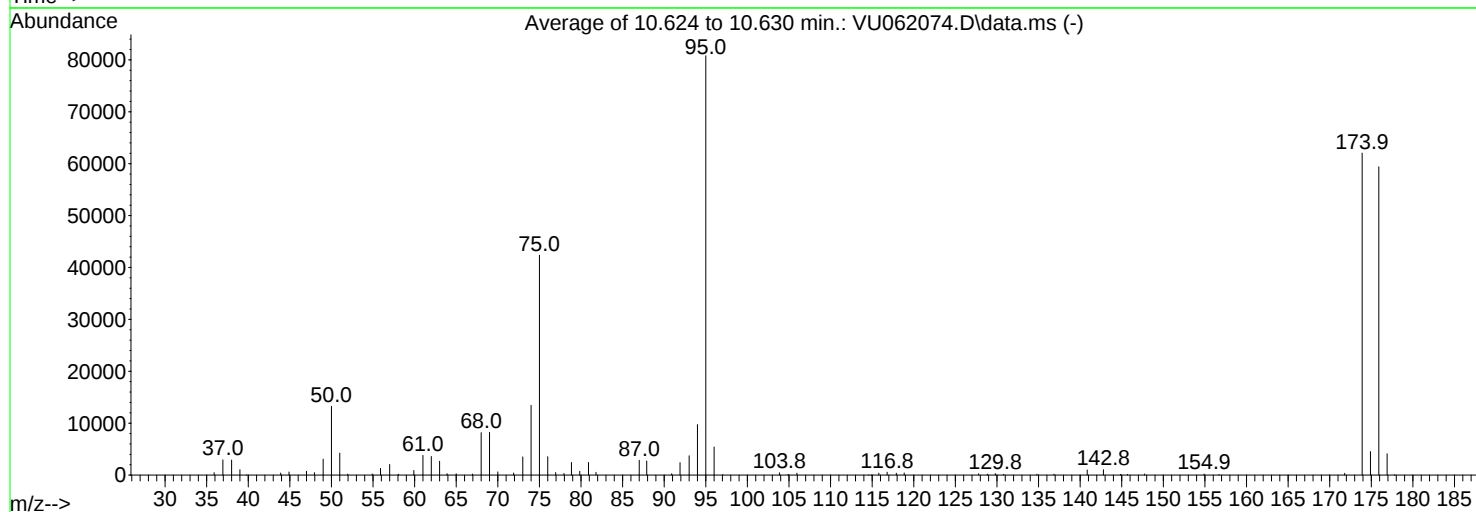


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120324\
Data File : VU062074.D
Acq On : 03 Dec 2024 08:10
Operator : MD/SY
Sample : BFB018
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB018

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120324.M
Title : TRACE VOA SOM01.0
Last Update : Tue Dec 03 20:41:18 2024

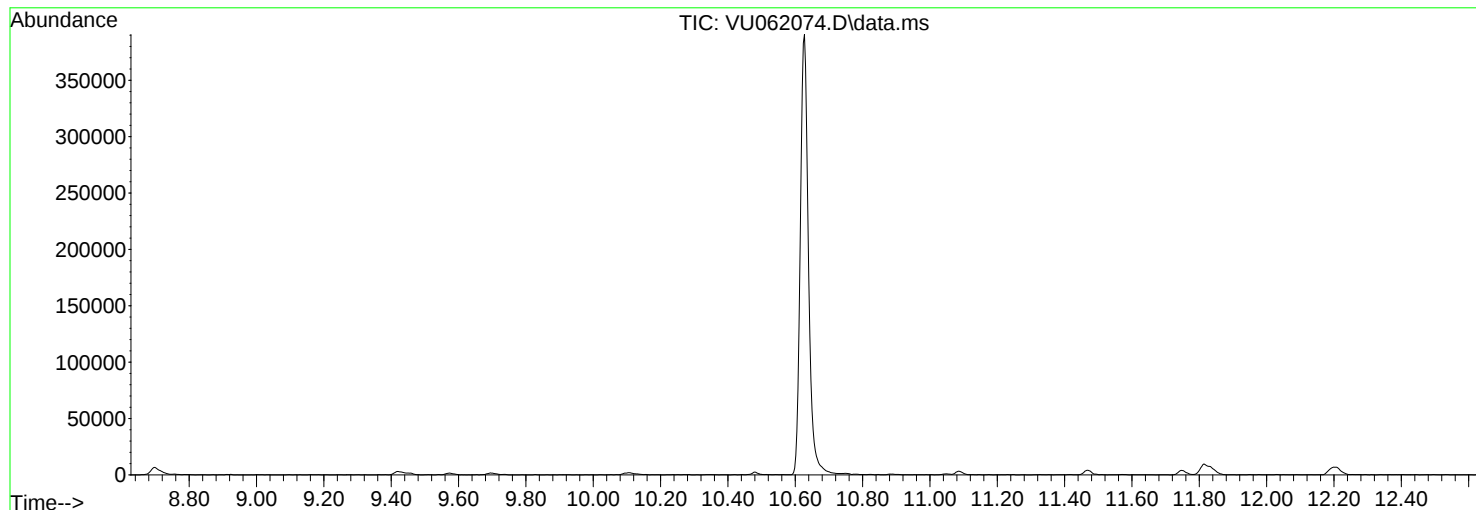

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	13251	PASS
75	95	30	80	52.4	42373	PASS
95	95	100	100	100.0	80800	PASS
96	95	5	9	6.7	5414	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.8	62040	PASS
175	174	5	9	7.3	4537	PASS
176	174	95	101	95.7	59403	PASS
177	176	5	9	6.9	4112	PASS

m/z	Abundance
43.90	174.0

Instrument :
MSVOA_U
ClientSampleId :
BFB018

m/z	Abundance
35.90	587.0
37.00	2967.0
38.00	2796.0
39.00	1088.0
39.80	103.0
43.90	585.0
44.90	610.0
47.00	683.0
48.00	423.0
49.00	3224.0
50.00	13942.0
51.00	4374.0
52.00	210.0
54.90	218.0
55.90	1281.0
57.00	2097.0
58.10	173.0
59.90	929.0
61.00	4095.0
62.00	3604.0
63.00	2709.0
63.90	284.0
65.10	263.0
67.00	262.0
68.00	8190.0
69.00	8433.0
70.00	661.0
71.90	474.0
73.00	3631.0
74.00	13792.0
75.00	42904.0
76.00	3656.0
76.90	518.0
78.00	316.0
78.80	2427.0
79.90	791.0
80.90	2531.0
81.90	589.0
87.00	2997.0
87.90	2665.0
90.90	272.0
91.90	2507.0
93.00	3726.0
94.00	9704.0
95.00	81784.0
96.00	5657.0
103.80	437.0
104.90	147.0
106.00	355.0
114.60	121.0
115.80	455.0
116.80	607.0
117.90	377.0
118.80	408.0
127.80	217.0
128.80	175.0
129.80	260.0
130.80	167.0
134.80	194.0
136.90	153.0
140.80	1006.0
142.80	1061.0
144.80	132.0
145.70	175.0
147.70	182.0
154.90	192.0
156.70	148.0
171.80	326.0
173.90	61976.0
174.90	4711.0
175.90	58936.0
176.90	4186.0
177.80	107.0

Instrument :
MSVOA_U
ClientSampleId :
BFB018

m/z	Abundance
35.90	483.0
37.00	2975.0
38.00	3017.0
39.00	1065.0
43.90	594.0
44.90	620.0
47.00	777.0
47.90	492.0
49.00	3185.0
50.00	13676.0
51.00	4361.0
52.00	200.0
54.90	234.0
55.90	1346.0
57.00	2133.0
58.10	185.0
59.90	920.0
61.00	3924.0
62.00	3688.0
63.00	2728.0
63.90	283.0
65.00	253.0
66.90	205.0
68.00	8489.0
69.00	8522.0
70.00	652.0
71.90	402.0
73.00	3593.0
74.00	13996.0
75.00	43632.0
76.00	3640.0
76.90	507.0
77.90	344.0
78.90	2513.0
79.80	755.0
80.90	2517.0
81.80	543.0
87.00	2898.0
87.90	2811.0
90.90	270.0
91.90	2468.0
93.00	3907.0
94.00	10030.0
95.00	83320.0
96.00	5605.0
97.00	122.0
103.90	465.0
104.90	155.0
105.90	395.0
114.90	105.0
115.80	389.0
116.80	588.0
117.90	379.0
118.80	403.0
127.80	276.0
128.90	183.0
129.80	292.0
130.80	137.0
134.80	179.0
136.90	188.0
140.90	1035.0
142.80	1058.0
144.80	133.0
145.70	155.0
147.80	224.0
154.90	220.0
156.70	125.0
171.80	374.0
173.90	63840.0
174.90	4651.0
175.90	61256.0
176.90	4259.0
177.80	125.0

Instrument :
MSVOA_U
ClientSampleId :
BFB018

m/z	Abundance
35.90	368.0
36.90	2852.0
38.00	2862.0
39.00	960.0
43.90	545.0
44.90	578.0
47.00	754.0
47.90	489.0
49.00	2817.0
50.00	12135.0
51.00	3984.0
51.90	163.0
54.90	228.0
55.90	1208.0
57.00	1909.0
58.00	129.0
59.90	810.0
61.00	3374.0
62.00	3482.0
63.00	2552.0
63.90	268.0
64.90	254.0
66.90	149.0
68.00	7845.0
69.00	7749.0
70.00	538.0
71.90	358.0
73.00	3308.0
74.00	12532.0
75.00	40584.0
76.00	3330.0
77.00	460.0
77.90	298.0
78.90	2363.0
79.80	656.0
80.90	2263.0
81.70	498.0
87.00	2689.0
87.90	2695.0
90.90	233.0
91.90	2236.0
93.00	3560.0
94.00	9470.0
95.00	77296.0
96.00	4979.0
97.10	118.0
103.90	431.0
104.90	155.0
105.90	388.0
115.80	289.0
116.80	514.0
117.90	349.0
118.90	433.0
127.80	285.0
128.90	168.0
129.80	326.0
130.70	101.0
134.80	176.0
136.80	200.0
140.90	922.0
142.80	985.0
144.90	128.0
145.70	112.0
147.80	246.0
154.90	209.0
156.70	108.0
171.80	376.0
173.90	60304.0
174.90	4248.0
175.90	58016.0
176.90	3892.0

Instrument :
MSVOA_U
ClientSampleId :
BFB018