
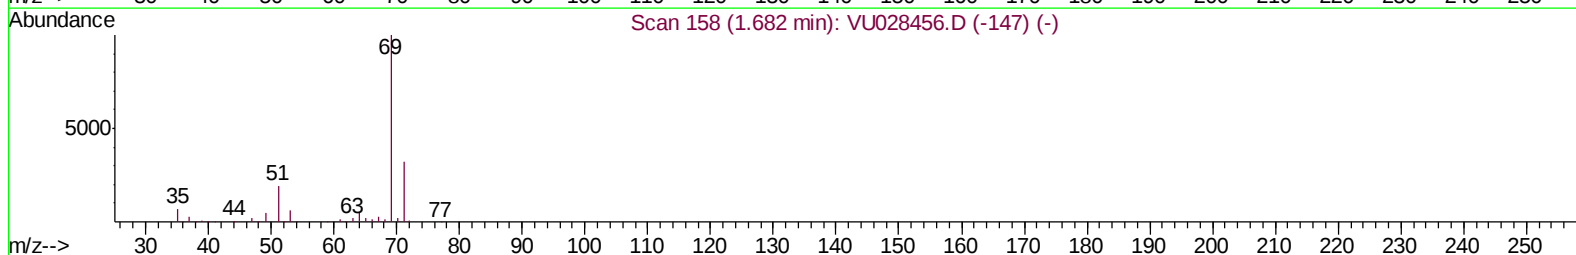
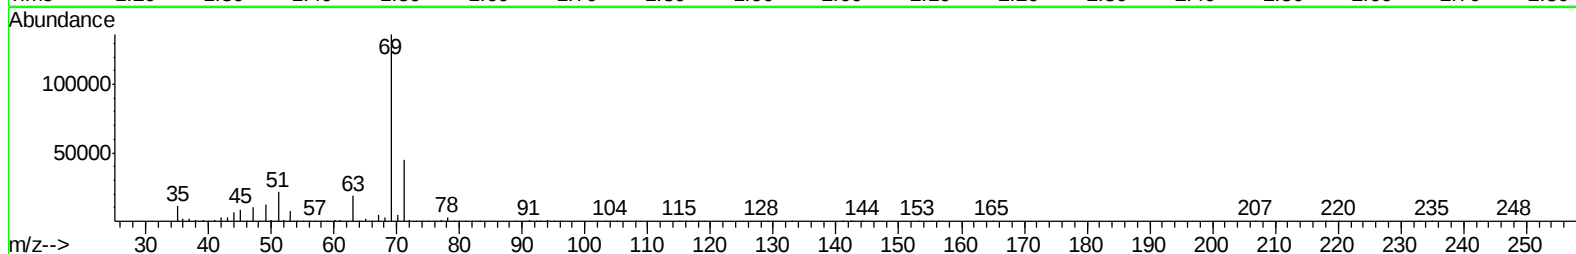


Data File : VU028465.D
Acq On : 04 Dec 2018 14:15
Operator : MD/SY
Sample : J6171-05ME RE
Misc : 6.73g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Dec 05 03:14:34 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM113018WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 05 03:10:52 2018
Response via : Initial Calibration

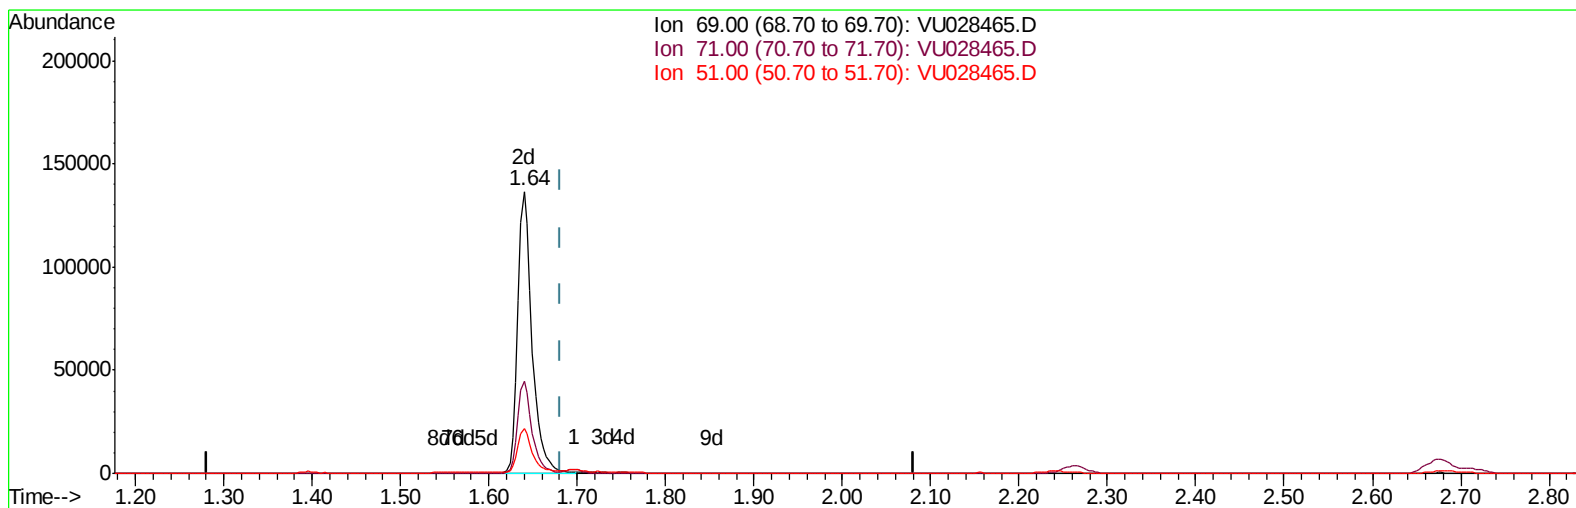

TIC: VU028465.D

(7) Chloroethane-d5 (S)

1.640min (-0.042) 32.10ug/L m

response 153490

Ion	Exp%	Act%
69.00	100	100
71.00	31.70	1.59#
51.00	28.20	1.12#
0.00	0.00	0.00