


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU120418\
 Data File : VU028455.D
 Acq On : 04 Dec 2018 09:39
 Operator : MD/SY
 Sample : BFB60
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB60

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM113018WMA.M
 Title : VOC Analysis
 Last Update : Wed Dec 05 03:10:52 2018

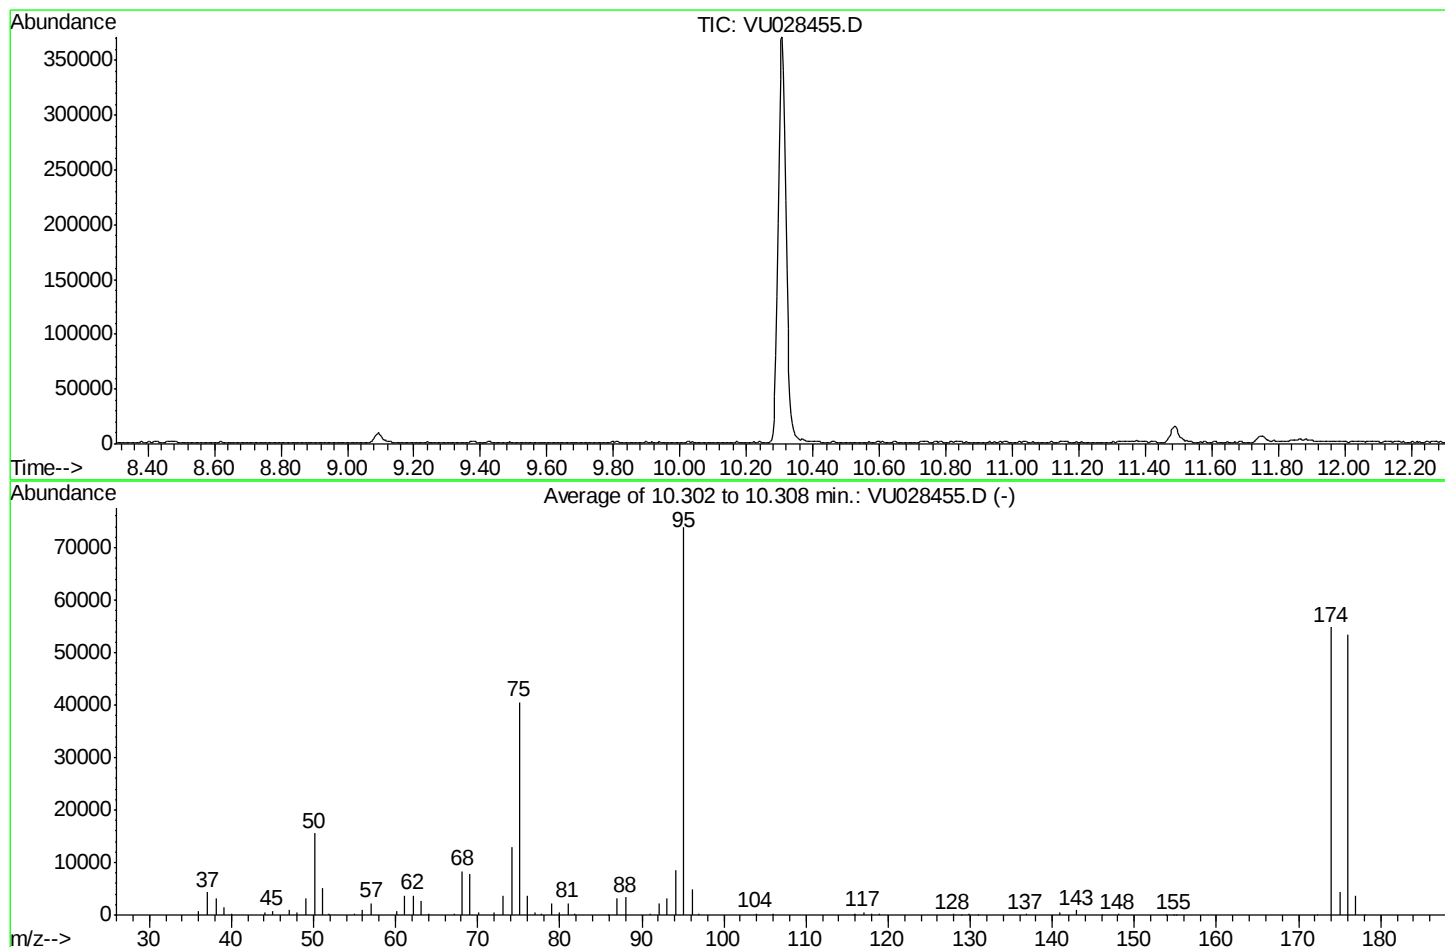

AutoFind: Scans 2839, 2840, 2841; Background Corrected with Scan 2827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	15591	PASS
75	95	30	80	54.9	40552	PASS
95	95	100	100	100.0	73864	PASS
96	95	5	9	6.7	4914	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	74.2	54837	PASS
175	174	5	9	8.1	4442	PASS
176	174	95	101	97.2	53304	PASS
177	176	5	9	6.7	3577	PASS

m/z	Abundance
36.00	795.0
37.10	4379.0
38.10	3037.0
39.10	1483.0
40.10	278.0
44.10	1192.0
45.00	722.0
47.10	937.0
48.10	469.0
49.10	2903.0
50.10	14701.0
51.10	5089.0
52.00	275.0
55.00	176.0
56.00	1002.0
57.10	2296.0
60.10	635.0
61.00	3191.0
62.10	3695.0
63.10	2434.0
64.00	315.0
67.10	151.0
68.10	7998.0
69.10	7531.0
70.10	512.0
72.00	450.0
73.10	3298.0
74.10	11935.0
75.10	38216.0
76.10	3638.0
77.00	500.0
77.80	324.0
79.00	2107.0
80.00	437.0
81.00	2119.0
81.80	301.0
87.00	3154.0
88.00	2928.0
91.00	257.0
92.10	2188.0
93.10	2873.0
94.10	7655.0
95.10	69584.0
96.10	4459.0
97.00	151.0
103.90	313.0
106.00	348.0
115.80	171.0
117.00	441.0
118.00	233.0
118.90	218.0
127.90	205.0
129.80	162.0
136.80	114.0
140.90	542.0
143.00	733.0
146.00	130.0
148.00	195.0
172.20	246.0
174.00	50176.0
175.00	4051.0
176.00	48480.0
177.00	3028.0
178.00	100.0

Instrument :
MSVOA_U
ClientSampleId :
BFB60

Scan 2827 (10.263 min): VU028455.D
BFB60

m/z	Abundance
39.10	109.0
40.00	247.0
41.10	110.0
44.10	702.0
207.00	105.0

Instrument :
MSVOA_U
ClientSampleId :
BFB60

m/z	Abundance
36.00	846.0
37.10	4239.0
38.10	3289.0
39.10	1486.0
40.10	534.0
44.10	1283.0
45.00	943.0
47.10	1061.0
48.00	592.0
49.10	3454.0
50.10	15913.0
51.10	4823.0
51.90	227.0
55.00	256.0
56.00	1059.0
57.10	2247.0
60.10	857.0
61.00	3825.0
62.10	3577.0
63.10	2671.0
64.00	186.0
67.20	208.0
68.10	8321.0
69.10	8110.0
70.10	558.0
72.00	478.0
73.10	3762.0
74.10	13538.0
75.10	41512.0
76.10	3543.0
77.00	631.0
77.80	389.0
79.00	2257.0
80.00	588.0
81.00	2466.0
81.90	427.0
85.90	134.0
87.00	3338.0
88.00	3645.0
91.10	347.0
92.00	2284.0
93.10	3289.0
94.10	9036.0
95.10	75600.0
96.10	5216.0
97.00	212.0
103.90	382.0
106.00	338.0
116.00	381.0
117.00	653.0
117.90	142.0
118.90	280.0
127.90	243.0
129.00	120.0
129.90	255.0
131.00	100.0
136.80	152.0
140.90	641.0
142.90	953.0
148.00	183.0
153.90	105.0
154.90	231.0
174.00	57784.0
175.00	4621.0
176.00	56360.0
177.00	4024.0
207.10	189.0

Instrument :
MSVOA_U
ClientSampleId :
BFB60

m/z	Abundance
36.00	880.0
37.10	4483.0
38.10	3310.0
39.10	1600.0
40.10	410.0
44.10	1297.0
45.00	925.0
47.10	1000.0
48.10	602.0
49.10	3297.0
50.10	16161.0
51.10	5124.0
52.00	270.0
55.00	211.0
56.00	1027.0
57.10	2340.0
60.10	863.0
61.00	3716.0
62.10	3846.0
63.10	2725.0
64.00	253.0
67.20	193.0
68.10	8589.0
69.10	8157.0
70.10	571.0
72.00	507.0
73.10	3743.0
74.10	13015.0
75.10	41928.0
76.10	3795.0
77.00	581.0
77.80	354.0
79.00	2301.0
80.00	537.0
81.00	2377.0
81.90	370.0
85.90	132.0
87.00	3252.0
88.00	3404.0
91.00	297.0
92.00	2352.0
93.10	3330.0
94.10	8715.0
95.10	76408.0
96.10	5068.0
97.00	227.0
103.90	366.0
106.00	355.0
116.00	263.0
117.00	590.0
118.00	164.0
118.90	276.0
127.90	249.0
128.90	119.0
129.90	196.0
136.80	143.0
140.90	619.0
143.00	913.0
146.00	127.0
148.10	212.0
154.80	137.0
155.10	136.0
174.00	56552.0
175.00	4655.0
176.00	55072.0
177.00	3680.0
207.00	113.0

Instrument :
MSVOA_U
ClientSampleId :
BFB60