

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U120419\
 Data File : VU035963.D
 Acq On : 04 Dec 2019 11:40
 Operator : JC/SP
 Sample : K6105-01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFE21

Quant Time: Dec 05 04:10:36 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR120319WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Dec 05 03:54:31 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	296236	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.45	117	331038	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.84	152	102741	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	158191	4.69	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.80%
7) Chloroethane-d5	1.93	69	132751	4.90	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.00%
11) 1,1-Dichloroethene-d2	2.59	63	174746	3.60	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.00%
20) 2-Butanone-d5	4.70	46	279933	46.81	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.62%
24) Chloroform-d	5.11	84	230457	4.97	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.40%
26) 1,2-Dichloroethane-d4	5.75	65	121290	4.94	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.80%
32) Benzene-d6	5.77	84	441792	4.51	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.20%
36) 1,2-Dichloropropane-d6	6.73	67	140459	4.43	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.60%
41) Toluene-d8	7.93	98	347583	3.85	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.00%
43) trans-1,3-Dichloropropene-	8.21	79	52303	4.08	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.60%
46) 2-Hexanone-d5	8.68	63	202812	40.22	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	80.44%
57) 1,1,2,2-Tetrachloroethane-	10.78	84	118212	4.43	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.60%
64) 1,2-Dichlorobenzene-d4	12.22	152	107450	5.06	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.20%


Target Compounds					Ovalue
13) Acetone	2.68	43	11008	2.036 ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU120419\
Data File : VU035963.D
Acq On : 04 Dec 2019 11:40
Operator : JC/SP
Sample : K6105-01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFE21

Quant Time: Dec 05 04:10:36 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR120319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 05 03:54:31 2019
Response via : Initial Calibration

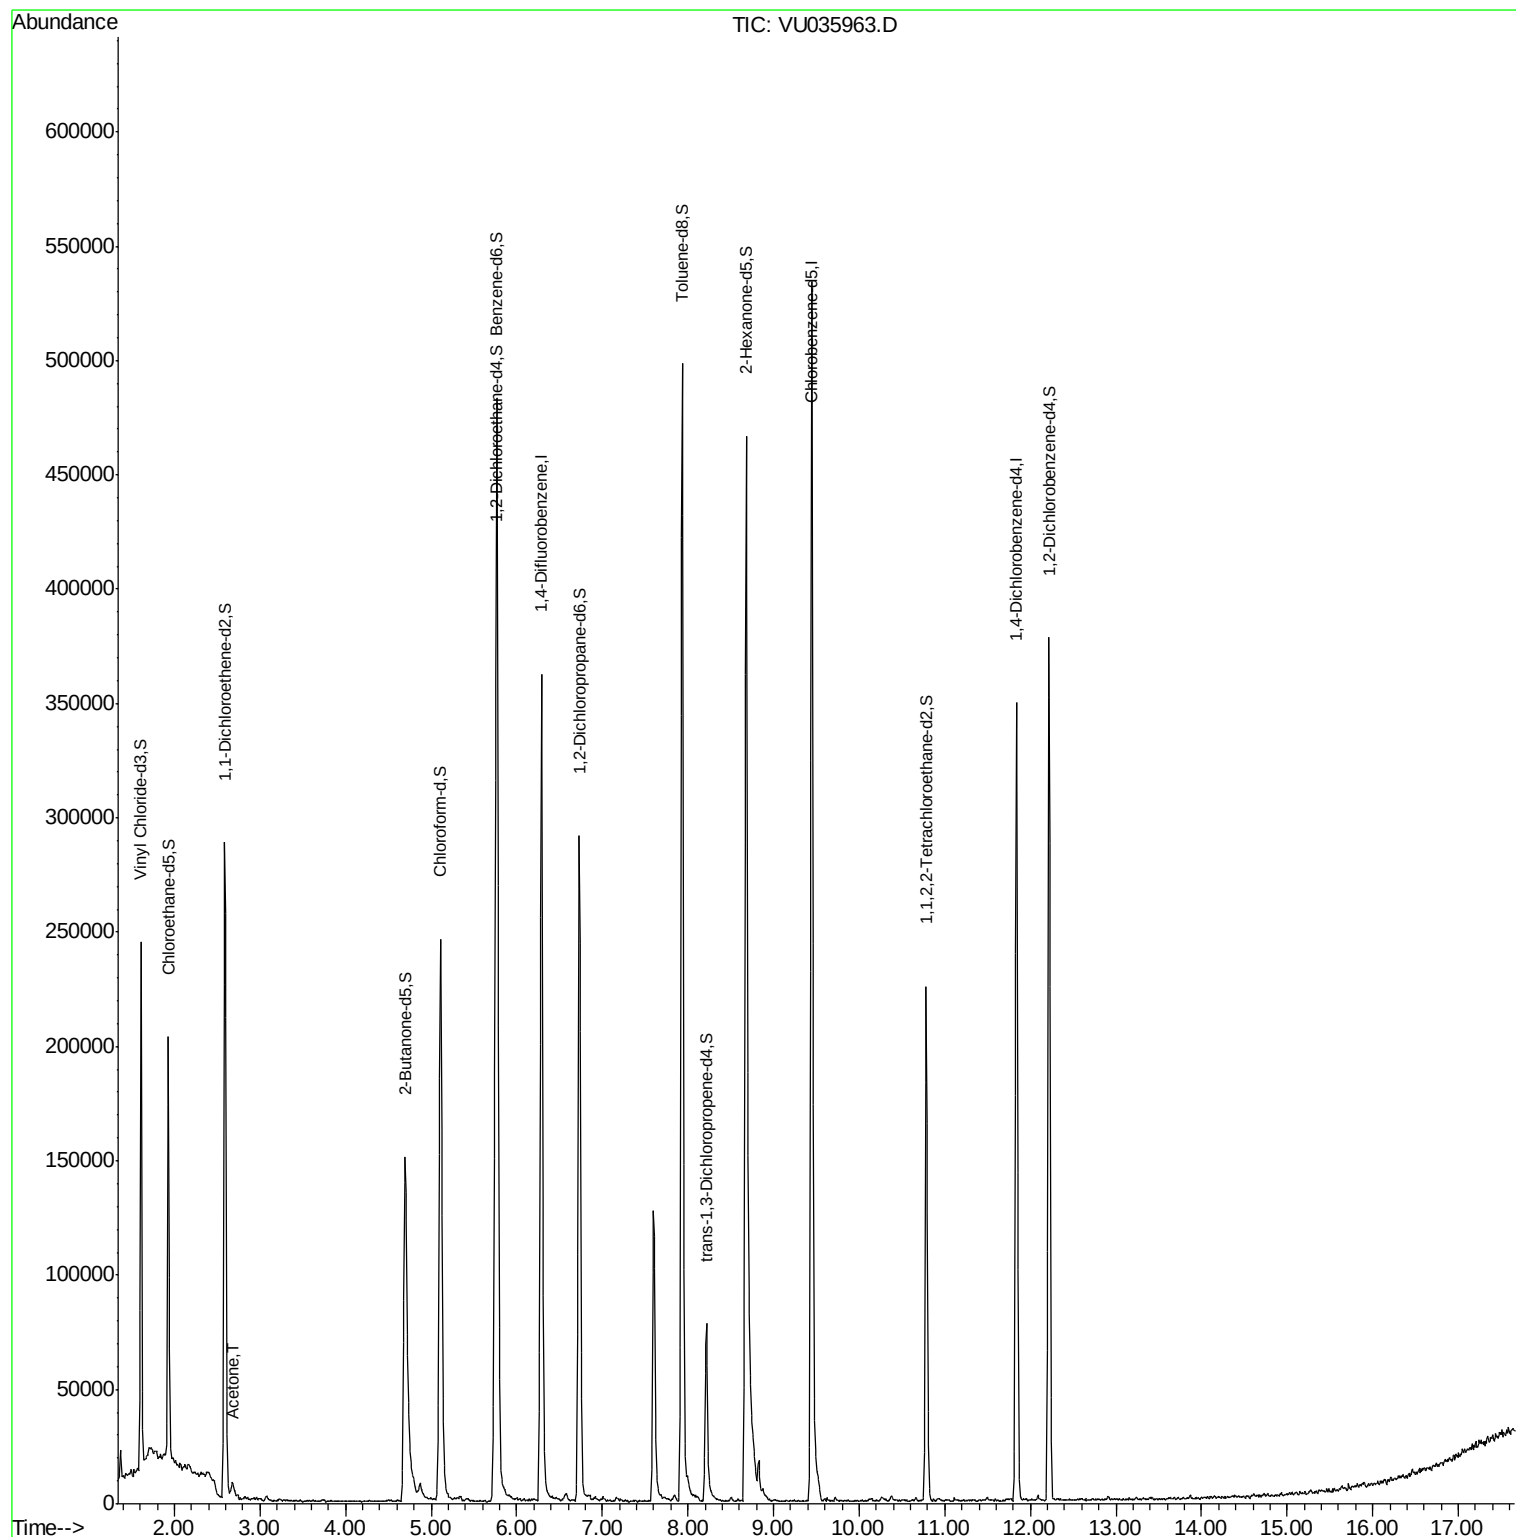

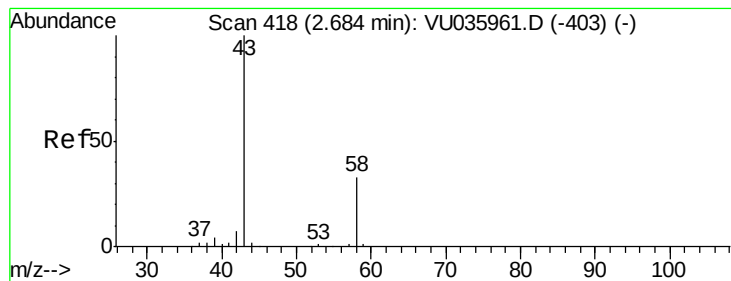

#13
Acetone
Concen: 2.036 ug/L
RT: 2.68 min Scan# 417
Delta R.T. -0.00 min
Lab File: VU035963.D
Acq: 04 Dec 2019 11:40

Instrument :
MSVOA_U
ClientSampleId :
BFE21

Tot Ion: 43 Resp: 11008
Ion Ratio Lower Upper
43 100
58 28.6 0.0 68.6

