

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU120419\
 Data File : VU035965.D
 Acq On : 04 Dec 2019 12:29
 Operator : JC/SP
 Sample : K6056-14DL 20X
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFE20DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR120319WMA.M
 Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.610	74	84	94	rBV	222880	252826	19.66%	2.310%
2	1.932	176	184	197	rVB	173441	220658	17.16%	2.016%
3	2.437	339	341	357	rVB2	8092	14237	1.11%	0.130%
4	2.594	378	390	408	rBV	278817	447810	34.82%	4.091%
5	3.083	531	542	556	rBV2	12294	23308	1.81%	0.213%
6	4.703	1030	1046	1087	rBV	148054	492195	38.27%	4.497%
7	5.112	1156	1173	1193	rBV	230339	524147	40.75%	4.789%
8	5.771	1357	1378	1412	rBV2	462156	1193819	92.81%	10.906%
9	6.292	1525	1540	1569	rBV	374377	740494	57.57%	6.765%
10	6.581	1619	1630	1647	rVB2	34372	66406	5.16%	0.607%
11	6.732	1661	1677	1700	rBV2	287701	574685	44.68%	5.250%
12	7.604	1935	1948	1973	rBV	124514	243713	18.95%	2.227%
13	7.935	2037	2051	2071	rBV	484591	878861	68.33%	8.029%
14	8.218	2127	2139	2158	rBV2	76244	151983	11.82%	1.388%
15	8.584	2239	2253	2269	rBV	750345	1286240	100.00%	11.751%
16	8.681	2271	2283	2330	rVB	481535	1168798	90.87%	10.678%
17	9.449	2508	2522	2560	rVB	540215	1003585	78.02%	9.169%
18	10.784	2925	2937	2953	rBV	225347	383275	29.80%	3.502%
19	11.838	3250	3265	3285	rBV	364404	633188	49.23%	5.785%
20	12.218	3369	3383	3398	rBV	374136	645717	50.20%	5.899%


Sum of corrected areas: 10945945

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU120419\
Data File : VU035965.D
Acq On : 04 Dec 2019 12:29
Operator : JC/SP
Sample : K6056-14DL 20X
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFE20DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR120319WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

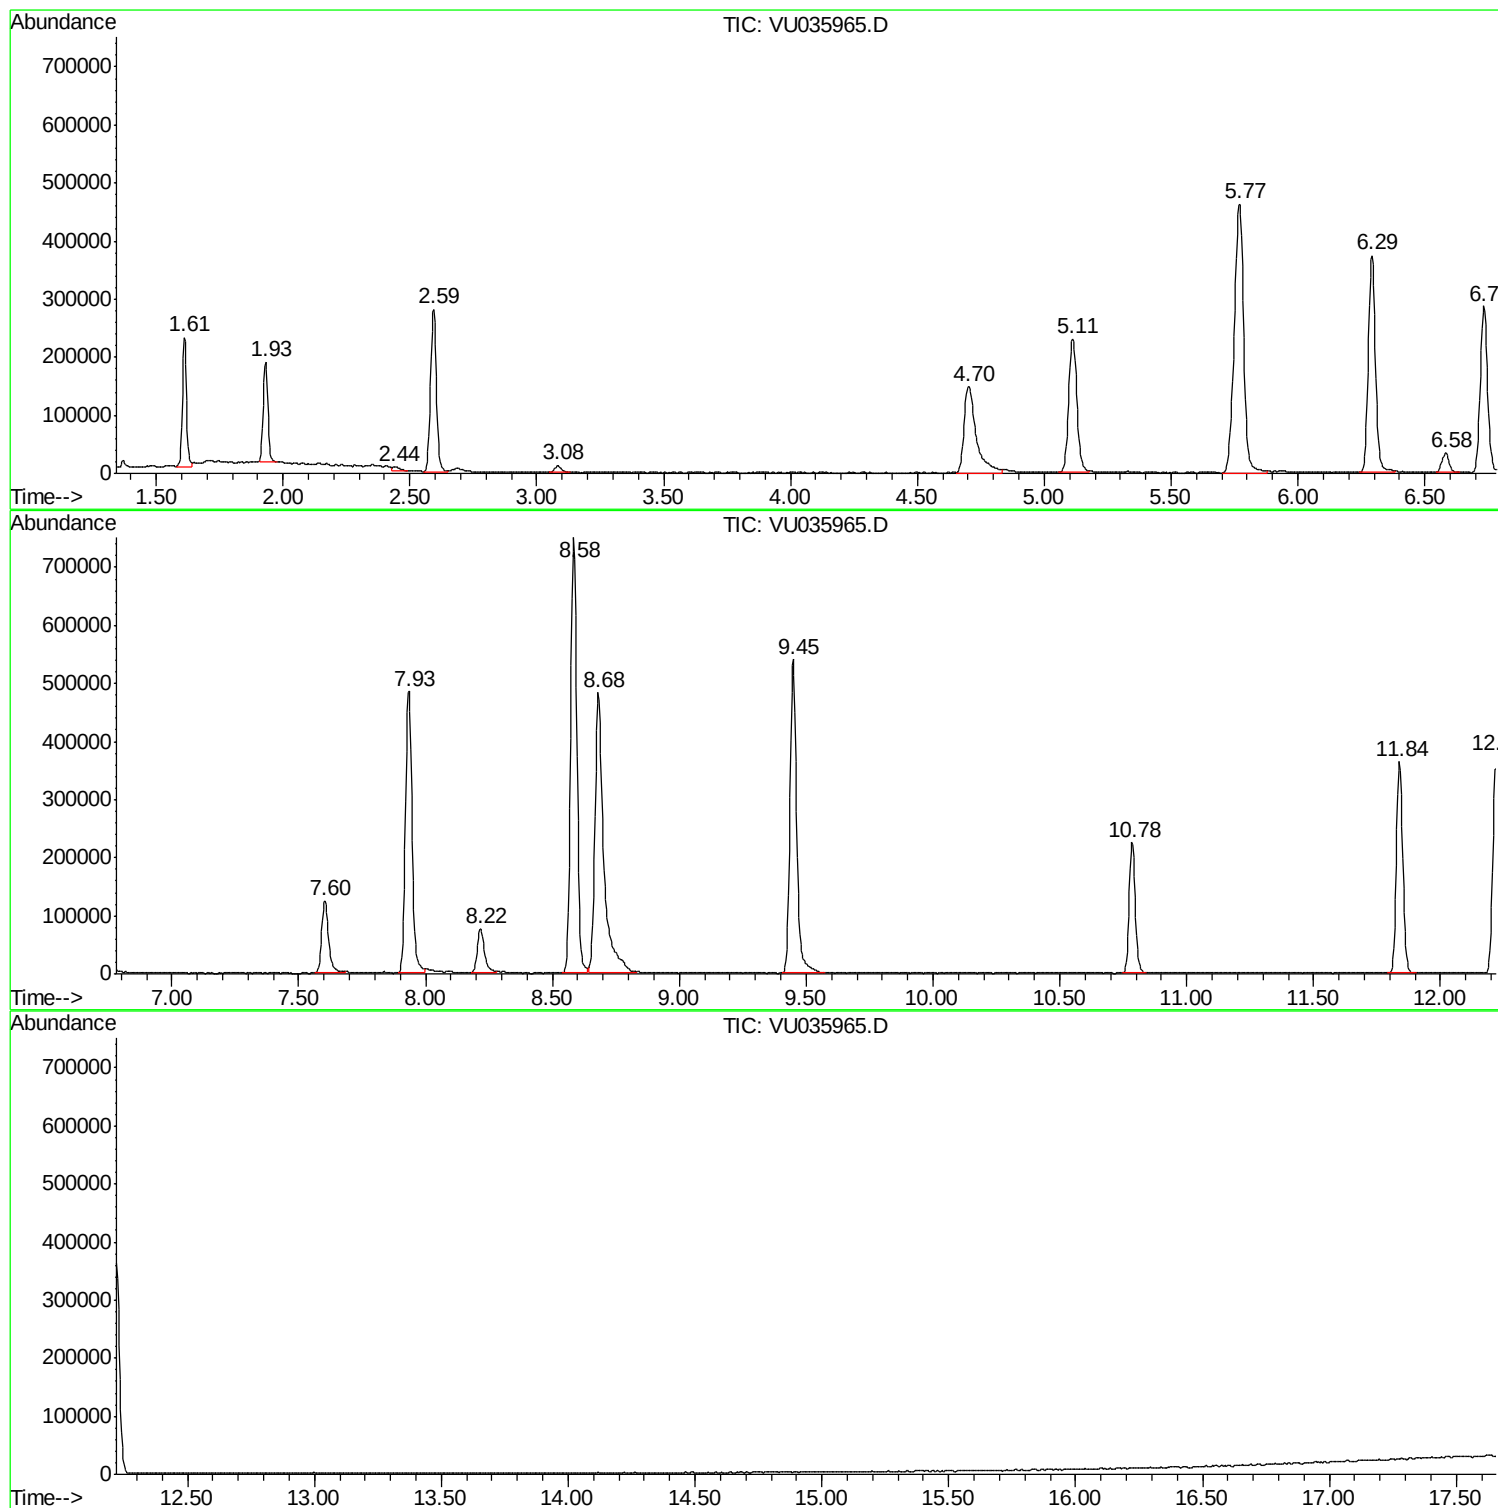

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU120419\
Data File : VU035965.D
Acq On : 04 Dec 2019 12:29
Operator : JC/SP
Sample : K6056-14DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFE20DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR120319WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU120419\
Data File : VU035965.D
Acq On : 04 Dec 2019 12:29
Operator : JC/SP
Sample : K6056-14DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFE20DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR120319WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc