


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU120419\
 Data File : VU035960.D
 Acq On : 04 Dec 2019 09:43
 Operator : JC/SP
 Sample : BFB11
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB11

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR120319WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Dec 06 00:57:26 2019

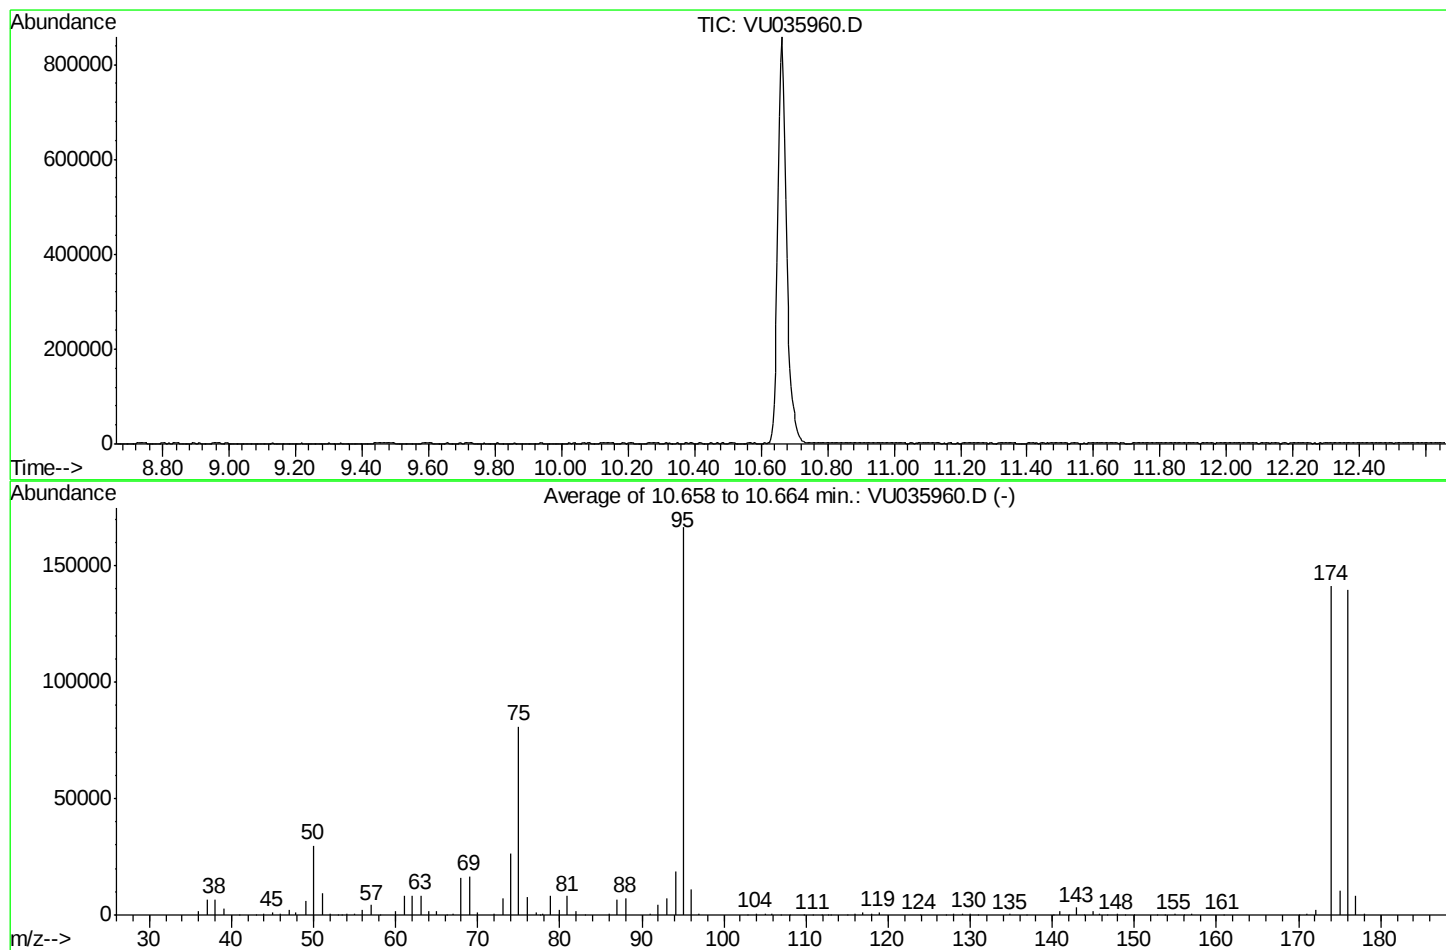

AutoFind: Scans 2898, 2899, 2900; Background Corrected with Scan 2883

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	29704	PASS
75	95	30	80	48.6	80952	PASS
95	95	100	100	100.0	166464	PASS
96	95	5	9	6.6	10917	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.9	141333	PASS
175	174	5	9	7.6	10718	PASS
176	174	95	101	98.7	139434	PASS
177	176	5	9	6.0	8383	PASS

m/z	Abundance
36.00	1412.0
37.10	6678.0
38.00	6561.0
39.10	2921.0
40.00	551.0
44.00	1807.0
45.00	1465.0
46.00	355.0
47.10	2315.0
47.90	1132.0
49.00	5827.0
50.00	29448.0
51.00	9071.0
52.00	590.0
52.90	158.0
53.40	106.0
54.10	395.0
55.10	437.0
56.00	2434.0
57.10	4286.0
58.10	156.0
60.00	1757.0
61.00	8306.0
62.00	8336.0
63.10	8523.0
64.10	1874.0
65.00	1437.0
66.20	106.0
67.10	505.0
68.00	15313.0
69.00	15884.0
70.00	1364.0
72.00	794.0
73.00	7001.0
74.00	24816.0
75.00	78744.0
76.10	7473.0
77.10	989.0
77.60	511.0
78.90	7960.0
79.90	1968.0
80.90	7798.0
82.00	1567.0
83.00	136.0
85.90	407.0
87.00	6306.0
88.00	7132.0
91.00	744.0
92.00	4257.0
93.00	7017.0
94.10	18712.0
95.00	161024.0
96.00	10522.0
97.00	343.0
102.80	105.0
103.90	772.0
105.00	284.0
106.00	805.0
106.90	181.0
108.00	226.0
109.80	152.0
110.90	161.0
111.90	103.0
112.70	144.0
115.00	142.0
116.00	562.0
117.00	1244.0
118.00	582.0
118.90	1467.0
123.90	207.0
127.00	135.0
128.00	504.0
129.00	366.0
130.00	571.0
130.90	172.0
134.90	268.0
136.80	215.0
140.10	191.0
141.00	1440.0
142.10	329.0
142.90	3369.0
143.90	164.0
144.90	1577.0
145.80	344.0
146.80	161.0
147.90	444.0
148.90	136.0
152.70	157.0
153.60	157.0
154.90	414.0
156.90	370.0
160.90	177.0

Instrument :
MSVOA_U
ClientSampleId :
BFB11

170.00	135.0
171.00	777.0
172.00	1997.0
174.00	134144.0
175.00	10188.0
176.00	132864.0
176.90	7949.0
178.00	303.0

Instrument :
MSVOA_U
ClientSampleId :
BFB11

m/z	Abundance
36.00	1590.0
37.10	6994.0
38.00	6950.0
39.00	3098.0
40.10	461.0
41.00	152.0
44.00	1683.0
45.00	1389.0
46.00	431.0
47.10	2445.0
47.90	1046.0
49.00	6276.0
50.00	30616.0
51.10	9619.0
52.00	553.0
53.00	205.0
54.10	444.0
55.00	476.0
56.00	2608.0
57.10	4317.0
58.10	190.0
60.00	1774.0
61.00	8627.0
62.00	8422.0
63.10	8740.0
64.10	1864.0
65.00	1543.0
66.20	119.0
67.10	467.0
68.00	16424.0
69.00	17024.0
70.00	1420.0
72.00	839.0
73.10	7378.0
74.00	26680.0
75.00	83096.0
76.10	7801.0
77.10	1216.0
78.00	536.0
78.90	8591.0
79.90	2160.0
81.00	8370.0
82.00	1637.0
83.10	176.0
86.00	425.0
87.00	6631.0
88.00	7651.0
91.00	731.0
92.00	4794.0
93.00	7565.0
94.10	19128.0
95.00	171264.0
96.00	11234.0
97.00	453.0
103.90	838.0
105.00	334.0
105.90	711.0
106.90	293.0
108.00	265.0
109.80	175.0
110.80	170.0
113.00	131.0
115.00	158.0
116.00	602.0
116.90	1244.0
118.00	670.0
118.90	1427.0
123.90	122.0
127.00	119.0
127.90	546.0
129.00	320.0
130.00	626.0
130.90	273.0
134.90	374.0
136.80	255.0
140.10	169.0
141.00	1600.0
142.10	332.0
143.00	3332.0
143.90	142.0
145.00	1754.0
145.80	313.0
146.80	149.0
147.80	450.0
148.90	105.0
150.00	136.0
152.70	141.0
153.70	171.0
154.90	426.0
156.10	131.0
156.90	447.0
160.80	159.0

Instrument :
MSVOA_U
ClientSampleId :
BFB11

170.10	169.0
171.00	802.0
172.10	2135.0
174.00	145408.0
175.00	10901.0
176.00	143552.0
177.00	8690.0
178.00	310.0

Instrument :
MSVOA_U
ClientSampleId :
BFB11

m/z	Abundance
36.00	1462.0
37.10	6705.0
38.00	6936.0
39.00	3073.0
39.90	451.0
41.00	161.0
43.00	137.0
44.00	1562.0
45.00	1242.0
46.00	438.0
47.10	2122.0
47.90	865.0
49.00	6330.0
50.00	29048.0
51.10	9347.0
52.00	505.0
53.00	279.0
54.00	440.0
55.00	546.0
56.00	2433.0
57.10	3901.0
58.20	171.0
60.00	1658.0
61.00	8282.0
62.00	7344.0
63.10	8257.0
64.10	1753.0
65.00	1658.0
66.20	100.0
67.00	436.0
68.00	15725.0
69.00	16968.0
70.00	1318.0
72.00	796.0
73.10	7050.0
74.00	27072.0
75.00	81016.0
76.10	7201.0
77.10	1155.0
77.90	689.0
78.90	8001.0
79.90	2065.0
81.00	8103.0
82.00	1657.0
83.10	209.0
86.10	405.0
87.00	7042.0
88.00	7386.0
91.00	650.0
92.00	4705.0
93.00	7725.0
94.10	18608.0
95.00	167104.0
96.00	10996.0
96.90	438.0
103.90	817.0
105.00	350.0
105.80	615.0
107.00	324.0
107.90	216.0
109.80	162.0
110.80	182.0
113.00	169.0
115.00	151.0
115.90	665.0
116.90	1231.0
118.00	680.0
118.90	1233.0
127.90	560.0
129.00	293.0
129.90	537.0
130.90	384.0
134.90	407.0
136.80	271.0
140.00	147.0
140.90	1656.0
141.90	221.0
143.00	3186.0
143.90	132.0
145.00	1858.0
145.80	266.0
146.70	146.0
147.80	457.0
150.00	150.0
153.60	119.0
154.90	440.0
156.10	161.0
156.90	437.0
160.80	166.0
170.10	151.0
170.90	702.0
172.00	2205.0

Instrument :
MSVOA_U
ClientSampleId :
BFB11

174.00	144448.0
175.00	11067.0
176.00	141888.0
177.00	8511.0
178.00	277.0

Instrument :
MSVOA_U
ClientSampleId :
BFB11

Scan 2883 (10.610 min): VU035960.D
BFB11

m/z	Abundance
40.00	513.0
44.00	1048.0

Instrument :
MSVOA_U
ClientSampleId :
BFB11