

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U120420\
 Data File : VU041477.D
 Acq On : 04 Dec 2020 17:49
 Operator : SY/MD
 Sample : VIBLK08
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK08

Quant Time: Dec 05 07:04:20 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR120420WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Dec 05 05:22:35 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	51279	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	51419	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	25242	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	12300	4.67	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.40%
7) Chloroethane-d5	1.92	69	11428	4.94	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.80%
11) 1,1-Dichloroethene-d2	2.58	63	21788	3.42	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.40%
20) 2-Butanone-d5	4.66	46	50202	50.83	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.66%
24) Chloroform-d	5.08	84	35669	4.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.00%
26) 1,2-Dichloroethane-d4	5.72	65	25718	5.26	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.20%
32) Benzene-d6	5.74	84	54520	4.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.20%
36) 1,2-Dichloropropane-d6	6.70	67	15416	4.60	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.00%
41) Toluene-d8	7.91	98	49233	4.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.80%
43) trans-1,3-Dichloropropene-	8.19	79	9460	4.76	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.20%
46) 2-Hexanone-d5	8.64	63	38847	47.04	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.08%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	16764	4.54	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.80%
64) 1,2-Dichlorobenzene-d4	12.19	152	22725	5.26	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.20%


Target Compounds					Ovalue
16) Methylene chloride	3.06	84	5832	1.456 ug/L	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU120420\
Data File : VU041477.D
Acq On : 04 Dec 2020 17:49
Operator : SY/MD
Sample : VIBLK08
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK08

Quant Time: Dec 05 07:04:20 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR120420WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Dec 05 05:22:35 2020
Response via : Initial Calibration

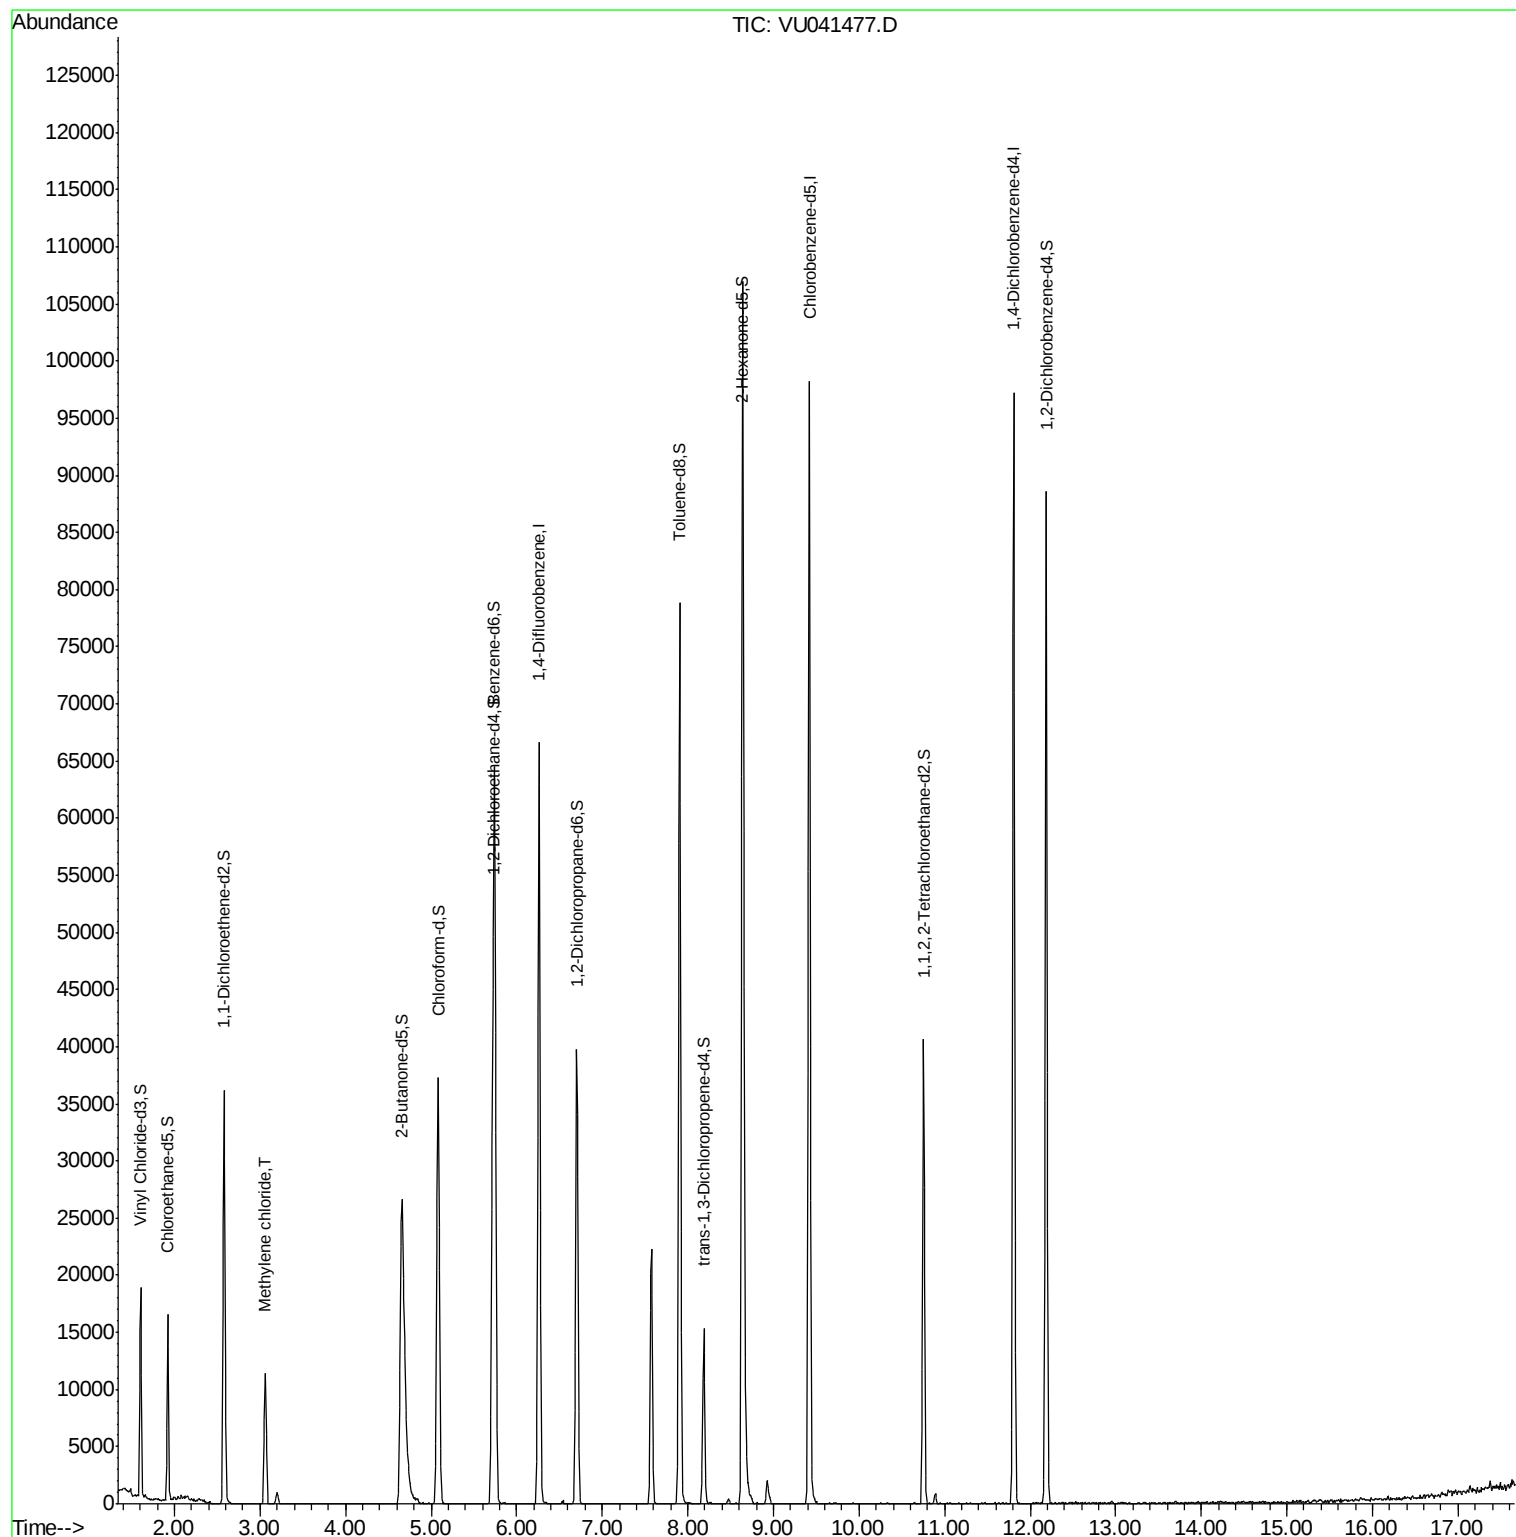

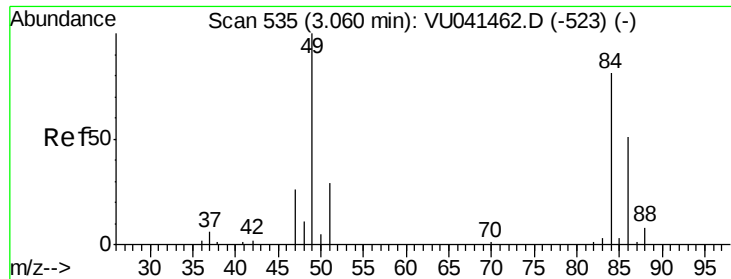

#16
 Methvlene chloride
 Concen: 1.456 ug/L
 RT: 3.06 min Scan# 536
 Delta R.T. 0.00 min
 Lab File: VU041477.D
 Acq: 04 Dec 2020 17:49

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK08

Tot Ion: 84 Resp: 5832
 Ion Ratio Lower Upper
 84 100
 86 57.2 44.1 81.9
 49 100.1 86.1 159.9

