


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU120420\
 Data File : VU041459.D
 Acq On : 04 Dec 2020 09:10
 Operator : SY/MD
 Sample : BFB19
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB19

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR120420WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat Dec 05 05:22:35 2020

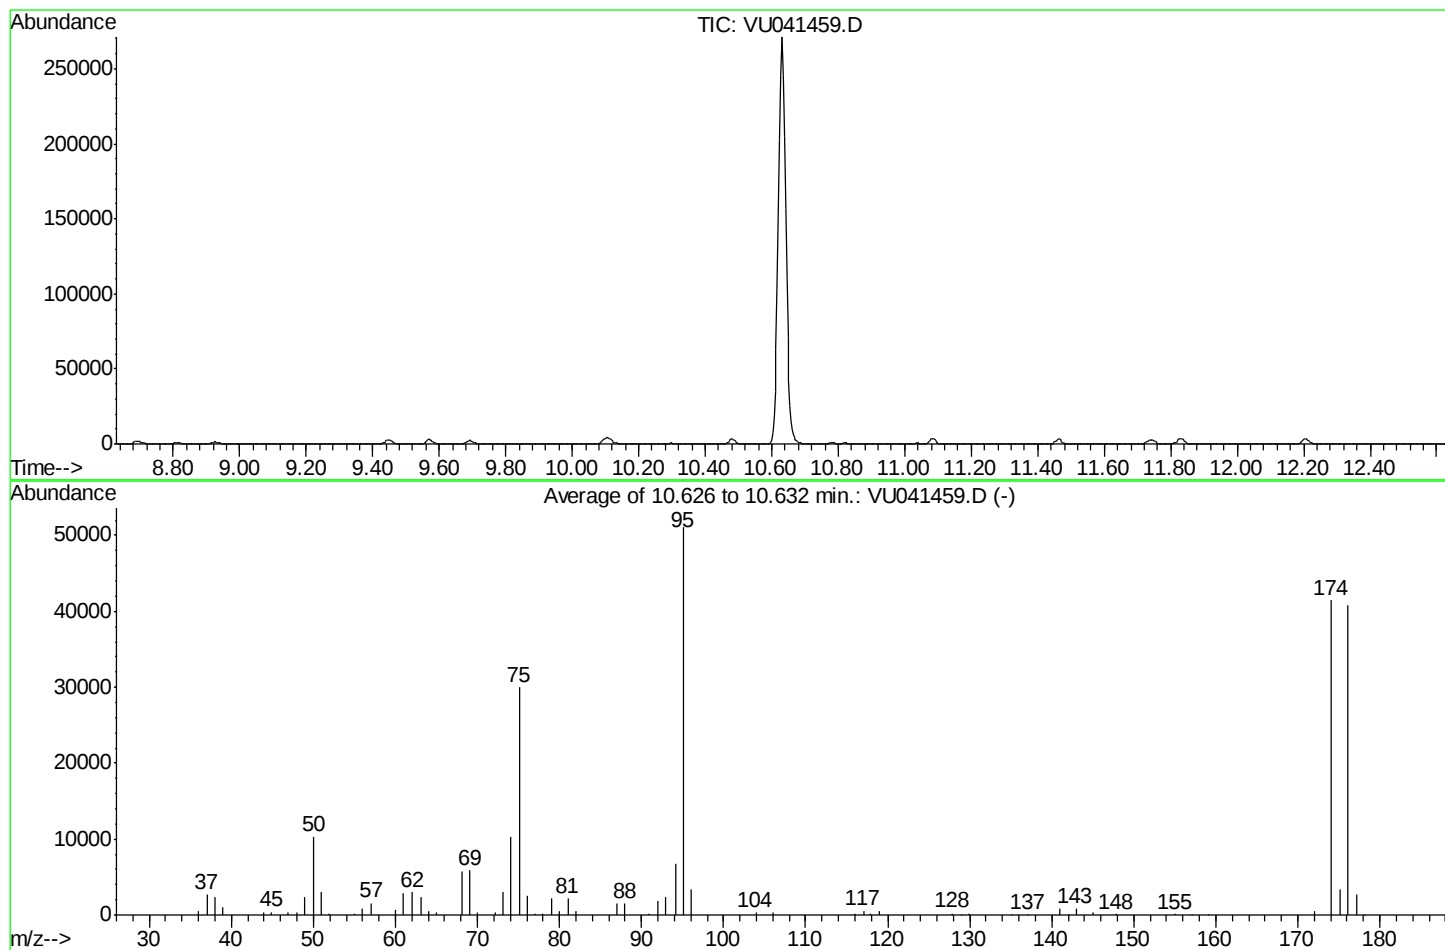

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	10340	PASS
75	95	30	80	58.7	30000	PASS
95	95	100	100	100.0	51064	PASS
96	95	5	9	6.6	3391	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	81.2	41461	PASS
175	174	5	9	8.0	3311	PASS
176	174	95	101	98.4	40792	PASS
177	176	5	9	6.7	2714	PASS

m/z	Abundance
36.00	477.0
37.00	2471.0
38.10	2332.0
39.00	980.0
44.00	297.0
45.00	442.0
46.90	407.0
48.00	311.0
49.00	2221.0
50.10	9810.0
51.00	2962.0
51.90	110.0
55.00	137.0
56.00	676.0
57.10	1422.0
60.00	648.0
61.00	2698.0
62.10	2865.0
63.10	2227.0
64.00	409.0
65.00	368.0
68.00	5328.0
69.10	5532.0
70.00	401.0
72.10	340.0
73.10	2872.0
74.10	9751.0
75.10	28096.0
76.10	2523.0
77.00	237.0
78.00	199.0
79.00	2025.0
80.00	522.0
81.00	1934.0
82.00	418.0
87.00	1515.0
88.00	1384.0
91.00	239.0
92.00	1690.0
93.00	2218.0
94.10	6291.0
95.10	48376.0
96.10	3299.0
104.00	247.0
106.00	239.0
116.00	229.0
117.00	485.0
118.00	254.0
119.00	417.0
128.00	208.0
130.00	167.0
141.00	758.0
142.10	134.0
143.00	782.0
145.00	235.0
147.90	136.0
155.00	181.0
159.00	116.0
172.00	426.0
174.10	38736.0
175.10	3019.0
176.10	38032.0
177.10	2560.0

Instrument :
MSVOA_U
ClientSampleId :
BFB19

m/z	Abundance
36.00	540.0
37.00	2678.0
38.00	2436.0
39.00	1137.0
44.00	310.0
45.00	417.0
46.90	361.0
48.00	364.0
49.00	2514.0
50.00	10734.0
51.00	3166.0
51.90	165.0
55.00	125.0
56.00	796.0
57.00	1566.0
60.00	679.0
61.00	3040.0
62.10	3140.0
63.10	2451.0
64.00	462.0
65.00	389.0
68.00	5864.0
69.10	6037.0
70.10	436.0
72.10	399.0
73.10	3103.0
74.10	10613.0
75.10	30936.0
76.10	2696.0
77.10	226.0
78.00	263.0
79.00	2187.0
80.00	559.0
81.00	2216.0
82.00	441.0
87.00	1498.0
88.00	1522.0
91.00	224.0
92.00	1873.0
93.00	2461.0
94.10	7012.0
95.10	52800.0
96.10	3468.0
104.00	334.0
106.00	278.0
115.90	222.0
117.10	603.0
118.00	251.0
119.00	500.0
128.00	212.0
129.90	210.0
137.10	111.0
141.00	852.0
142.10	106.0
143.00	881.0
145.00	298.0
147.90	139.0
155.10	174.0
157.00	113.0
159.00	120.0
172.00	459.0
174.10	42784.0
175.10	3427.0
176.10	42024.0
177.10	2788.0

Instrument :
MSVOA_U
ClientSampleId :
BFB19

m/z	Abundance
36.00	554.0
37.00	2727.0
38.00	2312.0
39.00	1157.0
44.00	314.0
44.90	371.0
46.90	308.0
48.00	396.0
49.00	2572.0
50.10	10476.0
51.00	3088.0
52.00	170.0
55.00	101.0
56.00	843.0
57.00	1591.0
60.10	670.0
61.00	3121.0
62.10	3077.0
63.10	2512.0
64.00	440.0
65.00	397.0
68.10	5924.0
69.10	6105.0
70.10	438.0
72.10	401.0
73.00	2926.0
74.10	10622.0
75.10	30968.0
76.10	2482.0
76.90	209.0
78.00	265.0
79.00	2169.0
80.00	583.0
81.00	2236.0
81.90	473.0
87.00	1357.0
88.00	1483.0
90.90	194.0
92.00	1809.0
93.00	2597.0
94.10	6977.0
95.10	52016.0
96.10	3407.0
104.00	359.0
106.00	345.0
115.90	203.0
117.00	634.0
117.90	227.0
119.00	494.0
127.90	218.0
129.00	104.0
129.90	231.0
135.00	103.0
137.10	116.0
141.00	859.0
143.00	848.0
145.00	312.0
155.00	141.0
157.10	110.0
172.00	433.0
174.10	42864.0
175.10	3487.0
176.10	42320.0
177.10	2796.0
178.10	109.0

Instrument :
MSVOA_U
ClientSampleId :
BFB19

m/z Abundance

Instrument :
MSVOA_U
ClientSampleId :
BFB19