
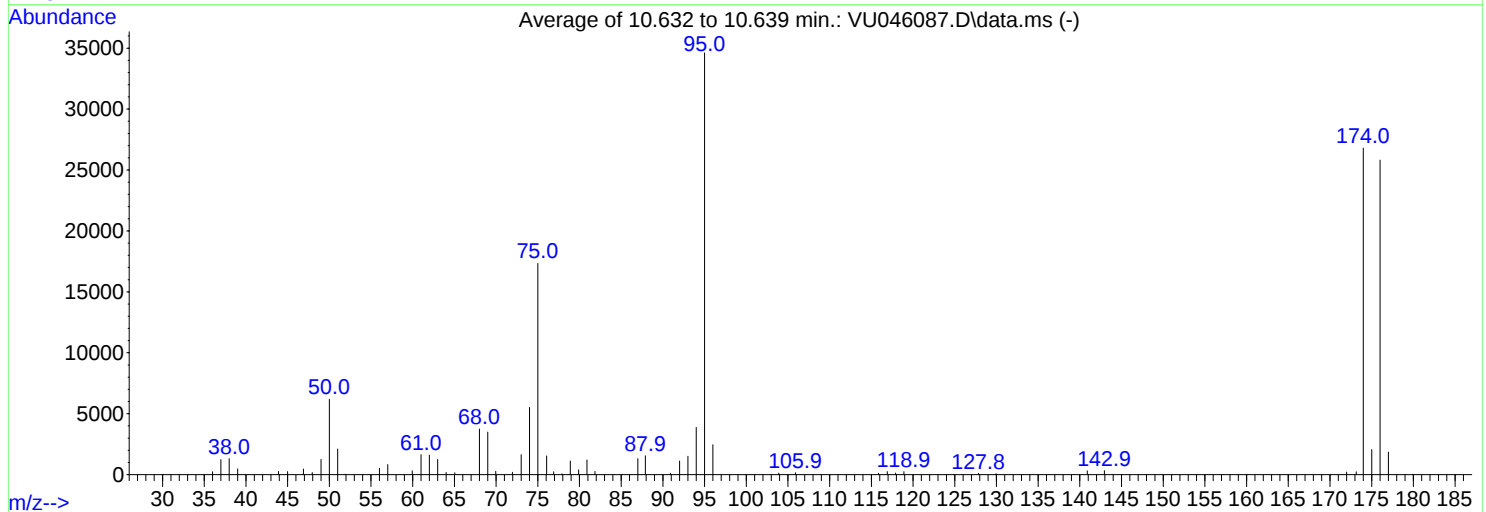


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120421\
 Data File : VU046087.D
 Acq On : 04 Dec 2021 12:24
 Operator : SY/MD
 Sample : BFB023
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB023

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis
 Last Update : Fri Dec 03 05:08:36 2021

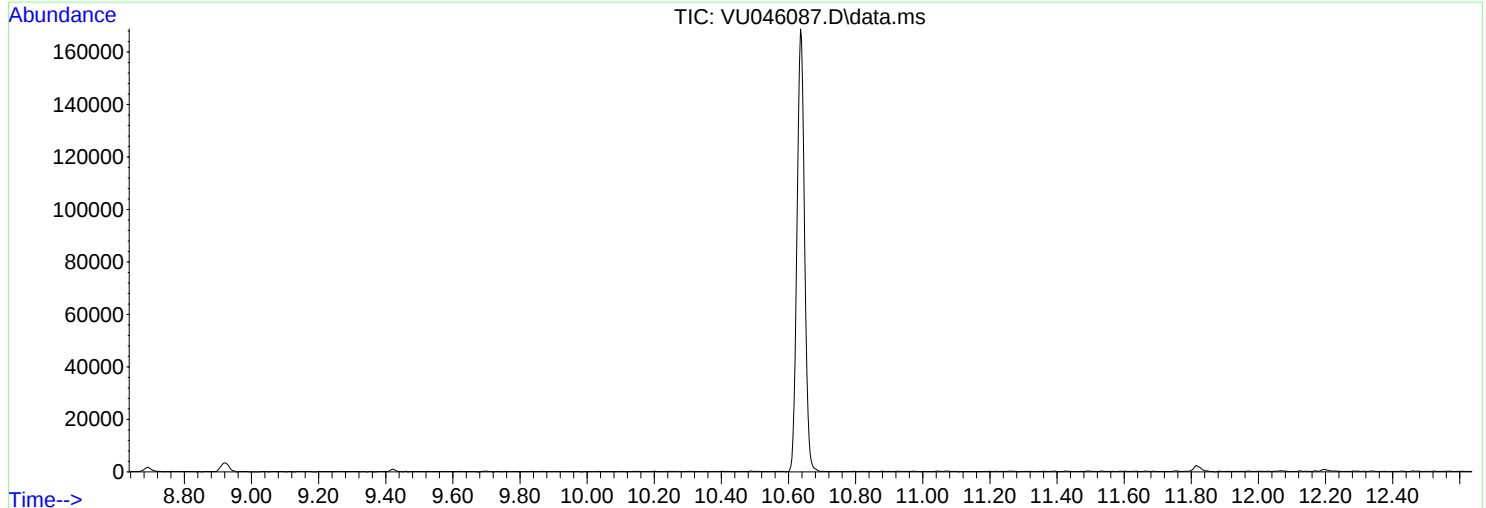

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	6181	PASS
75	95	30	80	50.1	17339	PASS
95	95	100	100	100.0	34616	PASS
96	95	5	9	7.1	2461	PASS
173	174	0.00	2	0.9	237	PASS
174	95	50	120	77.4	26795	PASS
175	174	5	9	7.7	2063	PASS
176	174	95	101	96.3	25816	PASS
177	176	5	9	7.2	1847	PASS

m/z	Abundance
43.90	113.0

Instrument :
MSVOA_U
ClientSampleId :
BFB023

m/z	Abundance
36.00	234.0
37.00	1276.0
38.00	1341.0
39.00	523.0
43.90	332.0
45.00	241.0
46.90	468.0
48.00	188.0
49.00	1209.0
50.00	5948.0
51.00	1947.0
56.00	501.0
57.00	760.0
59.90	295.0
61.00	1540.0
62.00	1565.0
63.00	1135.0
64.00	194.0
65.10	148.0
68.00	3603.0
69.00	3422.0
70.00	246.0
71.90	219.0
73.00	1598.0
74.00	5448.0
75.00	16584.0
76.10	1512.0
76.90	192.0
78.90	1069.0
79.90	394.0
80.90	1154.0
81.90	237.0
87.00	1215.0
87.90	1464.0
90.90	137.0
92.00	1095.0
93.00	1443.0
94.00	3809.0
95.00	33248.0
96.00	2472.0
103.90	119.0
105.90	169.0
115.90	107.0
116.90	263.0
117.90	132.0
118.90	238.0
127.80	106.0
140.90	315.0
142.90	304.0
172.00	224.0
173.10	234.0
174.00	24840.0
175.00	1872.0
176.00	24056.0
177.00	1808.0

Instrument :
MSVOA_U
ClientSampleId :
BFB023

m/z	Abundance
36.00	251.0
37.00	1282.0
38.00	1382.0
39.00	482.0
43.90	400.0
45.00	249.0
46.90	490.0
47.90	185.0
49.00	1294.0
50.00	6401.0
51.00	2204.0
56.00	521.0
57.00	868.0
59.90	341.0
61.00	1710.0
62.00	1684.0
63.00	1295.0
64.00	194.0
65.10	155.0
68.00	3864.0
69.00	3624.0
70.00	285.0
71.90	195.0
73.00	1700.0
74.00	5692.0
75.00	17888.0
76.00	1593.0
76.90	265.0
77.90	112.0
78.90	1145.0
79.90	411.0
80.90	1278.0
81.80	273.0
87.00	1340.0
87.90	1590.0
90.90	122.0
92.00	1176.0
93.00	1587.0
94.00	3984.0
95.00	35928.0
96.00	2543.0
103.90	137.0
105.90	163.0
115.90	111.0
116.90	248.0
117.90	135.0
118.90	258.0
127.90	103.0
129.90	101.0
140.90	318.0
142.90	323.0
172.00	222.0
173.10	238.0
174.00	27688.0
175.00	2138.0
176.00	26640.0
177.00	1952.0

Instrument :
MSVOA_U
ClientSampleId :
BFB023

m/z	Abundance
36.00	230.0
37.00	1145.0
38.00	1239.0
39.00	432.0
43.90	410.0
45.00	245.0
46.90	418.0
47.90	150.0
49.00	1252.0
50.00	6195.0
51.00	2152.0
51.90	106.0
56.00	502.0
57.00	855.0
60.00	323.0
61.00	1690.0
62.00	1547.0
63.00	1323.0
64.00	173.0
65.00	159.0
68.00	3777.0
69.00	3431.0
69.90	278.0
72.00	168.0
73.00	1624.0
74.00	5402.0
75.00	17544.0
76.00	1521.0
76.90	273.0
77.90	102.0
78.90	1152.0
79.90	395.0
80.90	1210.0
81.80	298.0
87.00	1376.0
87.90	1580.0
90.90	109.0
92.00	1074.0
93.00	1522.0
94.00	3837.0
95.00	34672.0
96.00	2367.0
103.90	137.0
105.90	156.0
115.80	123.0
116.90	230.0
117.90	120.0
118.90	261.0
127.90	107.0
130.00	122.0
140.90	335.0
143.00	366.0
172.00	186.0
173.20	239.0
174.00	27856.0
175.00	2180.0
176.00	26752.0
177.00	1782.0

Instrument :
MSVOA_U
ClientSampleId :
BFB023