


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU120518\
Data File : VU028467.D
Acq On : 05 Dec 2018 08:52
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\82U112818W.M
Title : SW846 8260
Last Update : Thu Nov 29 01:04:49 2018

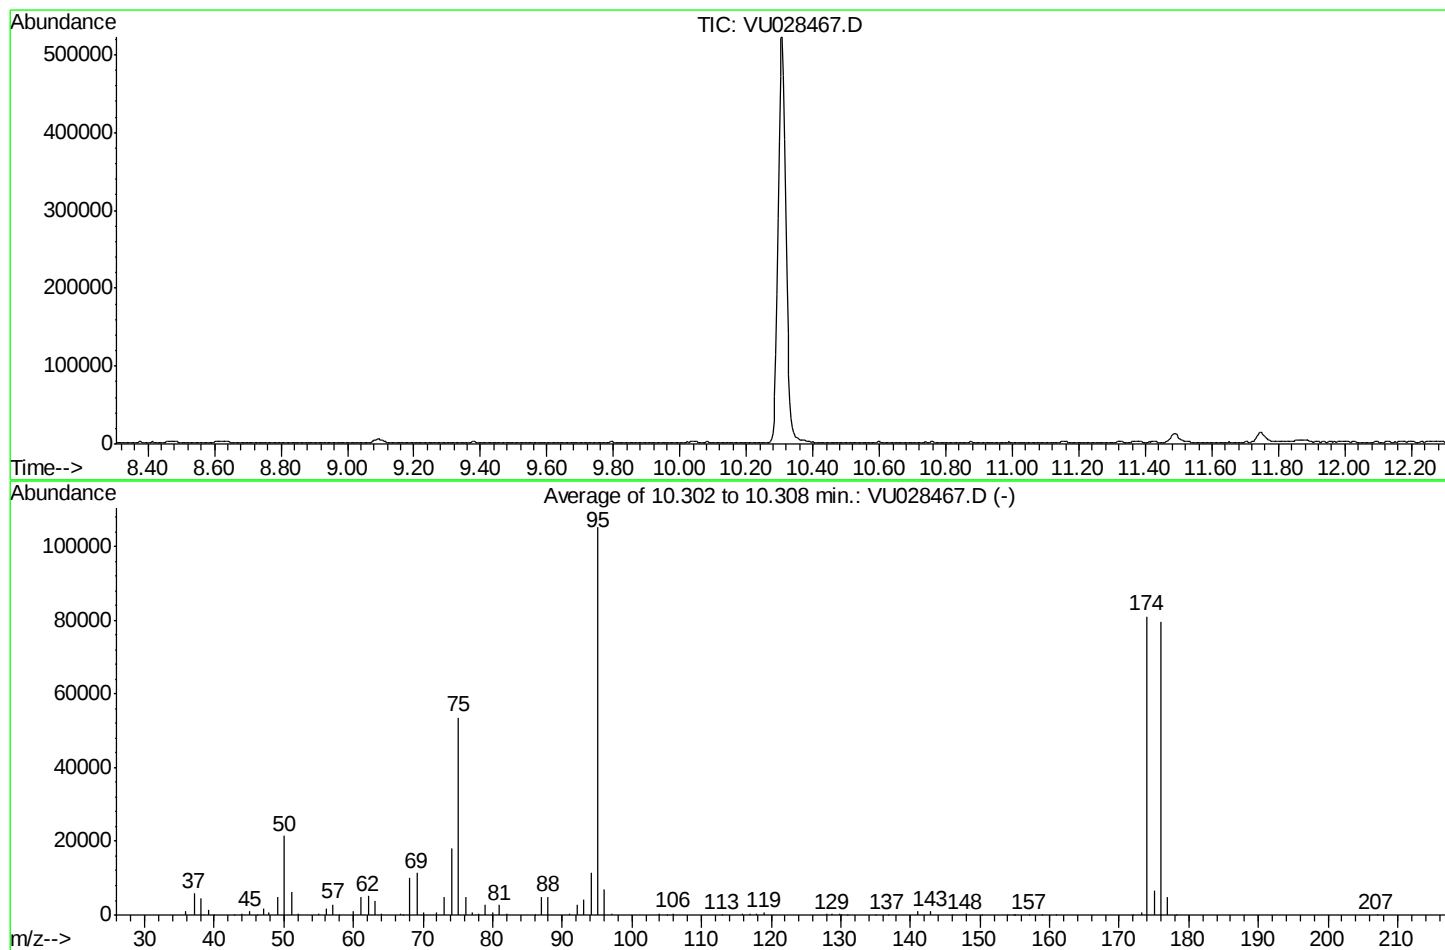

AutoFind: Scans 2839, 2840, 2841; Background Corrected with Scan 2826

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	21416	PASS
75	95	30	60	51.0	53618	PASS
95	95	100	100	100.0	105221	PASS
96	95	5	9	6.5	6825	PASS
173	174	0.00	2	1.0	843	PASS
174	95	50	100	77.1	81080	PASS
175	174	5	9	8.4	6787	PASS
176	174	95	101	98.1	79528	PASS
177	176	5	9	6.2	4917	PASS