

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU120519\
 Data File : VU036003.D
 Acq On : 05 Dec 2019 19:09
 Operator : JC/SP
 Sample : K6132-06
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFQR2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR120319WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.372	3	10	23	rVB2	82292	84753	7.86%	0.943%
2	1.504	46	51	57	rBV	19760	18697	1.73%	0.208%
3	1.613	76	85	92	rBV2	218649	254336	23.57%	2.831%
4	1.932	177	184	198	rVB	149926	190103	17.62%	2.116%
5	2.594	378	390	405	rBV	232801	385898	35.77%	4.295%
6	2.687	411	419	435	rVB3	5393	12924	1.20%	0.144%
7	4.703	1029	1046	1067	rBV	126509	400806	37.15%	4.461%
8	5.112	1157	1173	1192	rBV	212296	473147	43.85%	5.266%
9	5.771	1357	1378	1409	rBV2	424813	1074474	99.59%	11.959%
10	6.292	1526	1540	1558	rBV	335158	654032	60.62%	7.279%
11	6.732	1663	1677	1693	rBV2	254840	507793	47.07%	5.652%
12	7.292	1842	1851	1865	rVB7	7407	14504	1.34%	0.161%
13	7.414	1877	1889	1900	rBV4	21381	42769	3.96%	0.476%
14	7.603	1935	1948	1971	rBV	113627	219241	20.32%	2.440%
15	7.864	2016	2029	2038	rBV5	6885	14825	1.37%	0.165%
16	7.931	2038	2050	2067	rBV	437895	786698	72.92%	8.756%
17	8.214	2125	2138	2153	rBV	71090	136019	12.61%	1.514%
18	8.584	2245	2253	2261	rVB5	8481	12798	1.19%	0.142%
19	8.681	2267	2283	2321	rBV	459197	1078918	100.00%	12.009%
20	8.825	2322	2328	2340	rVB8	10052	19536	1.81%	0.217%
21	9.449	2507	2522	2543	rBV	493611	880237	81.59%	9.797%
22	9.722	2596	2607	2617	rVB	5571	10971	1.02%	0.122%
23	10.783	2925	2937	2955	rBV	210531	357498	33.13%	3.979%
24	11.838	3252	3265	3284	rBV	381894	642819	59.58%	7.155%
25	12.217	3369	3383	3399	rBV	398338	675339	62.59%	7.517%
26	13.262	3698	3708	3718	rBV7	20974	35456	3.29%	0.395%


Sum of corrected areas: 8984591

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU120519\
Data File : VU036003.D
Acq On : 05 Dec 2019 19:09
Operator : JC/SP
Sample : K6132-06
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFQR2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR120319WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

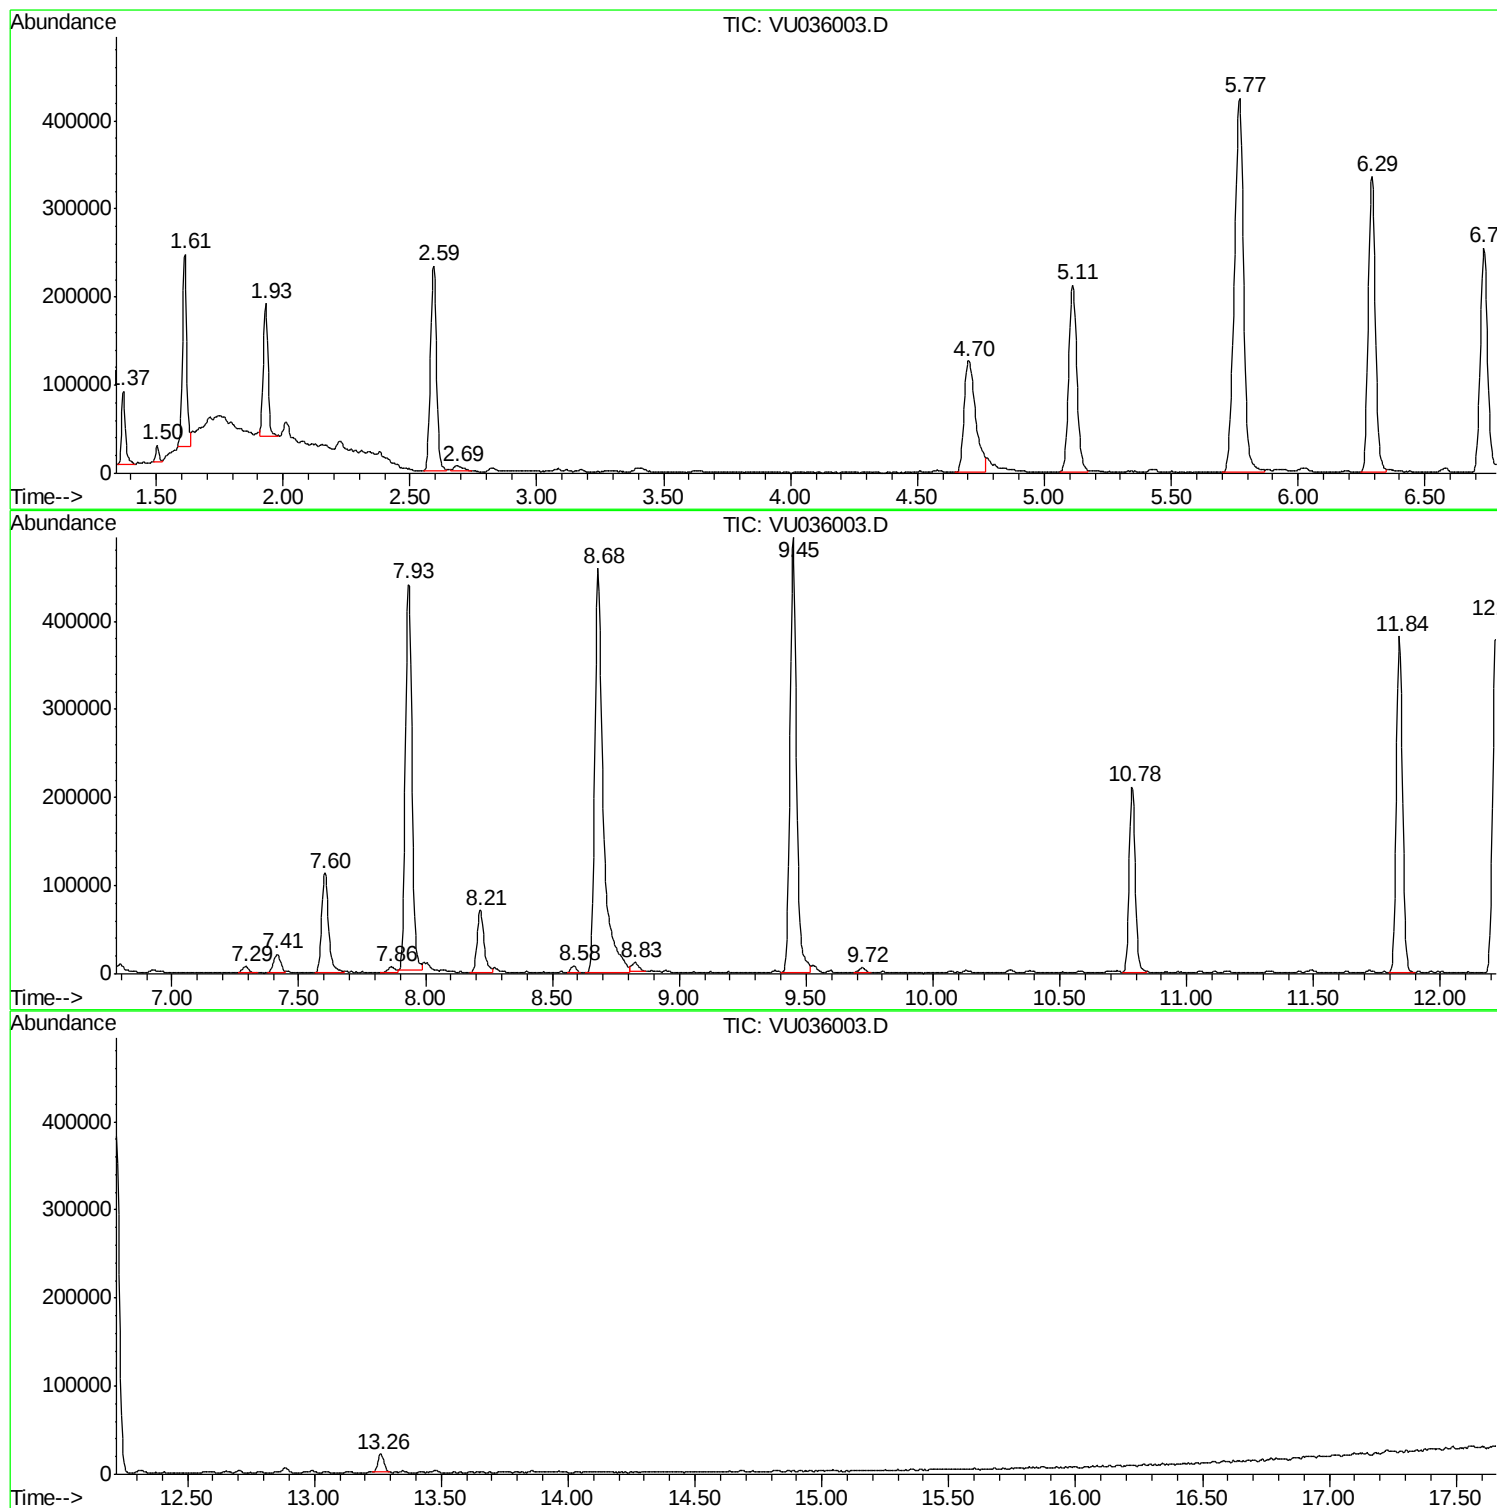

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU120519\
Data File : VU036003.D
Acq On : 05 Dec 2019 19:09
Operator : JC/SP
Sample : K6132-06
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFQR2










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR120319WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.37	0.65 ug/L	84753	1,4-Difluorobenzene	6.29

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propane	44	C3H8	000074-98-6	83
2			Propane	44	C3H8	000074-98-6	83
3			2-Butenal, (E)-	70	C4H6O	000123-73-9	64
4			Bis(3-methylbutyl) fluorene-2,7-...	466	C23H30O6S2	253664-95-8	64
5			Cyclopropanecarboxylic acid	86	C4H6O2	001759-53-1	53

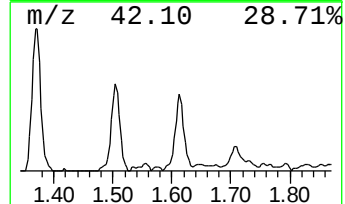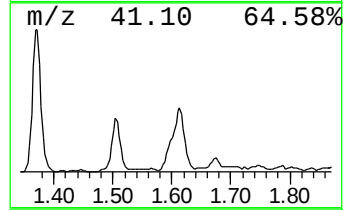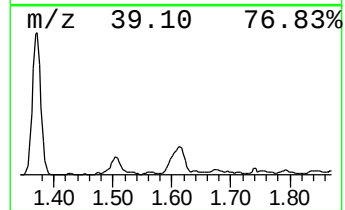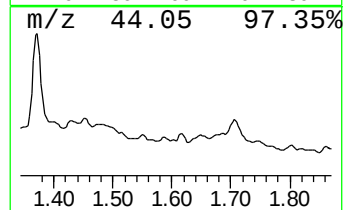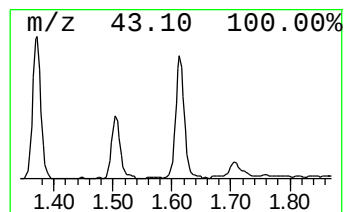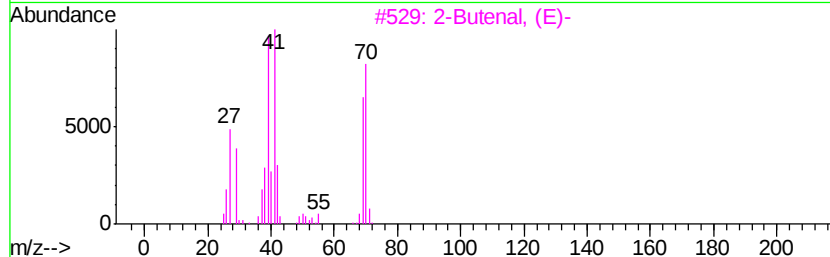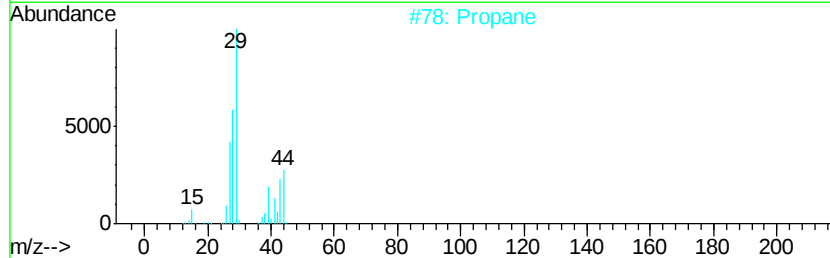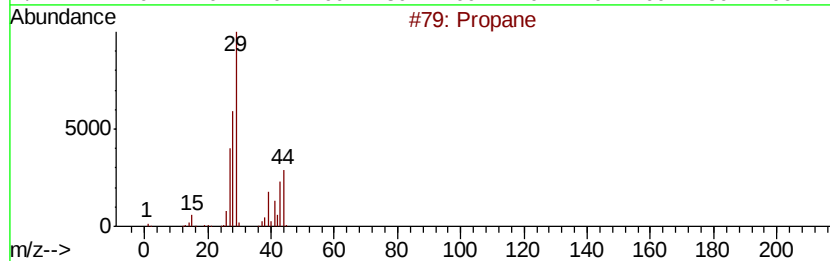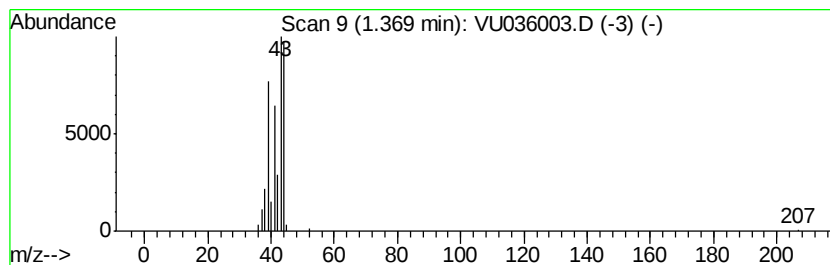

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU120519\
Data File : VU036003.D
Acq On : 05 Dec 2019 19:09
Operator : JC/SP
Sample : K6132-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFQR2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR120319WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: Str...	1.37	0.7	ug/L	84753	1	6.29	654032	5.0