


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU120519\
Data File : VU035986.D
Acq On : 05 Dec 2019 10:46
Operator : JC/SP
Sample : BFB12
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB12

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR120319WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Dec 06 22:30:31 2019

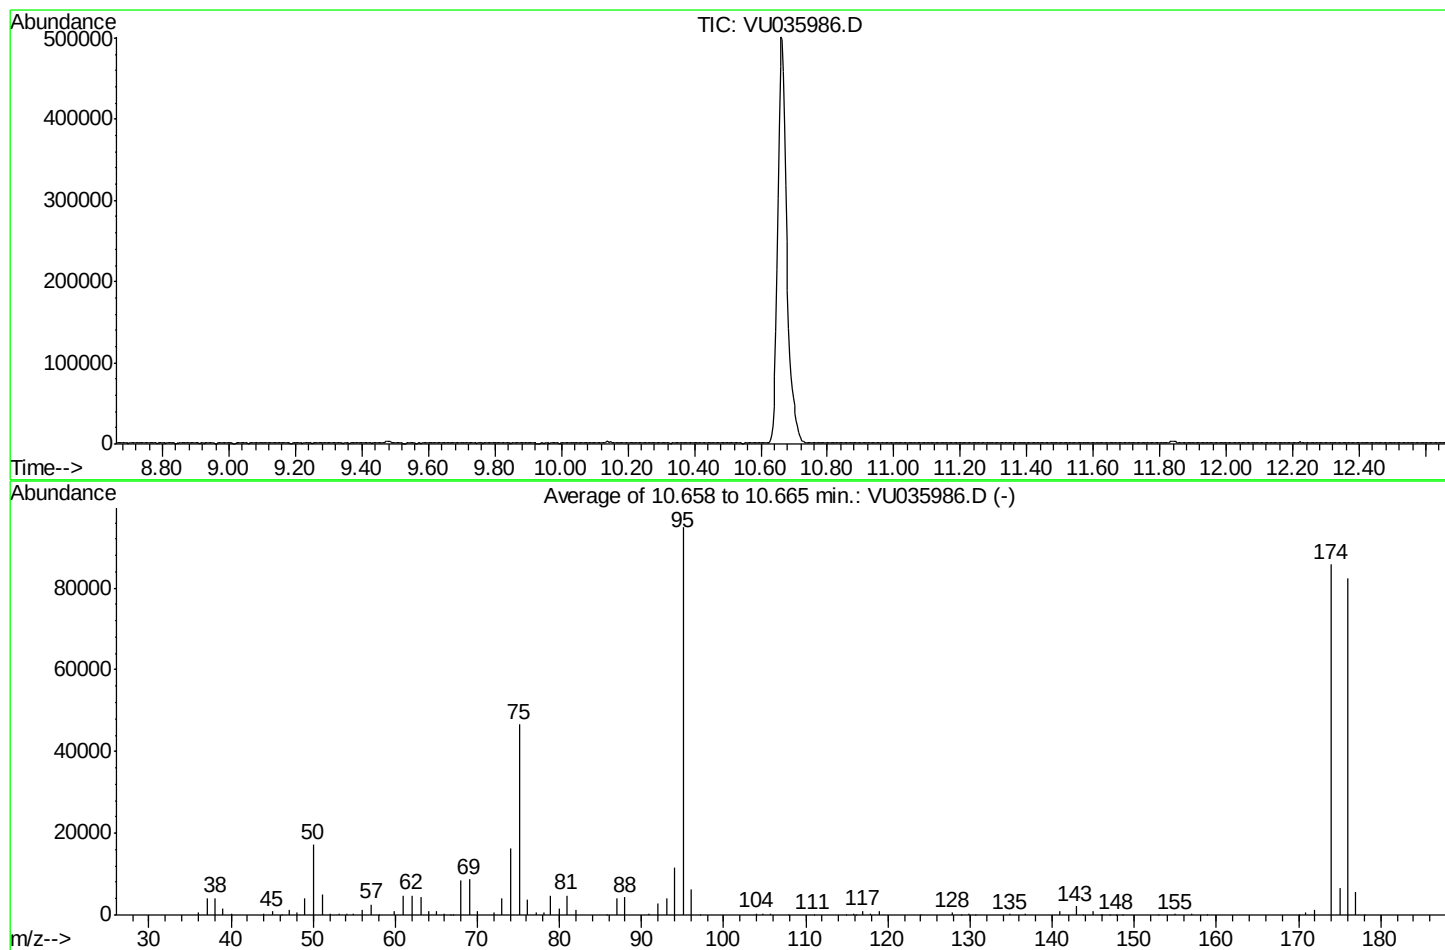

AutoFind: Scans 2898, 2899, 2900; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	17218	PASS
75	95	30	80	49.1	46546	PASS
95	95	100	100	100.0	94856	PASS
96	95	5	9	6.6	6289	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	90.4	85712	PASS
175	174	5	9	7.8	6711	PASS
176	174	95	101	96.0	82264	PASS
177	176	5	9	6.8	5624	PASS

m/z	Abundance
36.10	769.0
37.00	4235.0
38.10	4307.0
39.00	1517.0
40.00	374.0
44.00	1367.0
45.10	666.0
46.20	121.0
47.10	1327.0
48.00	483.0
49.00	3927.0
50.00	16944.0
51.10	4905.0
52.10	360.0
53.10	206.0
54.00	293.0
54.90	242.0
56.10	1172.0
57.10	2416.0
58.00	130.0
59.90	967.0
61.00	4625.0
62.00	4902.0
63.10	4250.0
64.20	1043.0
65.00	891.0
65.90	246.0
67.10	295.0
68.00	8241.0
69.10	8333.0
70.00	726.0
72.10	647.0
73.00	4561.0
74.10	15484.0
75.10	44784.0
76.10	3482.0
77.00	719.0
78.00	488.0
79.00	4106.0
79.90	1358.0
80.90	4759.0
82.00	1207.0
87.00	3943.0
88.00	4046.0
91.00	316.0
92.00	2758.0
93.00	3806.0
94.10	10919.0
95.10	90888.0
96.10	6133.0
97.00	119.0
104.00	499.0
104.80	262.0
105.70	484.0
110.90	114.0
114.90	174.0
115.90	359.0
116.90	917.0
117.80	412.0
118.90	808.0
123.90	111.0
127.90	455.0
128.90	156.0
129.80	364.0
130.70	104.0
134.90	172.0
136.80	241.0
140.90	953.0
142.90	1986.0
143.80	112.0
144.90	1086.0
145.90	194.0
147.00	103.0
147.80	129.0
155.00	115.0
156.90	237.0
170.00	100.0
170.90	608.0
172.00	1059.0
174.00	79848.0
175.00	6446.0
176.00	76872.0
177.00	5451.0
177.90	138.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12

m/z	Abundance
36.10	849.0
37.10	4196.0
38.10	4376.0
39.00	1494.0
40.10	386.0
44.00	1358.0
45.00	850.0
47.10	1241.0
48.10	527.0
49.00	4150.0
50.10	17960.0
51.10	5155.0
52.10	359.0
53.10	228.0
54.10	224.0
54.90	336.0
56.00	1362.0
57.10	2730.0
58.00	147.0
59.90	1014.0
61.00	4915.0
62.00	4963.0
63.10	4415.0
64.10	1135.0
65.10	936.0
65.90	198.0
66.80	241.0
68.00	8577.0
69.10	8714.0
70.00	915.0
72.00	644.0
73.00	4407.0
74.10	16608.0
75.10	47488.0
76.10	3698.0
77.10	744.0
78.10	592.0
78.90	4702.0
79.90	1533.0
80.90	4865.0
82.00	1281.0
85.80	106.0
87.00	4322.0
88.00	4506.0
90.80	438.0
92.10	2831.0
93.00	4093.0
94.10	11704.0
95.00	97416.0
96.10	6406.0
97.10	147.0
104.00	444.0
104.80	202.0
105.70	426.0
110.90	147.0
114.90	137.0
115.90	379.0
116.90	1034.0
117.90	457.0
119.00	911.0
124.00	118.0
127.80	515.0
128.90	152.0
129.80	410.0
130.70	142.0
134.90	255.0
136.80	230.0
141.00	1135.0
142.90	2225.0
144.90	1063.0
146.10	186.0
147.80	158.0
153.00	112.0
155.00	212.0
156.90	177.0
158.90	112.0
170.00	117.0
170.90	606.0
172.00	1121.0
174.00	88264.0
175.00	6842.0
176.00	84616.0
177.00	5871.0
178.00	146.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12

m/z	Abundance
36.00	762.0
37.10	3788.0
38.10	3915.0
39.10	1322.0
40.00	383.0
44.00	1222.0
45.00	935.0
47.10	1111.0
48.10	548.0
49.00	4013.0
50.10	16752.0
51.10	5000.0
52.20	376.0
53.10	224.0
54.20	143.0
54.90	290.0
56.00	1366.0
57.10	2775.0
58.00	127.0
59.90	992.0
61.00	4587.0
62.00	4681.0
63.10	4414.0
64.10	1005.0
65.10	930.0
66.00	160.0
66.80	193.0
68.00	8519.0
69.00	9072.0
70.00	981.0
72.00	616.0
73.00	4059.0
74.10	16440.0
75.10	47368.0
76.10	3711.0
77.20	715.0
78.00	659.0
78.90	5041.0
79.90	1581.0
80.90	4589.0
81.90	1329.0
87.00	4448.0
87.90	4357.0
90.80	536.0
92.10	2680.0
93.00	4081.0
94.00	11911.0
95.00	96264.0
96.10	6329.0
97.10	123.0
104.00	373.0
104.70	120.0
105.80	372.0
107.90	109.0
111.00	188.0
116.10	334.0
117.00	1015.0
117.90	482.0
119.00	946.0
124.10	105.0
127.80	498.0
128.90	133.0
129.80	392.0
130.70	121.0
134.90	290.0
136.70	230.0
141.00	1200.0
142.90	2302.0
144.90	1062.0
146.10	217.0
147.80	177.0
148.60	102.0
152.90	141.0
155.00	335.0
156.80	135.0
158.90	138.0
170.90	566.0
172.00	1313.0
174.00	89024.0
175.00	6846.0
176.00	85304.0
177.00	5550.0
178.10	139.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12

Scan 2884 (10.613 min): VU035986.D
BFB12

m/z	Abundance
39.80	297.0
44.00	957.0
72.90	143.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12