

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120522\
 Data File : VU052177.D
 Acq On : 05 Dec 2022 11:21
 Operator : JC/MD
 Sample : VU1205WBL06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Dec 05 22:33:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Dec 02 00:27:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.206	114	16280	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.349	117	14476	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.745	152	6199	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.598	65	10640	0.555	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery = 110.000%			
4) 1,2-Dichloroethane-d4	5.661	65	8297	0.457	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 92.000%			
7) 1,2-Dichloropropane-d6	6.639	67	9671	0.556	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery = 112.000%			
8) Toluene-d8	7.833	98	13992	0.534	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 106.000%			
10) 1,1,2,2-Tetrachloroeth...	10.682	84	9208	0.495	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery = 98.000%			
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.927	75	29	0.014	ug/L	Qvalue # 82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120522\
Data File : VU052177.D
Acq On : 05 Dec 2022 11:21
Operator : JC/MD
Sample : VU1205WBL06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Dec 05 22:33:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM120122.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 02 00:27:38 2022
Response via : Initial Calibration

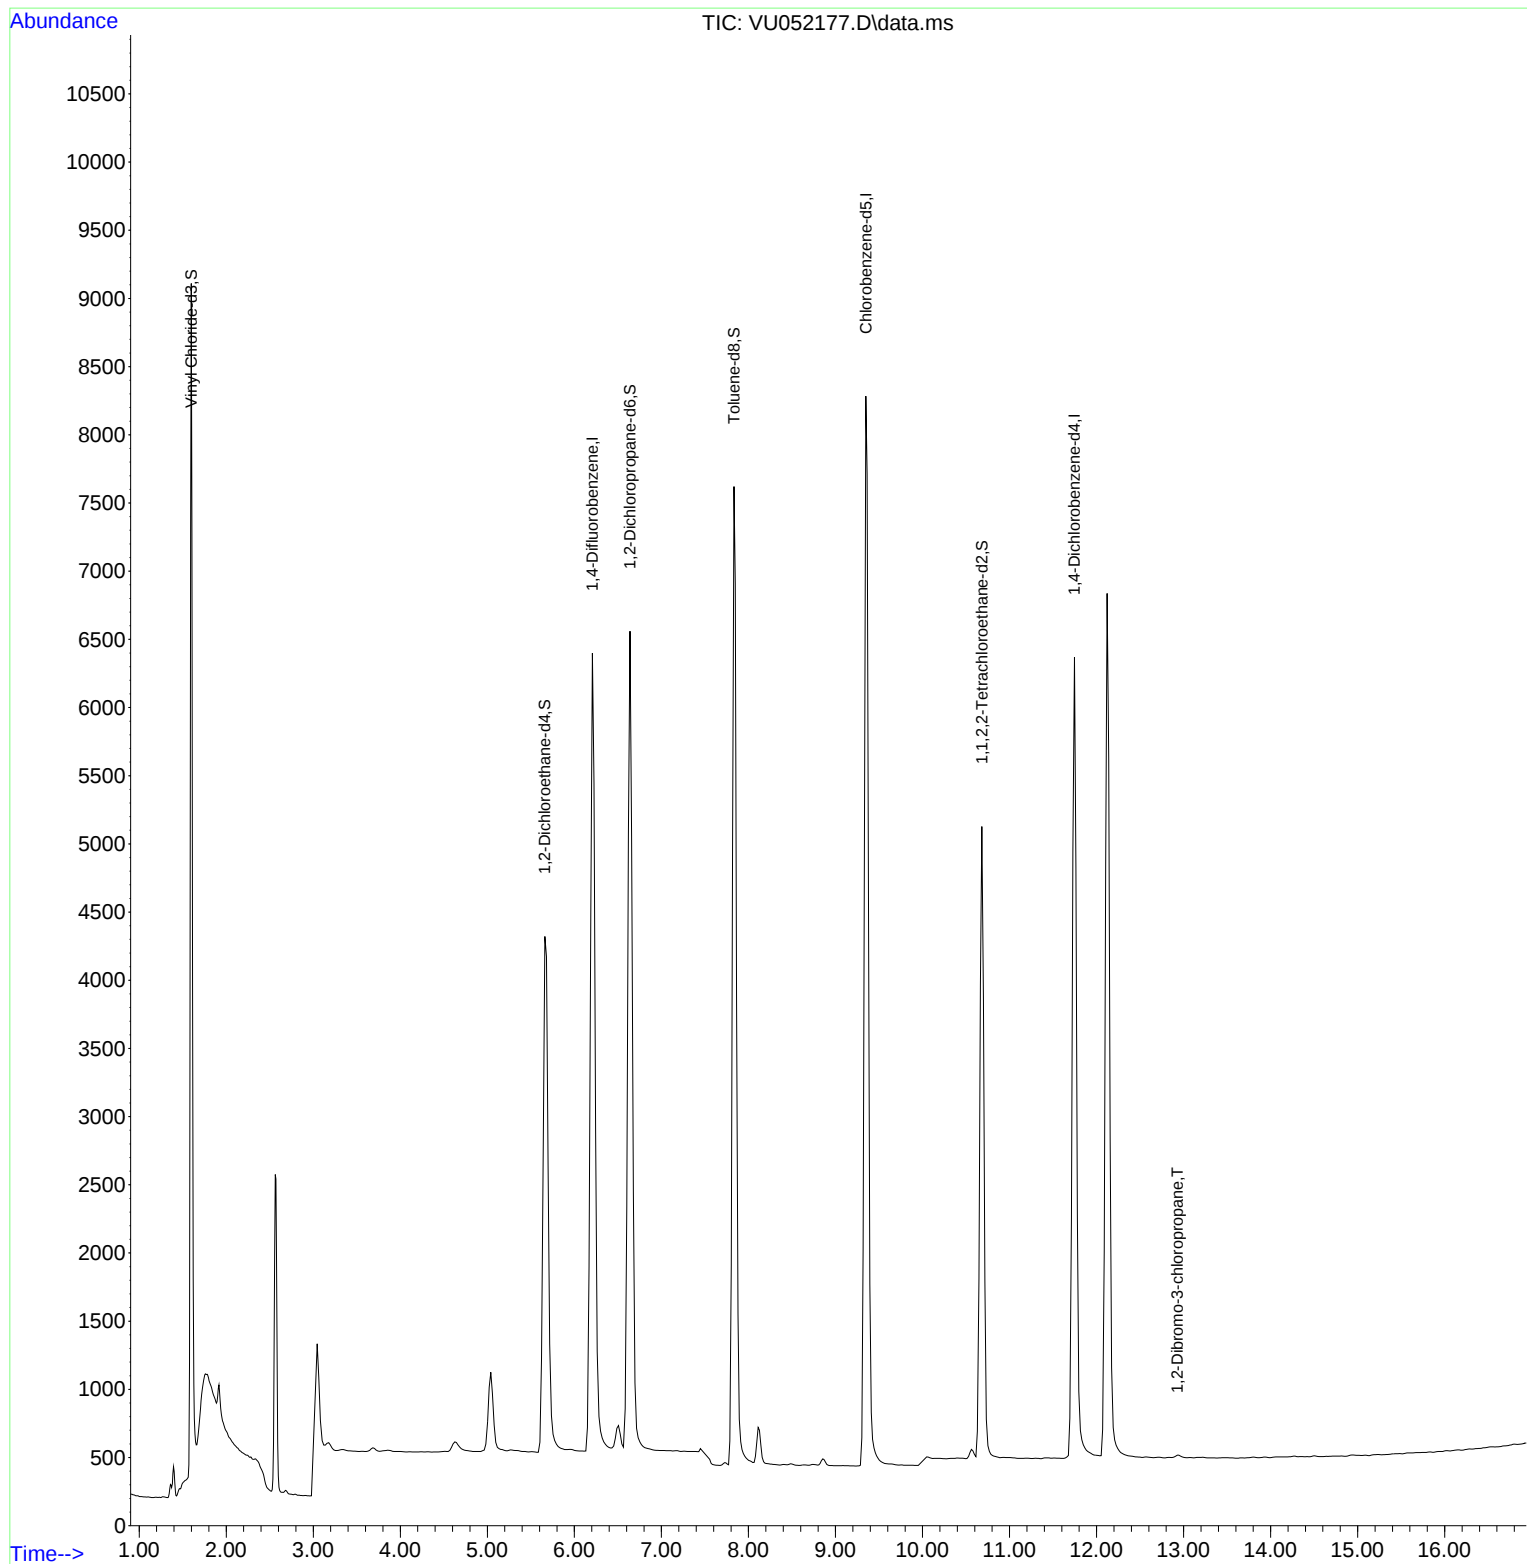

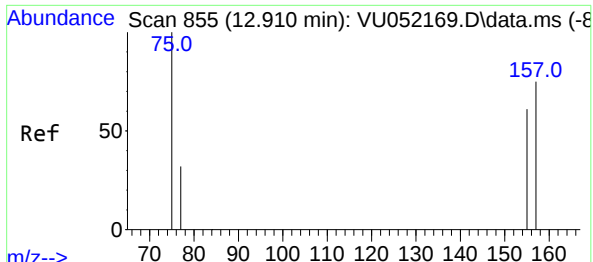

#13
1,2-Dibromo-3-chloropropane
Concen: 0.014 ug/L
RT: 12.927 min Scan# 856
Delta R.T. 0.017 min
Lab File: VU052177.D
Acq: 05 Dec 2022 11:21

Instrument :
MSVOA_U
ClientSampleId :

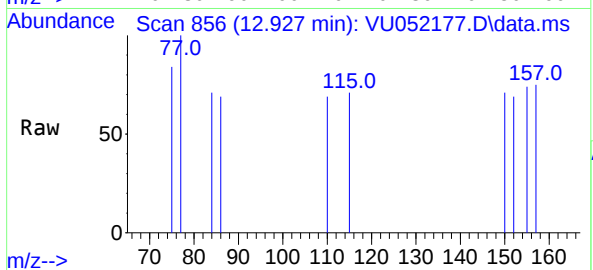

Tgt Ion: 75 Resp: 29
Ion Ratio Lower Upper
75 100
157 89.5 62.8 94.2
155 87.7 54.4 81.6#

